
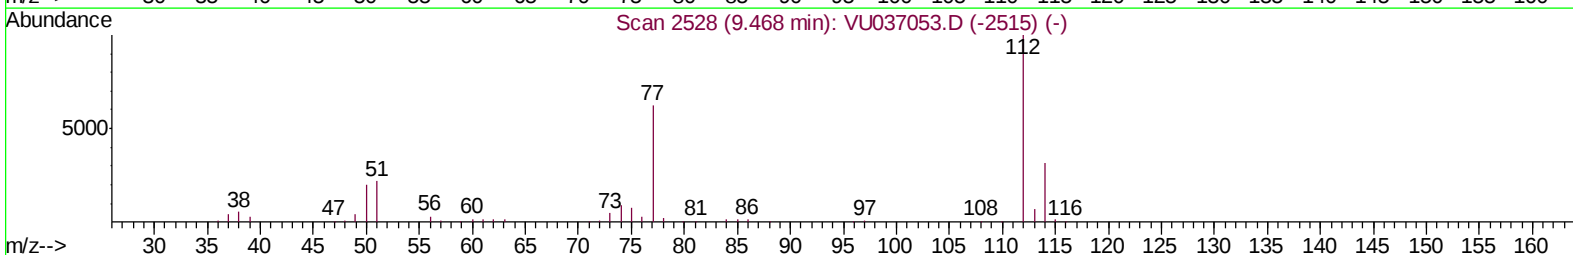
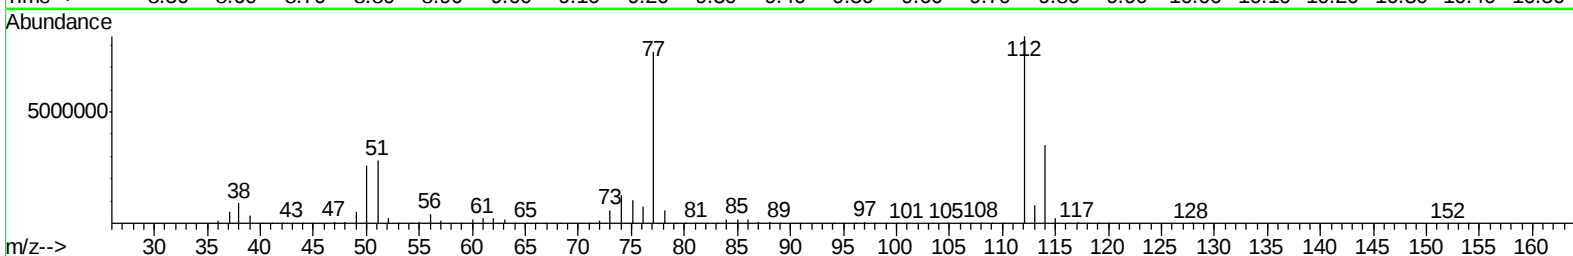


Data File : VU037057.D
Acq On : 04 Mar 2020 23:17
Operator : JC/MD
Sample : L1780-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Quant Time: Mar 05 02:57:50 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 05 02:52:45 2020
Response via : Initial Calibration

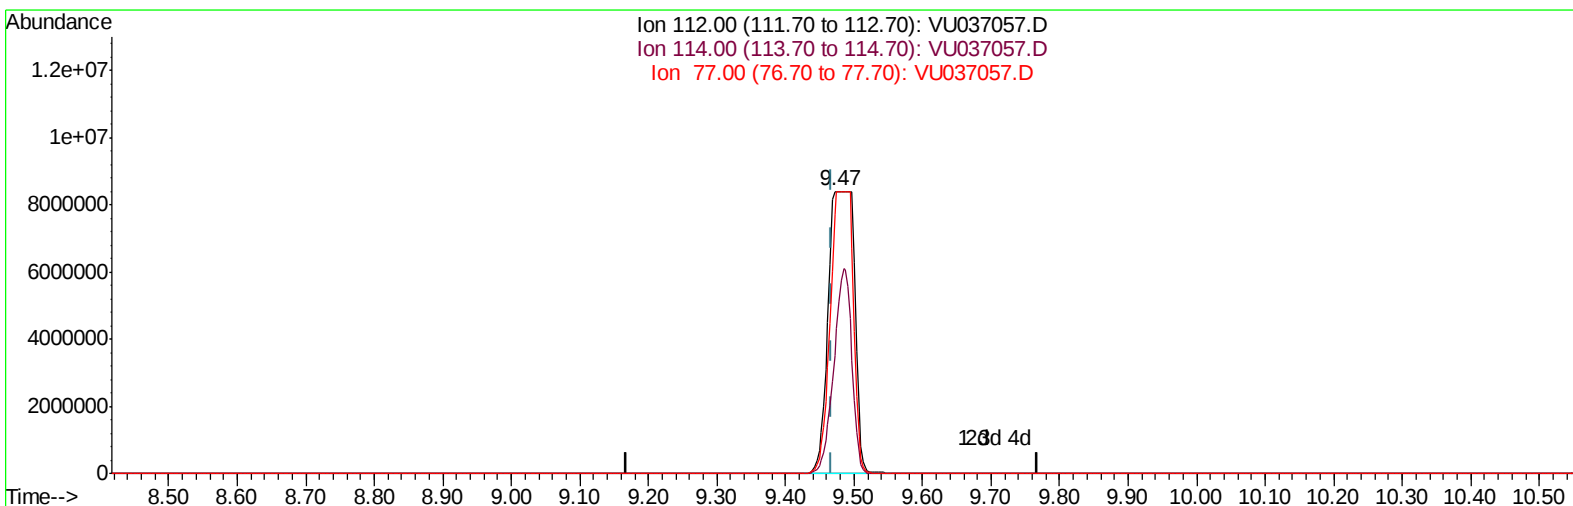

TIC: VU037057.D

(51) Chlorobenzene (T)

9.472min (+0.003) 4162.20ug/L m

response 22265080

Ion	Exp%	Act%
112.00	100	100
114.00	31.90	41.99#
77.00	62.60	91.66#
0.00	0.00	0.00