
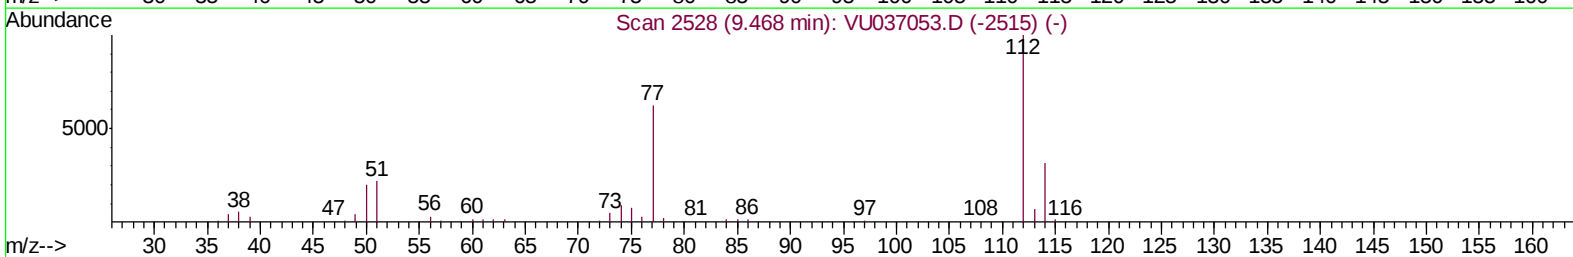
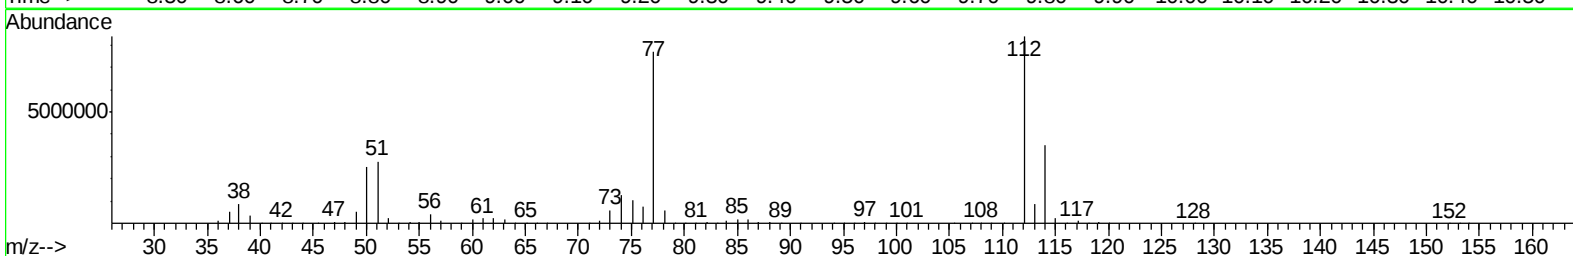


Data File : VU037061.D
Acq On : 05 Mar 2020 00:51
Operator : JC/MD
Sample : L1780-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Quant Time: Mar 05 02:58:51 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 05 02:52:45 2020
Response via : Initial Calibration

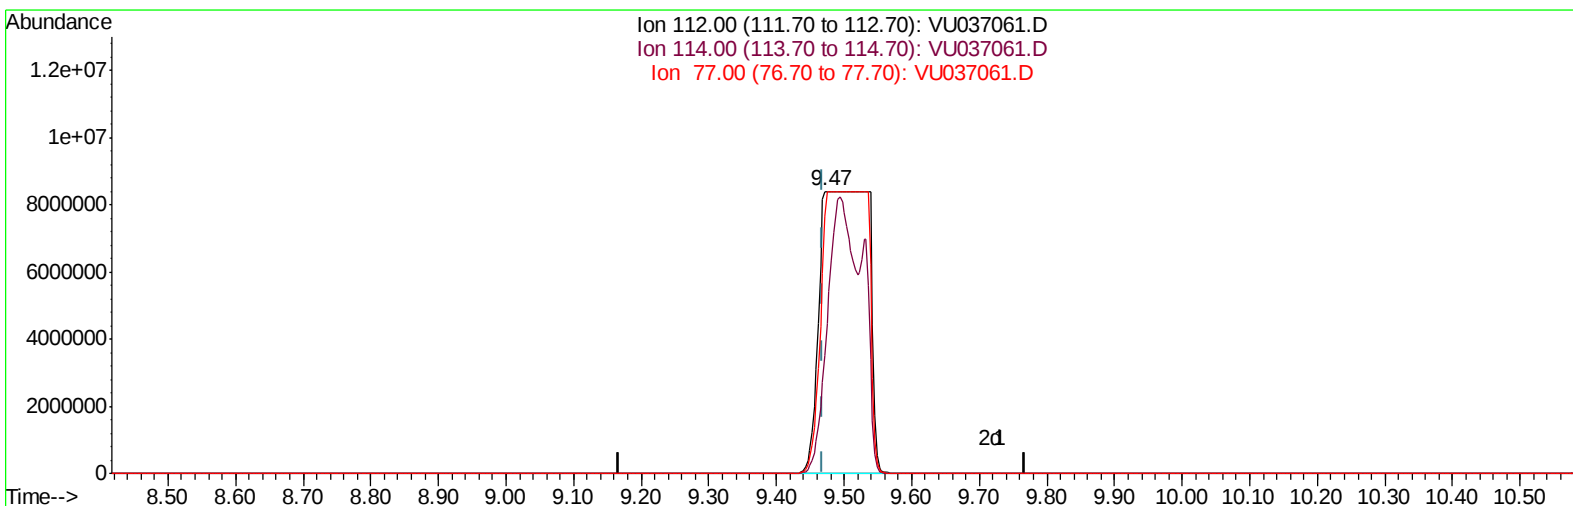

TIC: VU037061.D

(51) Chlorobenzene (T)

9.472min (+0.003) 7099.60ug/L m

response 42071457

Ion	Exp%	Act%
112.00	100	100
114.00	31.90	41.97#
77.00	62.60	91.49#
0.00	0.00	0.00