
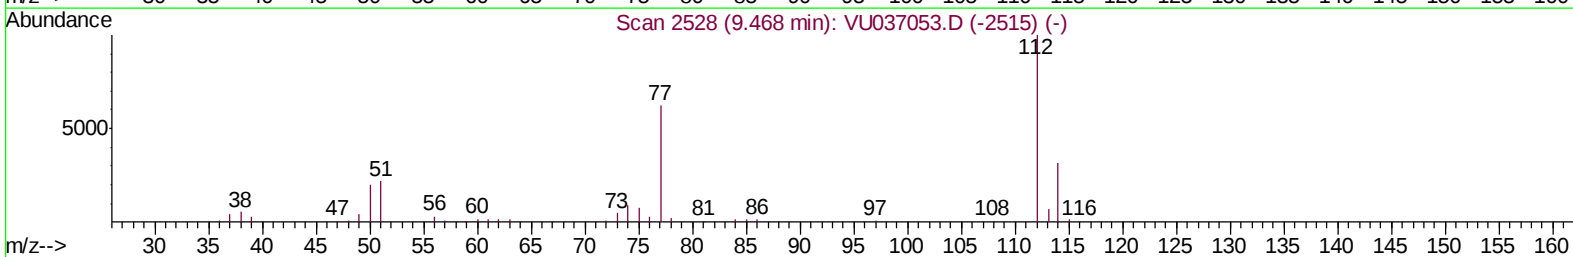
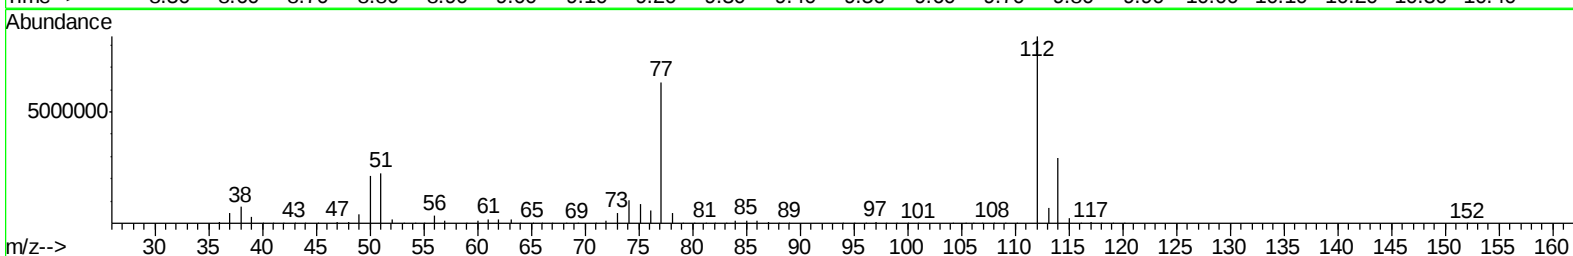


Data File : VU037064.D
Acq On : 05 Mar 2020 02:02
Operator : JC/MD
Sample : L1780-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Quant Time: Mar 05 02:59:33 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 05 02:52:45 2020
Response via : Initial Calibration

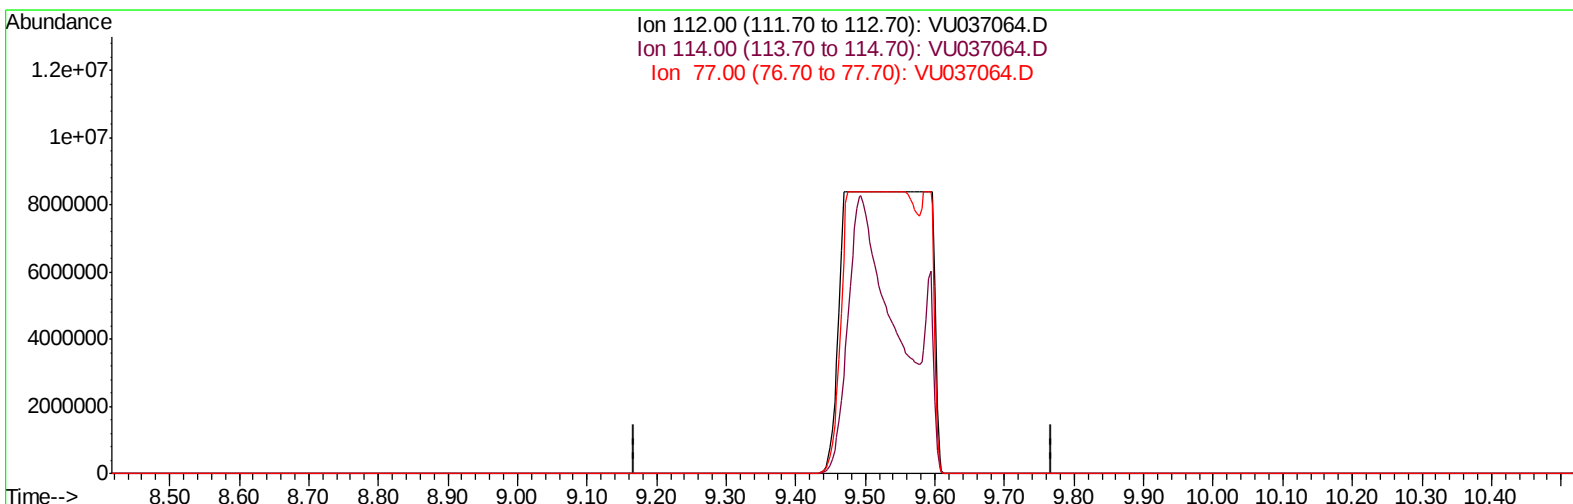

TIC: VU037064.D

(51) Chlorobenzene (T)

9.468min (-9.468) 0.00ug/L

response 0

Ion	Exp%	Act%
112.00	100	0.00
114.00	31.90	0.00#
77.00	62.60	0.00#
0.00	0.00	0.00