
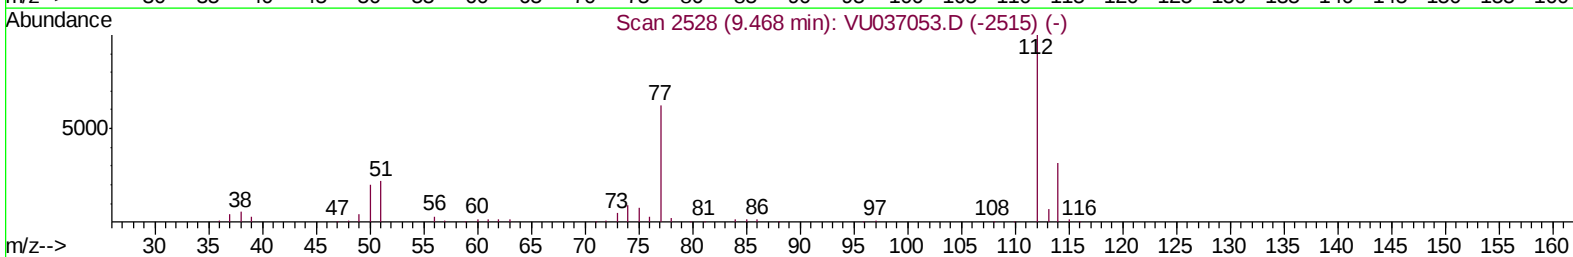
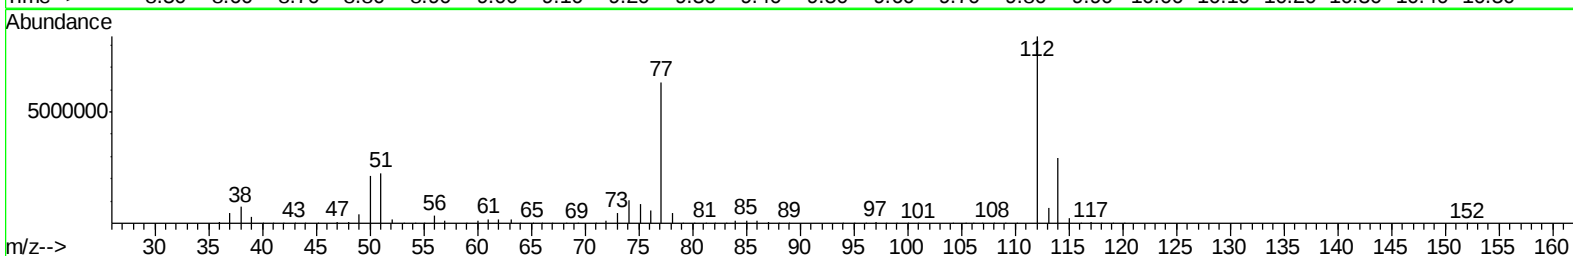


Data File : VU037064.D
Acq On : 05 Mar 2020 02:02
Operator : JC/MD
Sample : L1780-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Quant Time: Mar 05 02:59:33 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 05 02:52:45 2020
Response via : Initial Calibration

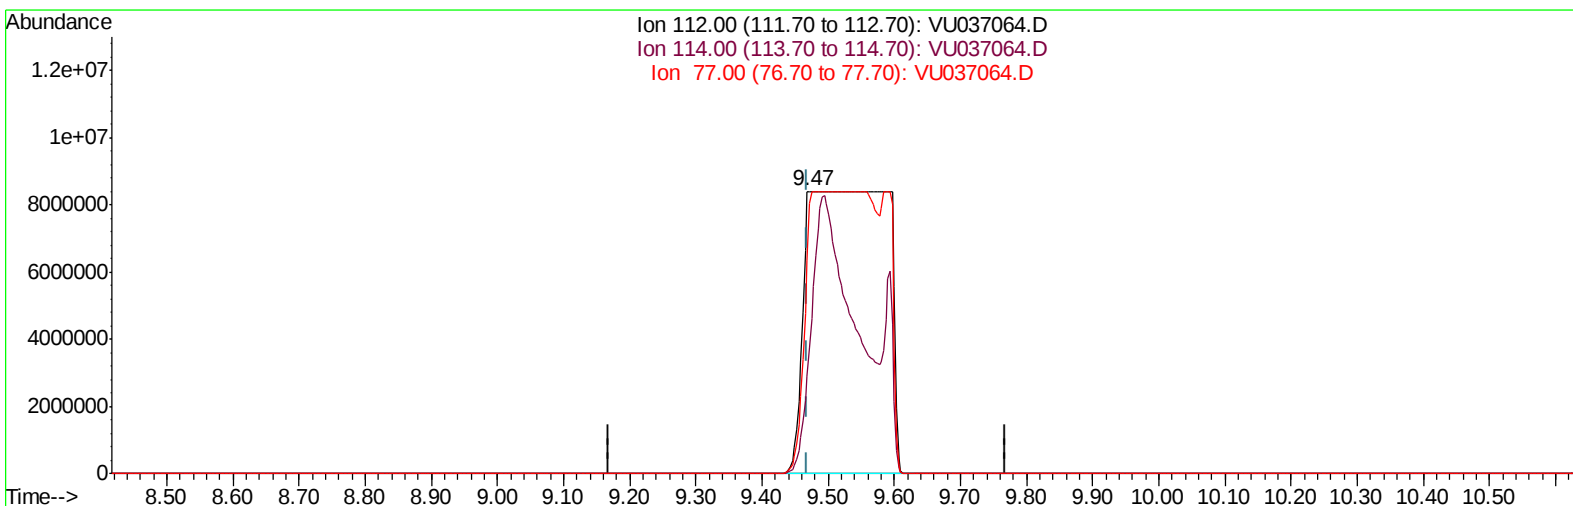

TIC: VU037064.D

(51) Chlorobenzene (T)

9.468min (+0.000) 19815.93ug/L m

response 71716560

Ion	Exp%	Act%
112.00	100	100
114.00	31.90	34.70
77.00	62.60	75.57#
0.00	0.00	0.00