


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU030420\
 Data File : VU037032.D
 Acq On : 04 Mar 2020 09:36
 Operator : JC/MD
 Sample : BFB57
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB57

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
 Title : VOC Analysis
 Last Update : Thu Mar 05 13:35:49 2020

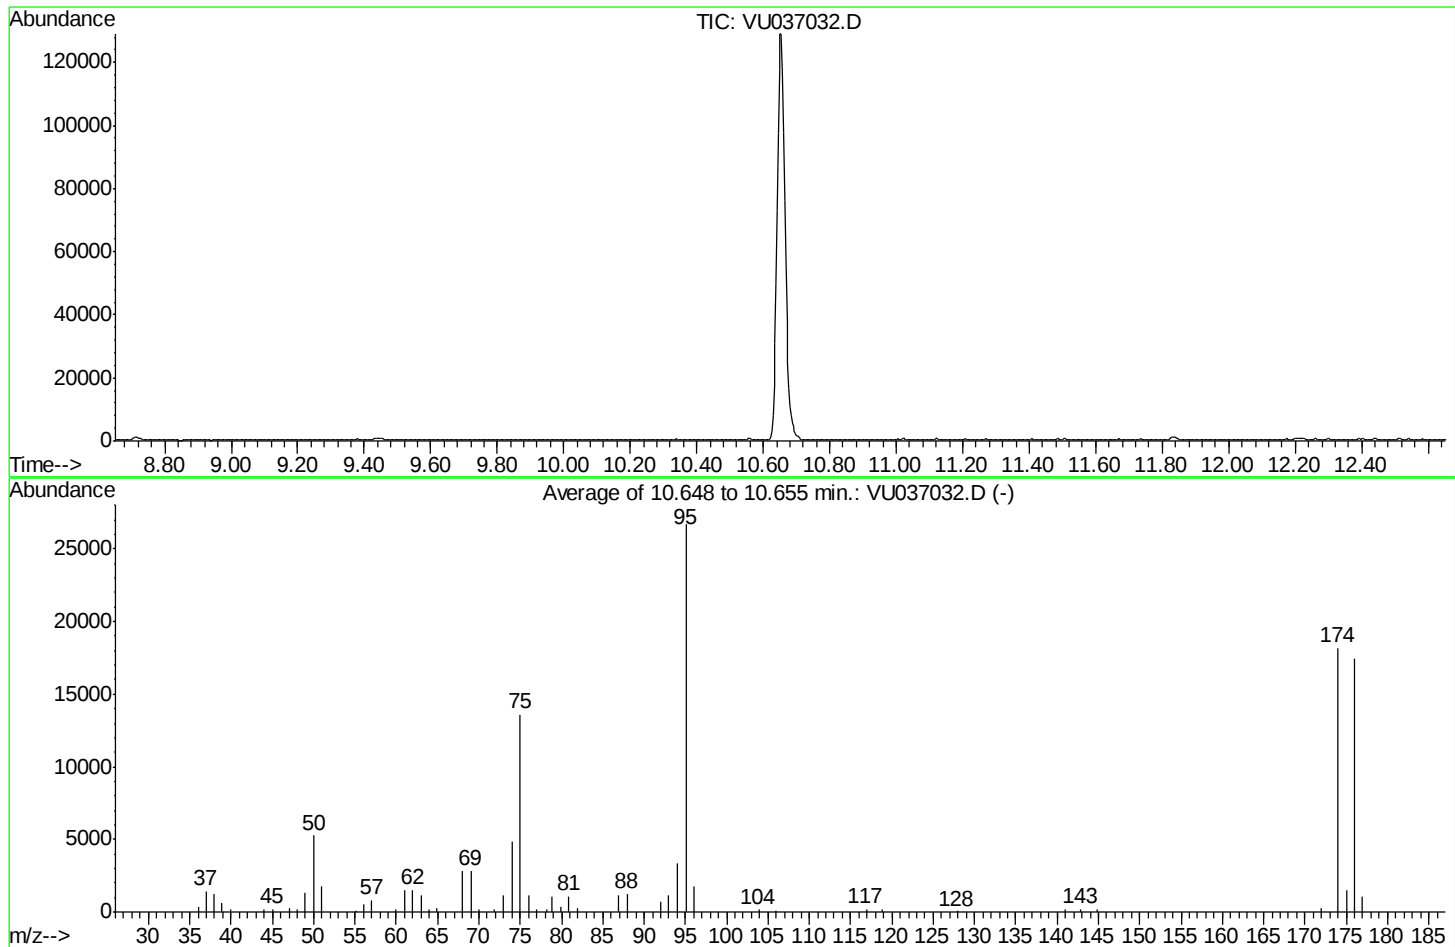

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2884

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	5274	PASS
75	95	30	80	50.9	13595	PASS
95	95	100	100	100.0	26688	PASS
96	95	5	9	6.7	1782	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	68.2	18194	PASS
175	174	5	9	8.4	1534	PASS
176	174	95	101	96.0	17465	PASS
177	176	5	9	6.1	1071	PASS

m/z	Abundance
35.90	382.0
37.00	1314.0
38.00	1241.0
38.90	618.0
39.90	126.0
44.10	423.0
45.00	187.0
47.10	272.0
48.00	179.0
49.00	1209.0
50.00	5052.0
51.00	1628.0
55.00	117.0
56.00	487.0
57.00	722.0
60.00	219.0
61.00	1534.0
62.00	1406.0
63.00	1107.0
63.90	145.0
64.90	255.0
68.00	2748.0
69.00	2738.0
70.00	180.0
71.90	169.0
73.00	1074.0
74.00	4437.0
75.00	12908.0
76.00	1174.0
77.00	155.0
78.10	160.0
78.90	944.0
80.00	277.0
80.90	940.0
81.90	302.0
87.00	938.0
87.90	1204.0
92.00	765.0
93.00	1061.0
94.00	3152.0
95.00	25168.0
96.10	1767.0
103.90	127.0
105.90	123.0
116.90	183.0
118.80	141.0
140.90	191.0
142.90	177.0
144.80	154.0
172.00	293.0
174.00	16576.0
175.00	1434.0
176.00	16117.0
177.00	1090.0

Instrument :
MSVOA_U
ClientSampleId :
BFB57

m/z	Abundance
36.00	345.0
37.00	1464.0
38.00	1275.0
38.90	655.0
39.90	151.0
44.00	427.0
45.00	223.0
47.00	240.0
48.00	205.0
49.00	1348.0
50.00	5483.0
51.00	1764.0
55.10	132.0
56.00	570.0
57.00	853.0
60.00	201.0
61.00	1526.0
62.00	1549.0
63.00	1210.0
63.90	166.0
64.90	270.0
68.00	2937.0
69.00	2907.0
70.00	199.0
71.90	157.0
73.00	1172.0
74.00	5029.0
75.00	14107.0
76.00	1199.0
77.00	189.0
78.10	161.0
78.90	1054.0
79.90	321.0
80.90	1109.0
81.90	315.0
87.00	1135.0
87.90	1286.0
92.00	752.0
93.00	1209.0
94.00	3391.0
95.00	27464.0
96.10	1822.0
103.90	170.0
105.90	141.0
116.90	200.0
118.80	150.0
127.90	118.0
141.00	193.0
142.90	193.0
144.80	156.0
172.00	316.0
174.00	18720.0
175.00	1583.0
176.00	17912.0
177.00	1094.0

Instrument :
MSVOA_U
ClientSampleId :
BFB57

m/z	Abundance
36.10	271.0
37.00	1457.0
38.00	1258.0
38.90	609.0
39.90	171.0
44.00	457.0
45.00	214.0
46.90	228.0
48.00	198.0
49.00	1403.0
50.10	5288.0
51.00	1803.0
55.10	121.0
56.00	569.0
57.00	881.0
59.90	193.0
61.00	1369.0
62.00	1553.0
63.00	1199.0
63.90	158.0
64.90	266.0
68.00	2736.0
69.00	2881.0
70.00	192.0
71.90	127.0
73.00	1251.0
74.00	5192.0
75.00	13770.0
76.00	1133.0
77.00	193.0
78.20	145.0
78.90	1095.0
79.90	397.0
80.90	1168.0
81.90	274.0
86.90	1248.0
88.00	1217.0
92.00	640.0
93.00	1281.0
94.00	3384.0
95.10	27432.0
96.00	1758.0
103.90	169.0
105.90	134.0
116.90	167.0
118.90	139.0
127.90	111.0
141.00	201.0
142.90	239.0
144.80	120.0
172.00	252.0
174.00	19288.0
175.00	1586.0
176.00	18368.0
177.00	1031.0

Instrument :
MSVOA_U
ClientSampleId :
BFB57

Scan 2884 (10.613 min): VU037032.D
BFB57

m/z	Abundance
43.90	285.0

Instrument :
MSVOA_U
ClientSampleId :
BFB57