

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030421\
 Data File : VU042479.D
 Acq On : 04 Mar 2021 13:01
 Operator : SY/MD
 Sample : M1570-15
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F1G15

Quant Time: Mar 05 00:33:19 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Mar 05 00:31:48 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.260	114	103087	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.427	117	98705	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.822	152	51263	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	30432	4.43	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	88.60%
7) Chloroethane-d5	1.919	69	23846	4.58	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.60%
11) 1,1-Dichloroethene-d2	2.575	63	49536	3.19	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.80%
20) 2-Butanone-d5	4.642	46	98574	43.69	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	87.38%
24) Chloroform-d	5.073	84	60533	4.45	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.00%
26) 1,2-Dichloroethane-d4	5.713	65	39967	4.78	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.60%
32) Benzene-d6	5.735	84	112540	4.65	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.00%
36) 1,2-Dichloropropane-d6	6.700	67	37522	4.81	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.20%
41) Toluene-d8	7.906	98	107209	4.54	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.80%
43) trans-1,3-Dichloroprop...	8.189	79	15565	4.27	ug/L	0.00
46) 2-Hexanone-d5	8.645	63	78488	44.94	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.88%
57) 1,1,2,2-Tetrachloroeth...	10.764	84	32304	4.65	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.00%
64) 1,2-Dichlorobenzene-d4	12.201	152	44117	4.75	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.00%
Target Compounds						
13) Acetone	2.655	43	6274	3.61	ug/L	Qvalue 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030421\
Data File : VU042479.D
Acq On : 04 Mar 2021 13:01
Operator : SY/MD
Sample : M1570-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F1G15


Quant Time: Mar 05 00:33:19 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Mar 05 00:31:48 2021
Response via : Initial Calibration

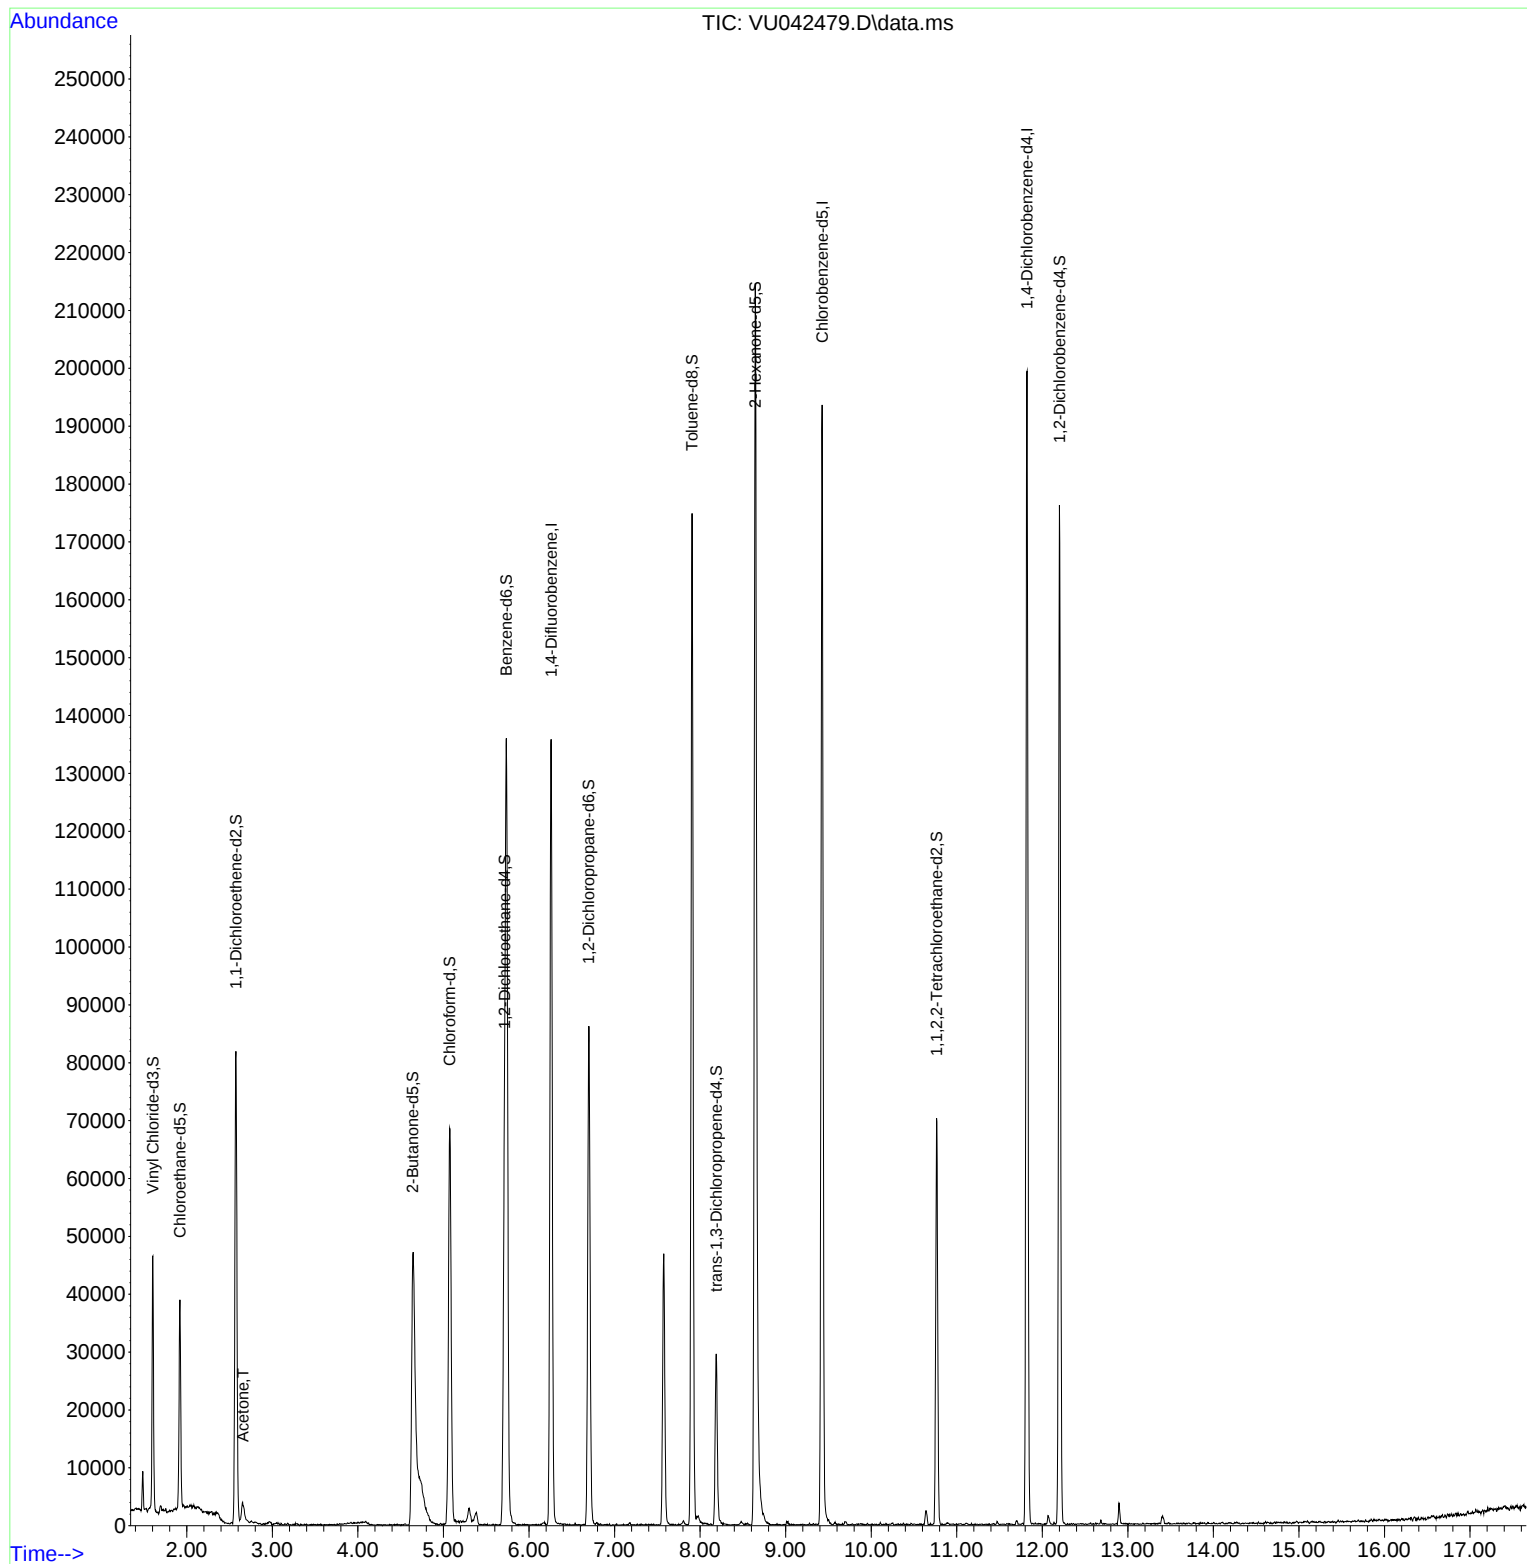

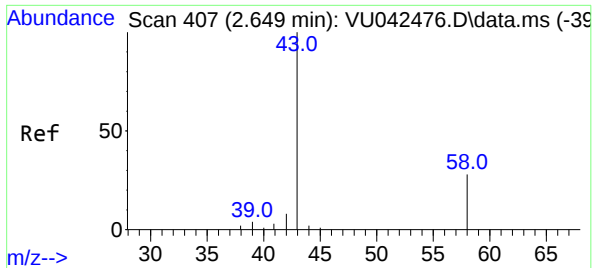

#13
Acetone
Concen: 3.61 ug/L
RT: 2.655 min Scan# 409
Delta R.T. 0.006 min
Lab File: VU042479.D
Acq: 04 Mar 2021 13:01

Instrument :
MSVOA_U
ClientSampleId :
F1G15

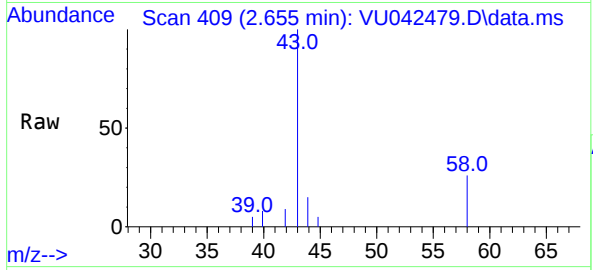

Tgt Ion: 43 Resp: 6274
Ion Ratio Lower Upper
43 100
58 22.3 0.0 55.8

