
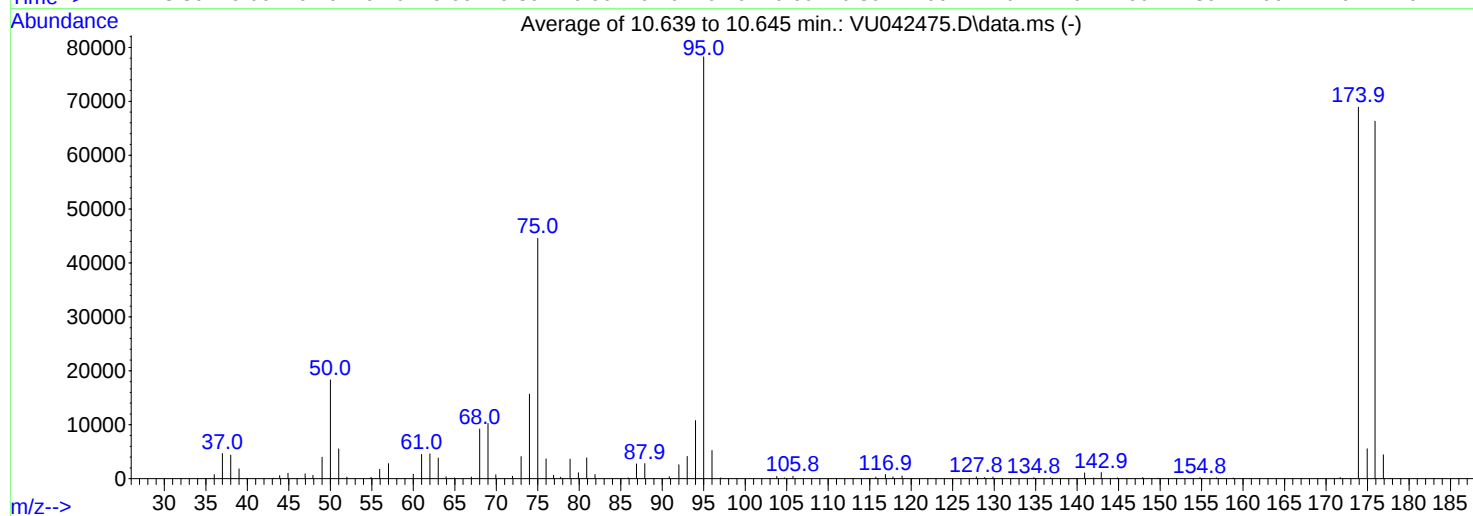


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030421\
 Data File : VU042475.D
 Acq On : 04 Mar 2021 10:09
 Operator : SY/MD
 Sample : BFB21
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB21

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Mar 05 00:31:48 2021

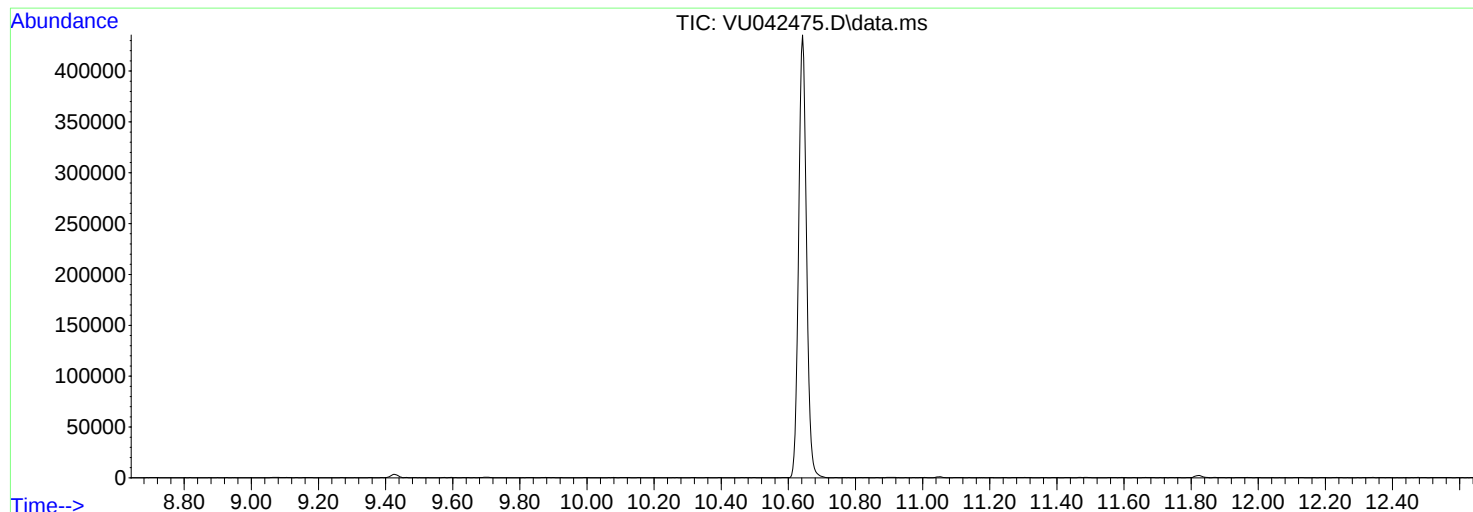

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.4	18328	PASS
75	95	30	80	57.0	44584	PASS
95	95	100	100	100.0	78245	PASS
96	95	5	9	6.7	5214	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	88.0	68893	PASS
175	174	5	9	8.0	5544	PASS
176	174	95	101	96.3	66320	PASS
177	176	5	9	6.7	4412	PASS

m/z	Abundance
36.00	787.0
37.00	4570.0
38.00	4458.0
39.00	1789.0
39.90	176.0
43.20	104.0
43.90	796.0
44.90	1029.0
46.90	859.0
47.90	694.0
49.00	3957.0
50.00	18560.0
51.00	5511.0
52.00	266.0
54.90	280.0
55.90	1788.0
57.00	2803.0
60.00	844.0
61.00	4465.0
62.00	4813.0
63.00	3700.0
64.00	416.0
64.90	201.0
67.00	288.0
68.00	9317.0
69.00	10101.0
69.90	725.0
72.00	437.0
73.00	4237.0
74.00	16084.0
75.00	44592.0
76.00	3771.0
76.90	588.0
77.70	256.0
78.90	3825.0
79.90	1079.0
80.90	3972.0
81.90	714.0
85.90	132.0
86.90	2768.0
87.90	2827.0
90.90	351.0
92.00	2707.0
93.00	4048.0
94.00	10849.0
95.00	78304.0
96.00	5444.0
97.00	129.0
103.80	447.0
104.80	163.0
105.70	477.0
115.70	352.0
116.90	698.0
117.80	371.0
118.90	528.0
127.80	385.0
128.90	231.0
129.80	317.0
134.80	188.0
136.80	151.0
140.90	1051.0
142.10	145.0
142.90	1073.0
144.90	170.0
147.90	178.0
149.70	105.0
154.80	192.0
156.80	144.0
158.80	128.0
160.80	111.0
173.90	65784.0
174.90	5495.0
175.90	63696.0
176.90	4326.0
177.80	115.0

Instrument :
MSVOA_U
ClientSampleId :
BFB21

m/z	Abundance
36.00	734.0
37.00	4809.0
38.00	4451.0
39.00	1875.0
39.90	202.0
43.10	108.0
43.90	832.0
44.90	1046.0
46.90	923.0
47.90	641.0
49.00	4110.0
50.00	18952.0
51.00	5718.0
52.00	314.0
54.90	251.0
56.00	1752.0
57.00	2892.0
60.00	856.0
61.00	4671.0
62.00	4761.0
63.00	4001.0
63.90	383.0
64.90	150.0
67.00	321.0
68.00	9474.0
69.00	10606.0
70.00	755.0
72.00	426.0
73.00	4237.0
74.00	16110.0
75.00	46040.0
76.00	3791.0
76.90	674.0
77.70	276.0
78.90	3743.0
79.90	1089.0
80.90	4044.0
81.90	797.0
85.90	157.0
86.90	2862.0
87.90	2940.0
90.90	349.0
92.00	2631.0
93.00	4283.0
94.00	11151.0
95.00	80664.0
96.00	5359.0
97.10	149.0
103.80	431.0
104.80	137.0
105.70	482.0
112.00	103.0
114.80	111.0
115.70	306.0
116.90	812.0
117.80	331.0
118.90	529.0
127.80	353.0
128.90	209.0
129.90	358.0
130.90	109.0
134.80	225.0
136.80	168.0
140.90	1126.0
142.00	141.0
142.90	1158.0
144.80	152.0
147.90	204.0
149.80	102.0
154.80	225.0
156.80	161.0
158.80	136.0
171.70	304.0
173.90	70872.0
174.90	5711.0
175.90	68416.0
176.90	4566.0
177.80	103.0

Instrument :
MSVOA_U
ClientSampleId :
BFB21

m/z	Abundance
36.00	674.0
37.00	4627.0
38.00	4166.0
39.00	1787.0
39.90	166.0
43.10	101.0
43.90	823.0
44.90	918.0
46.10	120.0
47.00	879.0
47.90	525.0
49.00	3873.0
50.00	17472.0
51.00	5297.0
52.00	291.0
54.90	214.0
56.00	1624.0
57.00	2699.0
60.00	801.0
61.00	4441.0
62.00	4251.0
63.00	3802.0
63.90	292.0
65.00	121.0
67.00	261.0
68.00	8825.0
69.00	9985.0
69.90	712.0
71.90	446.0
73.00	3853.0
74.00	14852.0
75.00	43120.0
76.00	3530.0
76.90	629.0
77.80	276.0
78.90	3295.0
79.90	1100.0
80.90	3600.0
81.90	801.0
83.00	109.0
85.90	141.0
86.90	2604.0
87.90	2630.0
90.80	356.0
92.00	2436.0
93.00	4028.0
94.00	10293.0
95.00	75768.0
96.00	4839.0
97.10	163.0
103.80	374.0
104.70	117.0
105.80	422.0
115.80	264.0
116.90	796.0
117.80	278.0
118.90	502.0
127.90	292.0
128.80	169.0
129.80	320.0
130.90	112.0
134.80	210.0
136.80	169.0
140.90	1075.0
141.90	156.0
142.90	1119.0
144.80	108.0
147.90	231.0
149.80	100.0
154.80	245.0
156.80	168.0
158.80	112.0
171.70	320.0
173.90	70024.0
175.00	5425.0
175.90	66848.0
176.90	4345.0

Instrument :
MSVOA_U
ClientSampleId :
BFB21

Scan 2879 (10.597 min): VU042475.D\data.ms
BFB21

m/z	Abundance
39.90	116.0
43.90	248.0

Instrument :
MSVOA_U
ClientSampleId :
BFB21