


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030519\
Data File : VU029807.D
Acq On : 05 Mar 2019 08:24
Operator : JC/SP
Sample : BFB55
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB55

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM021519WMA.M
Title : VOC Analysis
Last Update : Wed Mar 06 00:41:37 2019

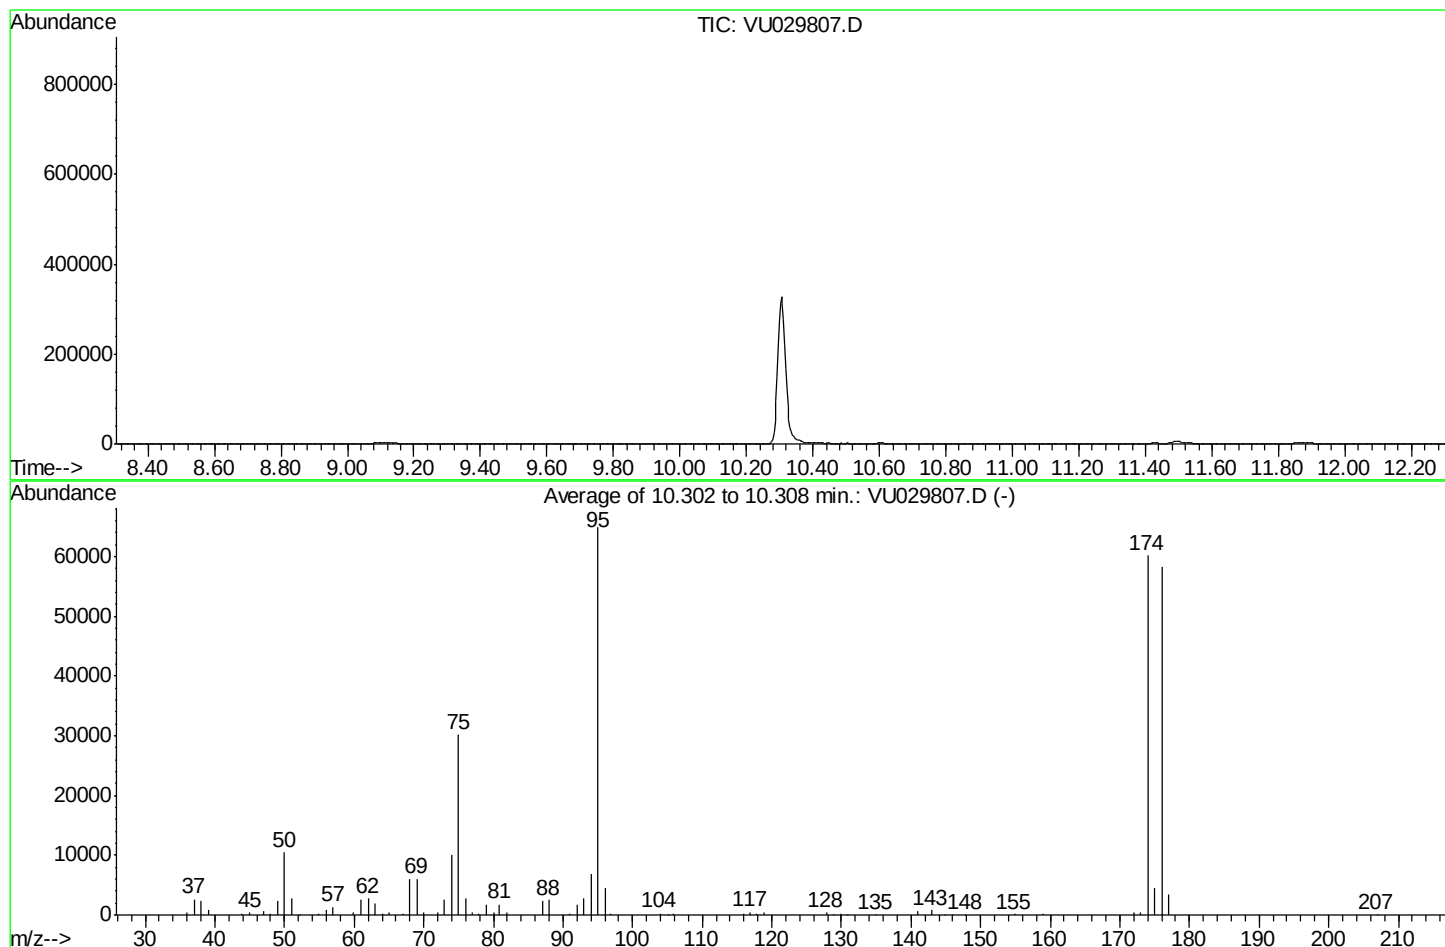

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2854

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	10450	PASS
75	95	30	80	46.4	30152	PASS
95	95	100	100	100.0	64920	PASS
96	95	5	9	7.0	4541	PASS
173	174	0.00	2	0.9	520	PASS
174	95	50	120	92.8	60216	PASS
175	174	5	9	7.5	4488	PASS
176	174	95	101	96.7	58224	PASS
177	176	5	9	6.0	3506	PASS

m/z	Abundance
35.90	422.0
37.00	2867.0
38.00	2316.0
39.00	917.0
39.90	456.0
43.90	634.0
45.10	404.0
47.00	562.0
48.00	277.0
49.00	2397.0
50.00	10467.0
51.00	2937.0
52.00	171.0
54.90	128.0
56.00	957.0
57.00	1376.0
60.00	511.0
61.00	2567.0
62.00	2714.0
63.10	1927.0
64.00	309.0
64.90	299.0
67.00	164.0
68.00	6082.0
69.00	6062.0
70.00	458.0
72.00	338.0
73.00	2509.0
74.00	9907.0
75.00	30136.0
76.00	2662.0
76.90	366.0
78.00	304.0
78.90	1736.0
80.00	539.0
80.90	1692.0
82.00	314.0
87.00	2518.0
87.90	2518.0
90.90	261.0
92.00	1713.0
93.00	2806.0
94.00	6884.0
95.00	64008.0
96.00	4434.0
96.90	199.0
103.90	309.0
105.90	169.0
116.00	214.0
117.00	429.0
117.80	165.0
118.90	367.0
127.90	358.0
129.90	196.0
135.00	100.0
140.90	681.0
142.90	878.0
145.00	101.0
146.00	101.0
147.80	105.0
154.90	151.0
158.90	111.0
172.00	495.0
172.90	483.0
174.00	58864.0
175.00	4341.0
176.00	56304.0
177.00	3476.0
207.00	138.0

Instrument :
MSVOA_U
ClientSampleId :
BFB55

m/z	Abundance
35.90	440.0
37.00	2723.0
38.00	2332.0
39.00	880.0
39.90	479.0
43.90	573.0
45.00	425.0
47.00	563.0
48.00	264.0
49.00	2473.0
50.00	10888.0
51.00	2945.0
52.10	135.0
54.90	142.0
56.00	951.0
57.00	1375.0
60.00	494.0
61.00	2555.0
62.00	2824.0
63.00	1998.0
64.00	269.0
65.00	343.0
67.00	170.0
68.00	6120.0
69.00	6385.0
70.00	495.0
72.00	356.0
73.00	2718.0
74.00	10423.0
75.00	30928.0
76.00	2753.0
76.90	355.0
78.00	320.0
78.90	1869.0
80.00	534.0
80.90	1832.0
82.00	338.0
87.00	2477.0
88.00	2616.0
90.90	276.0
92.00	1873.0
93.00	2895.0
94.00	7041.0
95.00	66728.0
96.00	4741.0
96.90	219.0
103.90	301.0
105.10	128.0
105.90	204.0
116.00	191.0
116.90	454.0
117.80	170.0
119.00	345.0
127.90	365.0
129.80	213.0
130.90	129.0
141.00	669.0
143.00	862.0
144.80	102.0
154.90	193.0
158.90	168.0
172.00	537.0
173.00	542.0
174.00	61960.0
175.00	4609.0
176.00	59800.0
177.00	3602.0
206.90	148.0

Instrument :
MSVOA_U
ClientSampleId :
BFB55

m/z	Abundance
35.90	403.0
37.00	2345.0
38.00	2208.0
39.00	836.0
39.90	484.0
43.90	555.0
45.00	447.0
46.90	589.0
47.90	322.0
49.00	2303.0
50.00	9995.0
51.00	2785.0
54.90	143.0
56.00	882.0
57.00	1334.0
59.90	467.0
61.00	2374.0
62.00	2685.0
63.00	1837.0
64.00	226.0
65.10	380.0
66.90	150.0
68.00	5673.0
69.00	5843.0
70.00	450.0
72.00	322.0
73.00	2674.0
74.00	9946.0
75.00	29392.0
76.00	2691.0
77.00	392.0
77.90	358.0
78.90	1829.0
80.00	431.0
80.90	1791.0
82.00	363.0
87.00	2268.0
88.00	2562.0
90.90	225.0
92.00	1785.0
93.00	2629.0
94.00	6699.0
95.00	64024.0
96.00	4448.0
96.90	174.0
104.00	287.0
105.00	147.0
105.90	239.0
115.90	189.0
116.90	452.0
117.80	163.0
119.00	331.0
127.90	293.0
128.90	121.0
129.80	199.0
130.90	160.0
134.80	100.0
141.00	566.0
143.00	794.0
154.90	197.0
158.90	189.0
172.00	518.0
173.00	537.0
174.00	59824.0
175.00	4514.0
176.00	58568.0
177.00	3440.0
206.90	165.0

Instrument :
MSVOA_U
ClientSampleId :
BFB55

Scan 2854 (10.267 min): VU029807.D
BFB55

m/z	Abundance
39.90	487.0
43.90	387.0
206.90	129.0

Instrument :
MSVOA_U
ClientSampleId :
BFB55