

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU030520\
 Data File : VU037091.D
 Acq On : 05 Mar 2020 18:26
 Operator : JC/MD
 Sample : L1780-05DL 400X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DF9DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.613	78	85	99	rBV	118476	125441	11.96%	1.484%
2	1.929	175	183	196	rVB	113508	145205	13.84%	1.718%
3	2.533	368	371	375	rBV2	283	202	0.02%	0.002%
4	2.591	377	389	406	rVV	181217	297610	28.37%	3.522%
5	2.790	444	451	456	rBV3	963	1108	0.11%	0.013%
6	2.977	506	509	512	rVB	290	196	0.02%	0.002%
7	3.073	534	539	548	rVB4	1135	1678	0.16%	0.020%
8	3.221	571	585	599	rVV	12456	27730	2.64%	0.328%
9	3.295	604	608	616	rVB2	235	391	0.04%	0.005%
10	3.456	649	658	660	rBV2	216	313	0.03%	0.004%
11	3.572	690	694	699	rBV	262	253	0.02%	0.003%
12	3.626	707	711	715	rBV2	242	253	0.02%	0.003%
13	3.883	788	791	796	rVB	267	214	0.02%	0.003%
14	4.176	876	882	887	rVB2	197	251	0.02%	0.003%
15	4.321	916	927	934	rVB2	233	453	0.04%	0.005%
16	4.427	955	960	962	rBV2	238	213	0.02%	0.003%
17	4.671	1019	1036	1069	rBV	110388	269825	25.72%	3.193%
18	4.829	1083	1085	1089	rVB2	585	439	0.04%	0.005%
19	4.851	1090	1092	1095	rBV3	397	221	0.02%	0.003%
20	5.044	1148	1152	1154	rBV2	368	232	0.02%	0.003%
21	5.105	1154	1171	1194	rVV	173976	386902	36.88%	4.578%
22	5.311	1230	1235	1237	rVV2	364	296	0.03%	0.004%
23	5.327	1237	1240	1248	rVB4	747	1052	0.10%	0.012%
24	5.375	1248	1255	1259	rBV2	224	251	0.02%	0.003%
25	5.420	1264	1269	1270	rBV2	342	262	0.02%	0.003%
26	5.581	1315	1319	1322	rBV2	248	237	0.02%	0.003%
27	5.629	1331	1334	1339	rVB2	361	275	0.03%	0.003%
28	5.761	1353	1375	1386	rBV2	384288	1019911	97.22%	12.068%
29	6.073	1470	1472	1478	rBV3	367	369	0.04%	0.004%
30	6.144	1490	1494	1496	rBV	383	287	0.03%	0.003%
31	6.282	1522	1537	1556	rBV	336769	628841	59.94%	7.441%
32	6.565	1616	1625	1636	rVB9	2396	4317	0.41%	0.051%
33	6.723	1660	1674	1693	rBV	240974	462752	44.11%	5.476%
34	6.832	1704	1708	1709	rBV2	633	468	0.04%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU030520\
 Data File : VU037091.D
 Acq On : 05 Mar 2020 18:26
 Operator : JC/MD
 Sample : L1780-05DL 400X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DF9DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
 Title : VOC Analysis

35	6.867	1715	1719	1722	rBV3	352	247	0.02%	0.003%
36	7.015	1760	1765	1769	rBV2	162	209	0.02%	0.002%
37	7.076	1779	1784	1789	rBV2	234	262	0.02%	0.003%
38	7.205	1818	1824	1838	rBV2	2567	4022	0.38%	0.048%
39	7.308	1845	1856	1863	rVB2	349	754	0.07%	0.009%
40	7.349	1863	1869	1871	rBV	255	259	0.02%	0.003%
41	7.433	1888	1895	1897	rBV2	247	296	0.03%	0.004%
42	7.494	1911	1914	1918	rBV2	240	249	0.02%	0.003%
43	7.533	1920	1926	1929	rBV	239	267	0.03%	0.003%
44	7.594	1932	1945	1964	rBV	121872	212332	20.24%	2.512%
45	7.710	1973	1981	1986	rBV4	1642	2147	0.20%	0.025%
46	7.771	1998	2000	2005	rVB	629	363	0.03%	0.004%
47	7.819	2010	2015	2016	rBV	455	368	0.04%	0.004%
48	7.925	2033	2048	2066	rBV	444659	766058	73.02%	9.065%
49	8.205	2122	2135	2151	rVV	82862	142585	13.59%	1.687%
50	8.275	2155	2157	2161	rVB3	439	291	0.03%	0.003%
51	8.420	2197	2202	2207	rBV	233	236	0.02%	0.003%
52	8.446	2207	2210	2216	rVB2	204	194	0.02%	0.002%
53	8.658	2264	2276	2302	rBV	277211	532349	50.74%	6.299%
54	8.973	2364	2374	2378	rBV3	1032	1764	0.17%	0.021%
55	9.311	2476	2479	2484	rVB2	276	308	0.03%	0.004%
56	9.346	2484	2490	2492	rBV	257	268	0.03%	0.003%
57	9.439	2503	2519	2559	rBV2	463205	1049110	100.00%	12.414%
58	9.710	2599	2603	2606	rBV2	237	260	0.02%	0.003%
59	9.919	2663	2668	2675	rBV2	298	350	0.03%	0.004%
60	9.957	2675	2680	2683	rBV2	235	267	0.03%	0.003%
61	10.070	2710	2715	2721	rVB2	329	504	0.05%	0.006%
62	10.140	2734	2737	2743	rVV2	322	260	0.02%	0.003%
63	10.189	2747	2752	2755	rBV2	219	214	0.02%	0.003%
64	10.639	2887	2892	2896	rBV	332	417	0.04%	0.005%
65	10.774	2922	2934	2953	rVB	310205	508088	48.43%	6.012%
66	11.298	3092	3097	3100	rBV2	277	324	0.03%	0.004%
67	11.394	3123	3127	3129	rBV	210	201	0.02%	0.002%
68	11.436	3137	3140	3143	rBV	276	237	0.02%	0.003%
69	11.600	3187	3191	3194	rBV	328	288	0.03%	0.003%
70	11.671	3206	3213	3216	rBV2	226	331	0.03%	0.004%
71	11.764	3229	3242	3250	rBV	23763	38052	3.63%	0.450%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU030520\
 Data File : VU037091.D
 Acq On : 05 Mar 2020 18:26
 Operator : JC/MD
 Sample : L1780-05DL 400X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DF9DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
 Title : VOC Analysis

72	11.828	3250	3262	3285	rVB3	388946	859436	81.92%	10.170%
73	12.211	3368	3381	3400	rBV3	418578	906983	86.45%	10.732%
74	12.314	3409	3413	3418	rBV2	374	326	0.03%	0.004%
75	12.449	3451	3455	3459	rBV2	290	279	0.03%	0.003%
76	12.475	3460	3463	3468	rVB2	292	222	0.02%	0.003%
77	12.902	3591	3596	3599	rBV2	308	342	0.03%	0.004%
78	13.028	3631	3635	3641	rBV2	269	313	0.03%	0.004%
79	13.240	3696	3701	3703	rBV3	590	477	0.05%	0.006%
80	13.333	3727	3730	3736	rBV	298	282	0.03%	0.003%
81	13.433	3756	3761	3768	rBV2	300	439	0.04%	0.005%
82	13.500	3774	3782	3787	rVB2	252	354	0.03%	0.004%
83	13.639	3821	3825	3829	rBV	272	290	0.03%	0.003%
84	13.716	3844	3849	3854	rBV2	397	458	0.04%	0.005%
85	13.870	3887	3897	3906	rBV3	17200	25497	2.43%	0.302%
86	13.963	3923	3926	3930	rVB3	312	201	0.02%	0.002%
87	13.983	3930	3932	3936	rBV	278	213	0.02%	0.003%
88	14.111	3970	3972	3975	rBV3	328	192	0.02%	0.002%
89	14.160	3984	3987	3990	rBV2	333	208	0.02%	0.002%
90	14.362	4041	4050	4061	rVB5	5660	8283	0.79%	0.098%
91	14.446	4073	4076	4079	rBV	315	210	0.02%	0.002%
92	14.516	4095	4098	4104	rBV2	206	198	0.02%	0.002%
93	14.658	4139	4142	4146	rVB	373	265	0.03%	0.003%
94	14.848	4198	4201	4204	rBV2	340	203	0.02%	0.002%
95	14.886	4210	4213	4217	rBV2	301	241	0.02%	0.003%
96	15.034	4253	4259	4265	rBV2	500	674	0.06%	0.008%
97	15.063	4265	4268	4272	rVV2	436	359	0.03%	0.004%
98	15.330	4348	4351	4354	rBV	504	307	0.03%	0.004%
99	15.677	4455	4459	4461	rBV	462	415	0.04%	0.005%
100	16.114	4593	4595	4596	rBV	457	198	0.02%	0.002%


Sum of corrected areas: 8451044

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU030520\
Data File : VU037091.D
Acq On : 05 Mar 2020 18:26
Operator : JC/MD
Sample : L1780-05DL 400X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
C0DF9DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

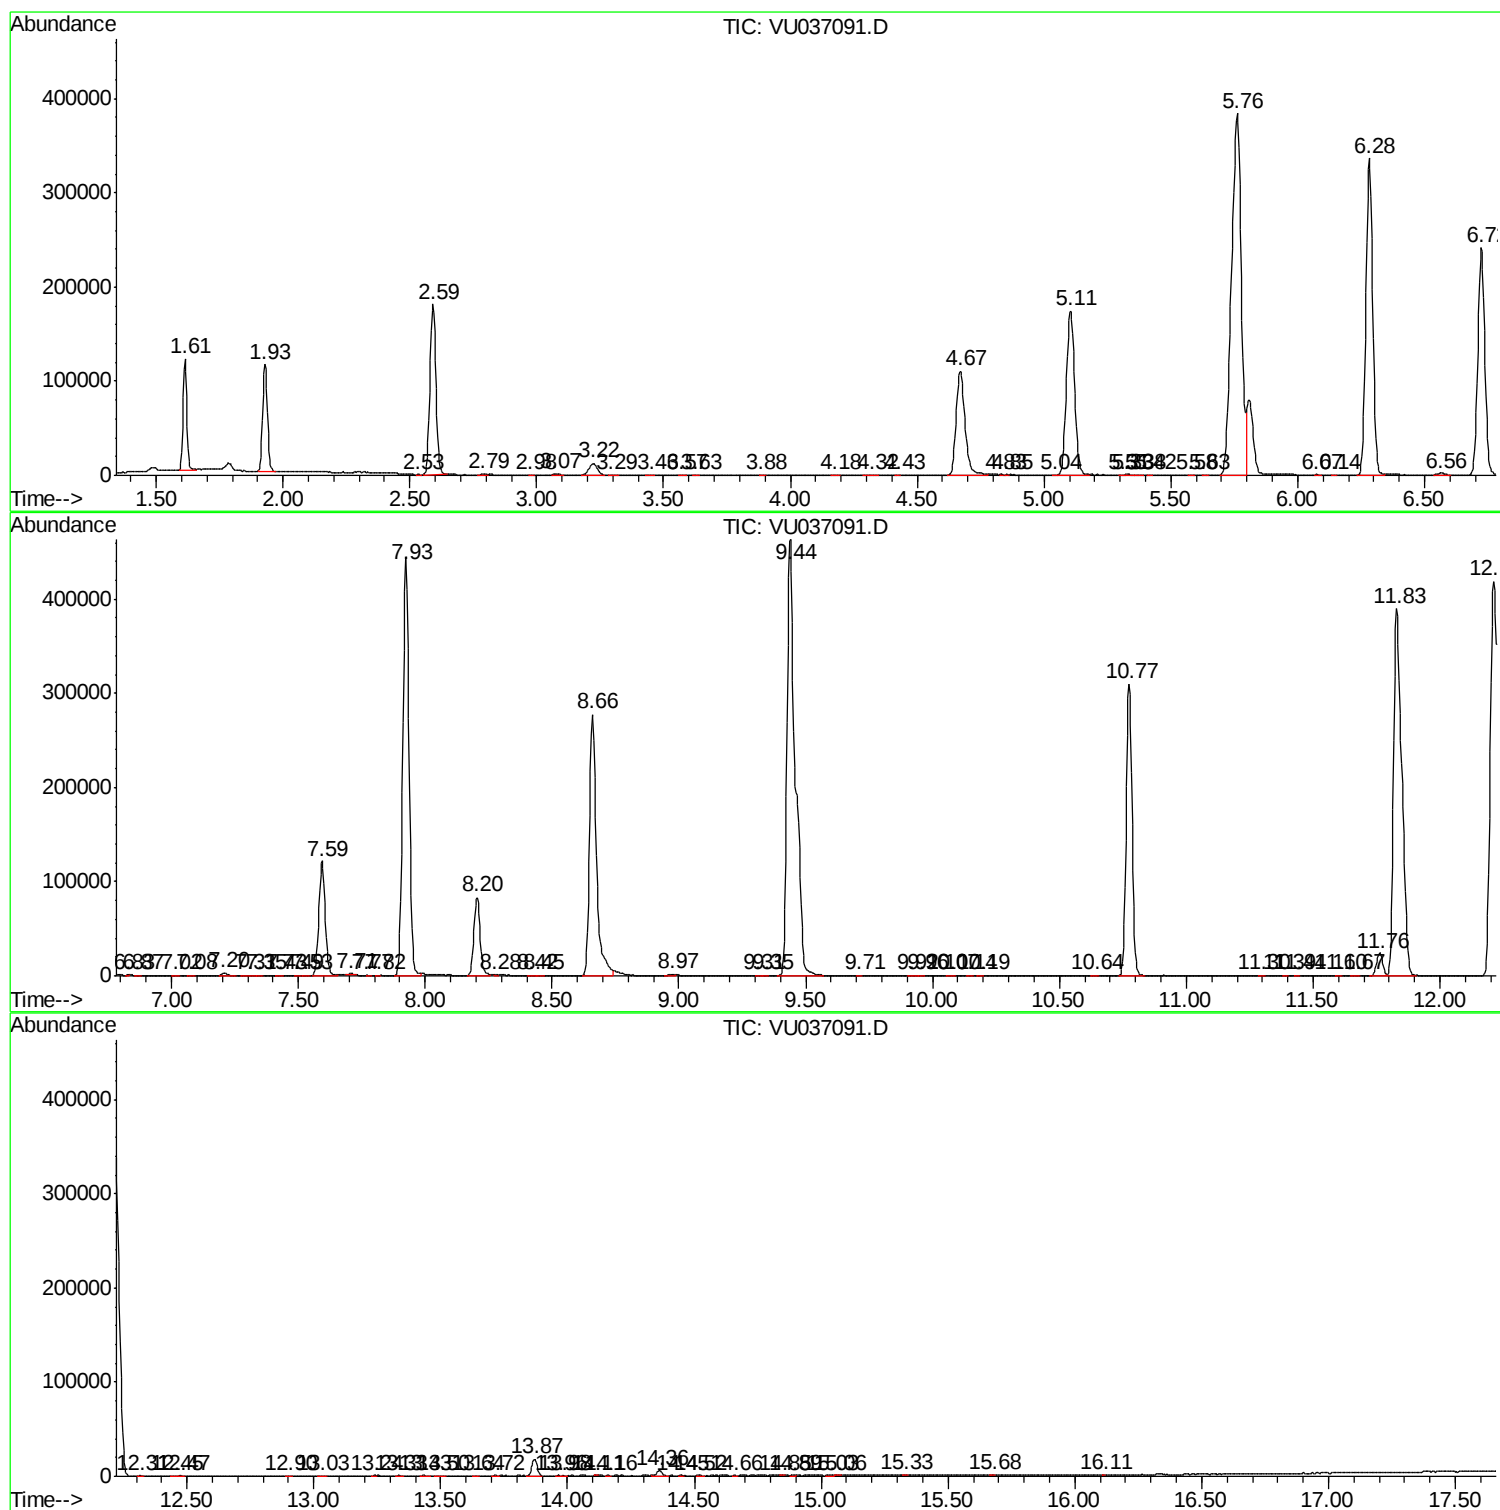

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU030520\
Data File : VU037091.D
Acq On : 05 Mar 2020 18:26
Operator : JC/MD
Sample : L1780-05DL 400X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DF9DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_U\DATA\VU030520\
Data File : VU037091.D
Acq On : 05 Mar 2020 18:26
Operator : JC/MD
Sample : L1780-05DL 400X
Misc : 5.0mL/MSV0A_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSV0A_U
ClientSampleId :
C0DF9DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_U\METHOD\SOMULM022420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc