


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU030520\
 Data File : VU037071.D
 Acq On : 05 Mar 2020 09:29
 Operator : JC/MD
 Sample : BFB58
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB58

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
 Title : VOC Analysis
 Last Update : Fri Mar 06 23:54:55 2020

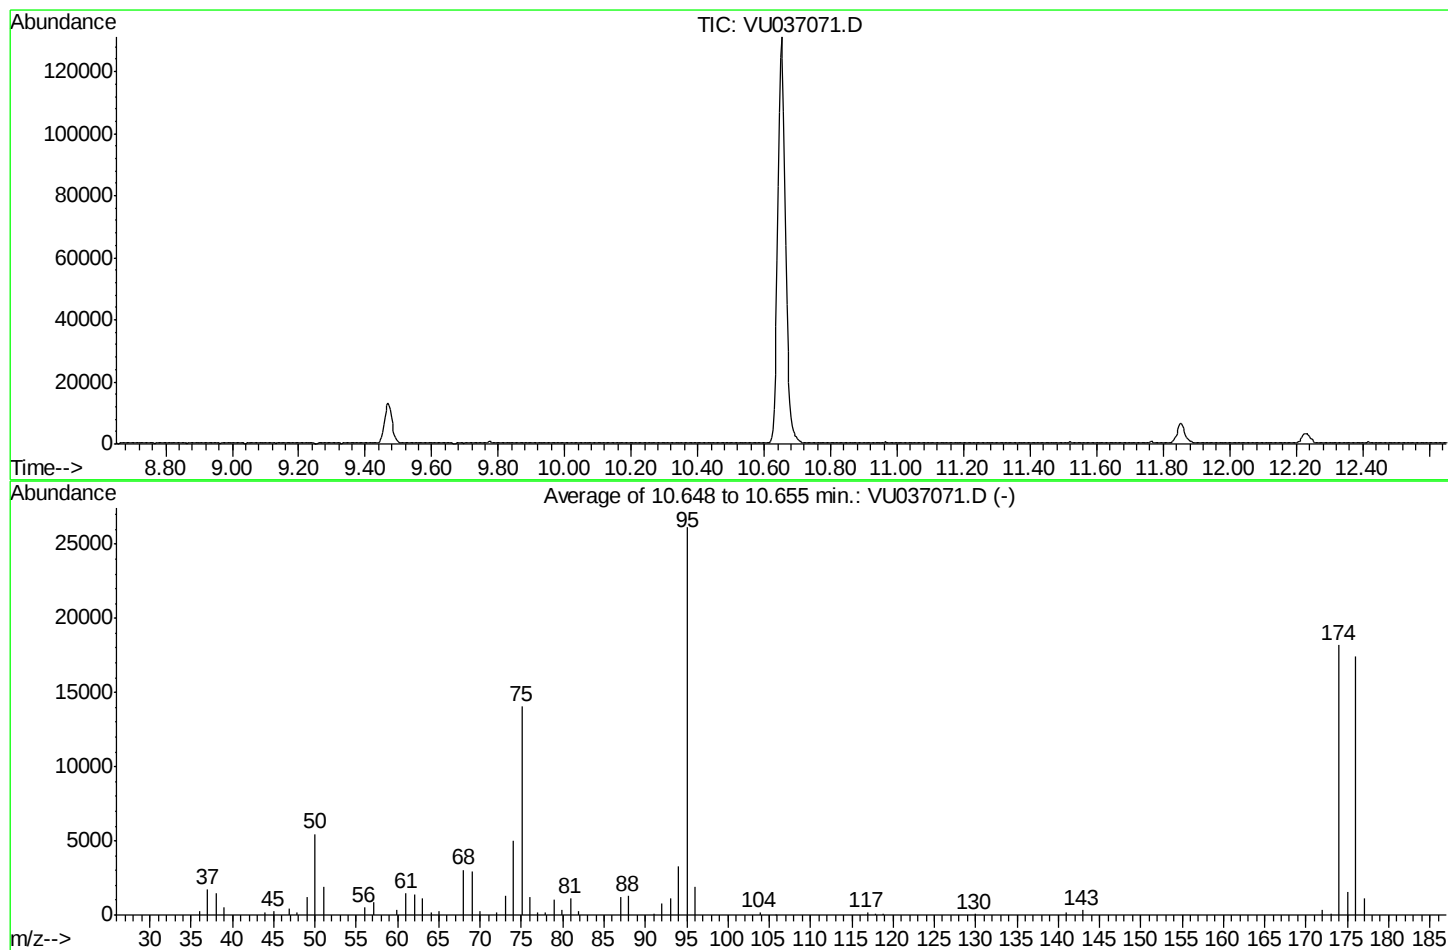

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2884

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	5446	PASS
75	95	30	80	53.7	14044	PASS
95	95	100	100	100.0	26141	PASS
96	95	5	9	7.3	1915	PASS
173	174	0.00	2	0.6	106	PASS
174	95	50	120	69.6	18197	PASS
175	174	5	9	8.4	1520	PASS
176	174	95	101	95.7	17410	PASS
177	176	5	9	6.6	1155	PASS

m/z	Abundance
35.90	275.0
37.00	1661.0
38.00	1511.0
38.90	564.0
40.10	120.0
43.90	485.0
45.00	218.0
46.90	381.0
47.80	185.0
49.00	1140.0
50.00	5339.0
51.00	1870.0
56.00	535.0
57.10	870.0
59.90	300.0
61.00	1419.0
62.00	1374.0
63.00	1084.0
64.10	121.0
65.00	216.0
68.00	3055.0
69.00	2916.0
70.00	258.0
72.00	172.0
73.00	1247.0
74.00	5137.0
75.00	14061.0
76.00	1231.0
77.00	177.0
77.90	170.0
78.90	997.0
79.90	382.0
80.90	1178.0
81.90	288.0
87.00	1149.0
88.00	1262.0
92.00	819.0
93.00	1122.0
94.00	3458.0
95.10	25552.0
96.00	1946.0
103.90	129.0
116.90	142.0
117.90	117.0
118.80	148.0
141.00	150.0
142.90	327.0
171.90	323.0
174.00	17720.0
175.00	1528.0
176.00	16704.0
177.00	1117.0

Instrument :
MSVOA_U
ClientSampleId :
BFB58

m/z	Abundance
36.00	266.0
37.00	1748.0
38.10	1507.0
38.90	532.0
40.10	115.0
43.90	456.0
45.00	231.0
46.90	410.0
47.90	191.0
49.00	1264.0
50.00	5644.0
51.00	1986.0
56.00	508.0
57.00	931.0
59.90	324.0
61.00	1456.0
62.00	1388.0
63.00	1154.0
64.00	146.0
65.00	235.0
68.00	3159.0
69.00	2986.0
69.90	232.0
72.00	195.0
73.00	1354.0
74.00	5234.0
75.00	14670.0
76.10	1249.0
77.00	192.0
77.90	166.0
78.90	1085.0
80.00	376.0
80.90	1174.0
81.90	289.0
86.90	1265.0
87.90	1328.0
91.00	128.0
92.00	822.0
93.00	1107.0
94.00	3422.0
95.10	27128.0
96.00	2007.0
103.90	147.0
116.90	165.0
117.90	102.0
118.90	127.0
129.90	105.0
140.90	181.0
143.00	348.0
172.00	345.0
174.00	18728.0
175.00	1602.0
176.00	18048.0
177.00	1189.0

Instrument :
MSVOA_U
ClientSampleId :
BFB58

m/z	Abundance
36.00	263.0
37.00	1659.0
38.10	1384.0
39.00	448.0
40.10	103.0
44.00	454.0
44.90	253.0
46.90	406.0
47.90	159.0
49.00	1314.0
50.00	5357.0
51.00	1817.0
56.00	429.0
57.00	872.0
59.90	299.0
61.00	1510.0
62.00	1332.0
63.00	1193.0
64.00	135.0
65.00	207.0
68.00	2888.0
69.00	2813.0
69.90	209.0
72.00	165.0
73.00	1298.0
74.00	4769.0
75.10	13401.0
76.10	1179.0
77.00	180.0
77.90	141.0
78.90	1045.0
80.00	319.0
80.90	1013.0
81.90	275.0
86.90	1262.0
87.90	1259.0
91.00	140.0
92.00	787.0
93.00	1044.0
94.00	3041.0
95.10	25744.0
96.00	1792.0
103.90	132.0
105.80	108.0
116.90	184.0
129.90	115.0
141.00	205.0
143.00	292.0
172.00	339.0
173.00	320.0
174.00	18144.0
175.00	1430.0
176.00	17480.0
177.00	1160.0

Instrument :
MSVOA_U
ClientSampleId :
BFB58

Scan 2884 (10.613 min): VU037071.D
BFB58

m/z	Abundance
39.90	144.0
43.90	283.0

Instrument :
MSVOA_U
ClientSampleId :
BFB58