

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030521\
 Data File : VU042497.D
 Acq On : 05 Mar 2021 10:52
 Operator : SY/MD
 Sample : VU0305WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Quant Time: Mar 05 13:46:18 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Mar 05 00:31:48 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)




Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	93212	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	87893	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.819	152	43785	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	27121	4.36	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	87.20%
7) Chloroethane-d5	1.919	69	22737	4.83	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.60%
11) 1,1-Dichloroethene-d2	2.575	63	45860	3.27	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	65.40%
20) 2-Butanone-d5	4.645	46	111018m	54.41	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	108.82%
24) Chloroform-d	5.073	84	58124	4.73	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.60%
26) 1,2-Dichloroethane-d4	5.713	65	38456	5.09	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.80%
32) Benzene-d6	5.735	84	105727	4.91	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.20%
36) 1,2-Dichloropropane-d6	6.700	67	34958	5.03	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.60%
41) Toluene-d8	7.906	98	98441	4.68	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.60%
43) trans-1,3-Dichloroprop...	8.189	79	15043	4.63	ug/L	0.00
46) 2-Hexanone-d5	8.645	63	79904	51.38	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	102.76%
57) 1,1,2,2-Tetrachloroeth...	10.764	84	31761	5.13	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.60%
64) 1,2-Dichlorobenzene-d4	12.201	152	40343	5.08	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.60%

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030521\
Data File : VU042497.D
Acq On : 05 Mar 2021 10:52
Operator : SY/MD
Sample : VU0305WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Mar 05 13:46:18 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Mar 05 00:31:48 2021
Response via : Initial Calibration

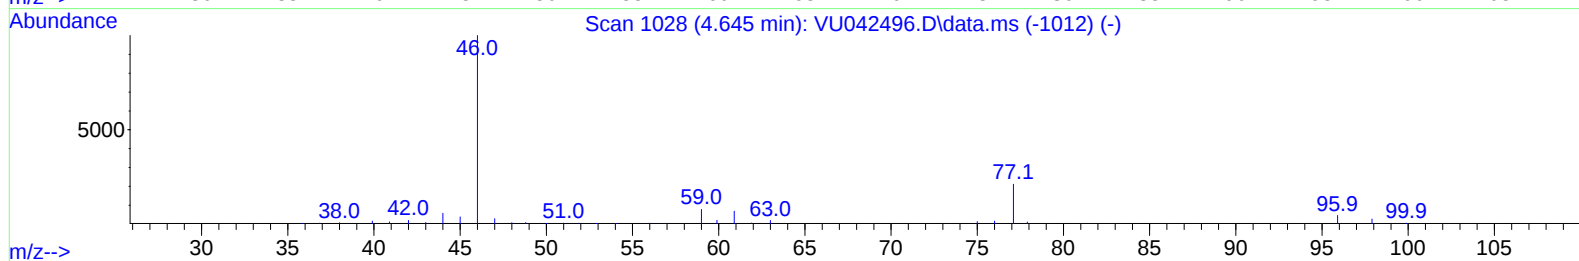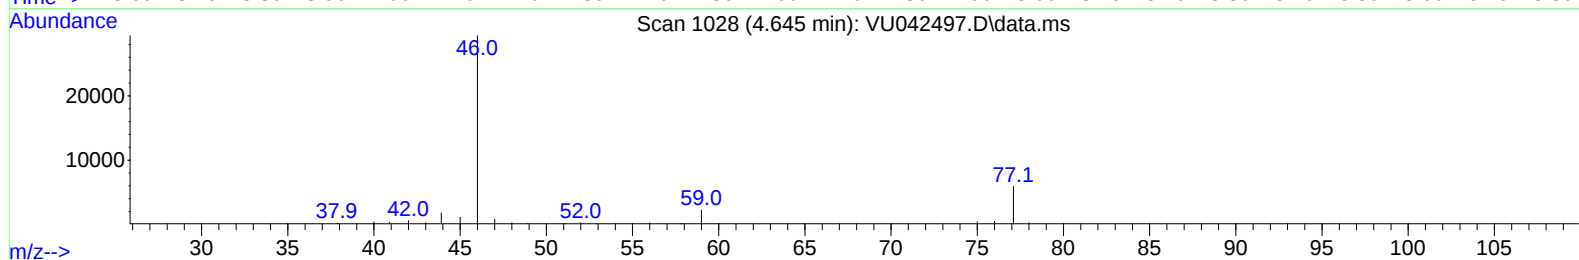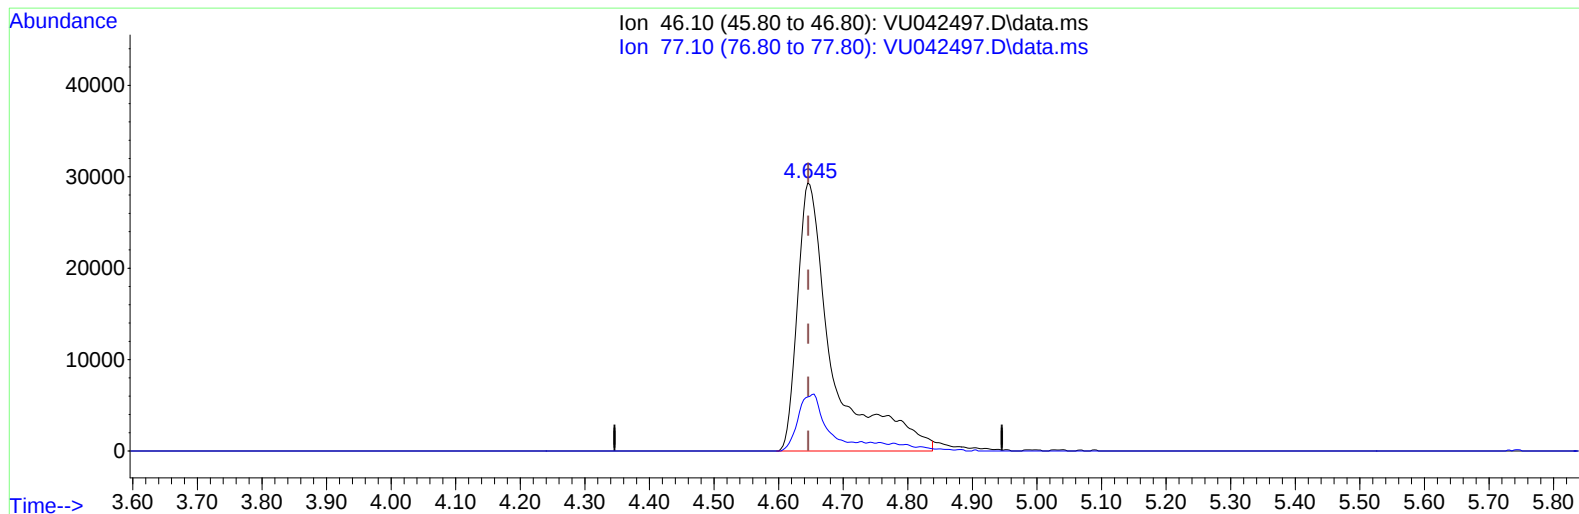

TIC: VU042497.D\data.ms

(20) 2-Butanone-d5 (S)




4.645min (-0.000) 54.41 ug/L m

response 111018

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	22.00	16.49
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030521\
Data File : VU042497.D
Acq On : 05 Mar 2021 10:52
Operator : SY/MD
Sample : VU0305WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Mar 05 13:46:18 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Mar 05 00:31:48 2021
Response via : Initial Calibration

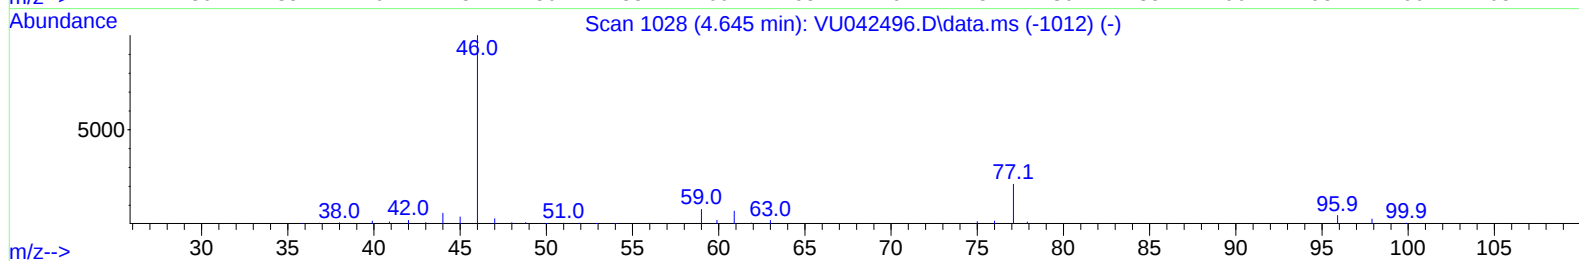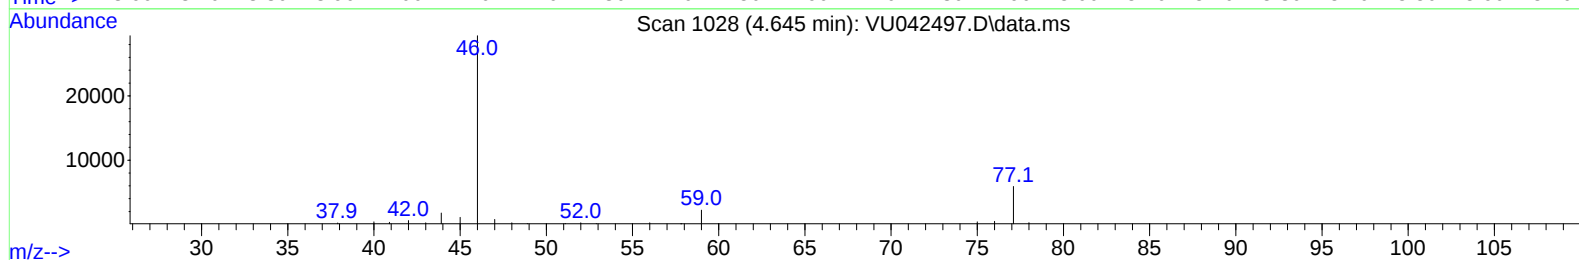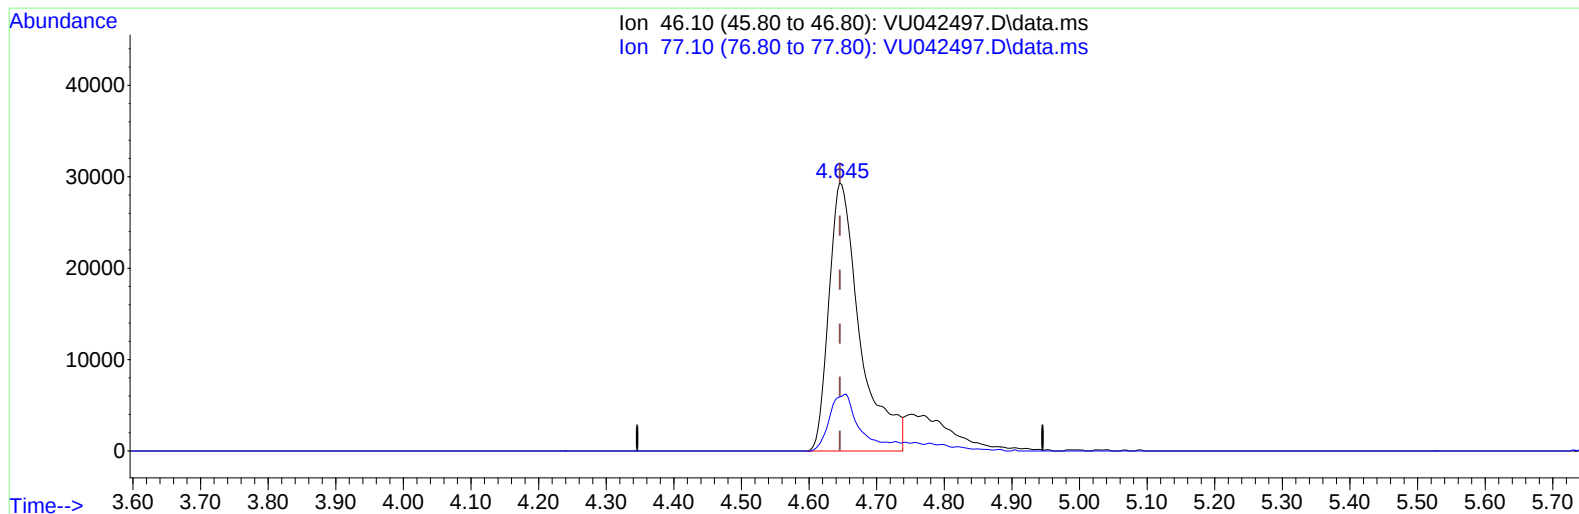

TIC: VU042497.D\data.ms

(20) 2-Butanone-d5 (S)

4.645min (-0.000) 46.00 ug/L

response 93849

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	22.00	19.51
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030521\
Data File : VU042497.D
Acq On : 05 Mar 2021 10:52
Operator : SY/MD
Sample : VU0305WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Mar 05 13:46:18 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Mar 05 00:31:48 2021
Response via : Initial Calibration

