

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030521\
 Data File : VU042506.D
 Acq On : 05 Mar 2021 16:40
 Operator : SY/MD
 Sample : M1588-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C03T1

Quant Time: Mar 06 00:49:11 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Mar 05 00:31:48 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	84041	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.426	117	81208	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.819	152	39320	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	24669	4.40	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	88.00%
7) Chloroethane-d5	1.919	69	21400	5.04	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.80%
11) 1,1-Dichloroethene-d2	2.575	63	44507	3.52	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.40%
20) 2-Butanone-d5	4.645	46	87440	47.53	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	95.06%
24) Chloroform-d	5.073	84	54806	4.95	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.00%
26) 1,2-Dichloroethane-d4	5.710	65	36325	5.33	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.60%
32) Benzene-d6	5.735	84	98619	4.95	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.00%
36) 1,2-Dichloropropane-d6	6.700	67	32676	5.09	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.80%
41) Toluene-d8	7.906	98	91259	4.69	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.80%
43) trans-1,3-Dichloroprop...	8.189	79	13600	4.53	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.60%
46) 2-Hexanone-d5	8.645	63	72846	50.70	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	101.40%
57) 1,1,2,2-Tetrachloroeth...	10.764	84	28621	5.00	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.00%
64) 1,2-Dichlorobenzene-d4	12.201	152	38266	5.37	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.40%
Target Compounds					Qvalue	
13) Acetone	2.658	43	2372	1.67	ug/L	82

(#) = qualifier out of range (m) = manual integration (+) = signals summed




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030521\
Data File : VU042506.D
Acq On : 05 Mar 2021 16:40
Operator : SY/MD
Sample : M1588-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C03T1

Quant Time: Mar 06 00:49:11 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Mar 05 00:31:48 2021
Response via : Initial Calibration

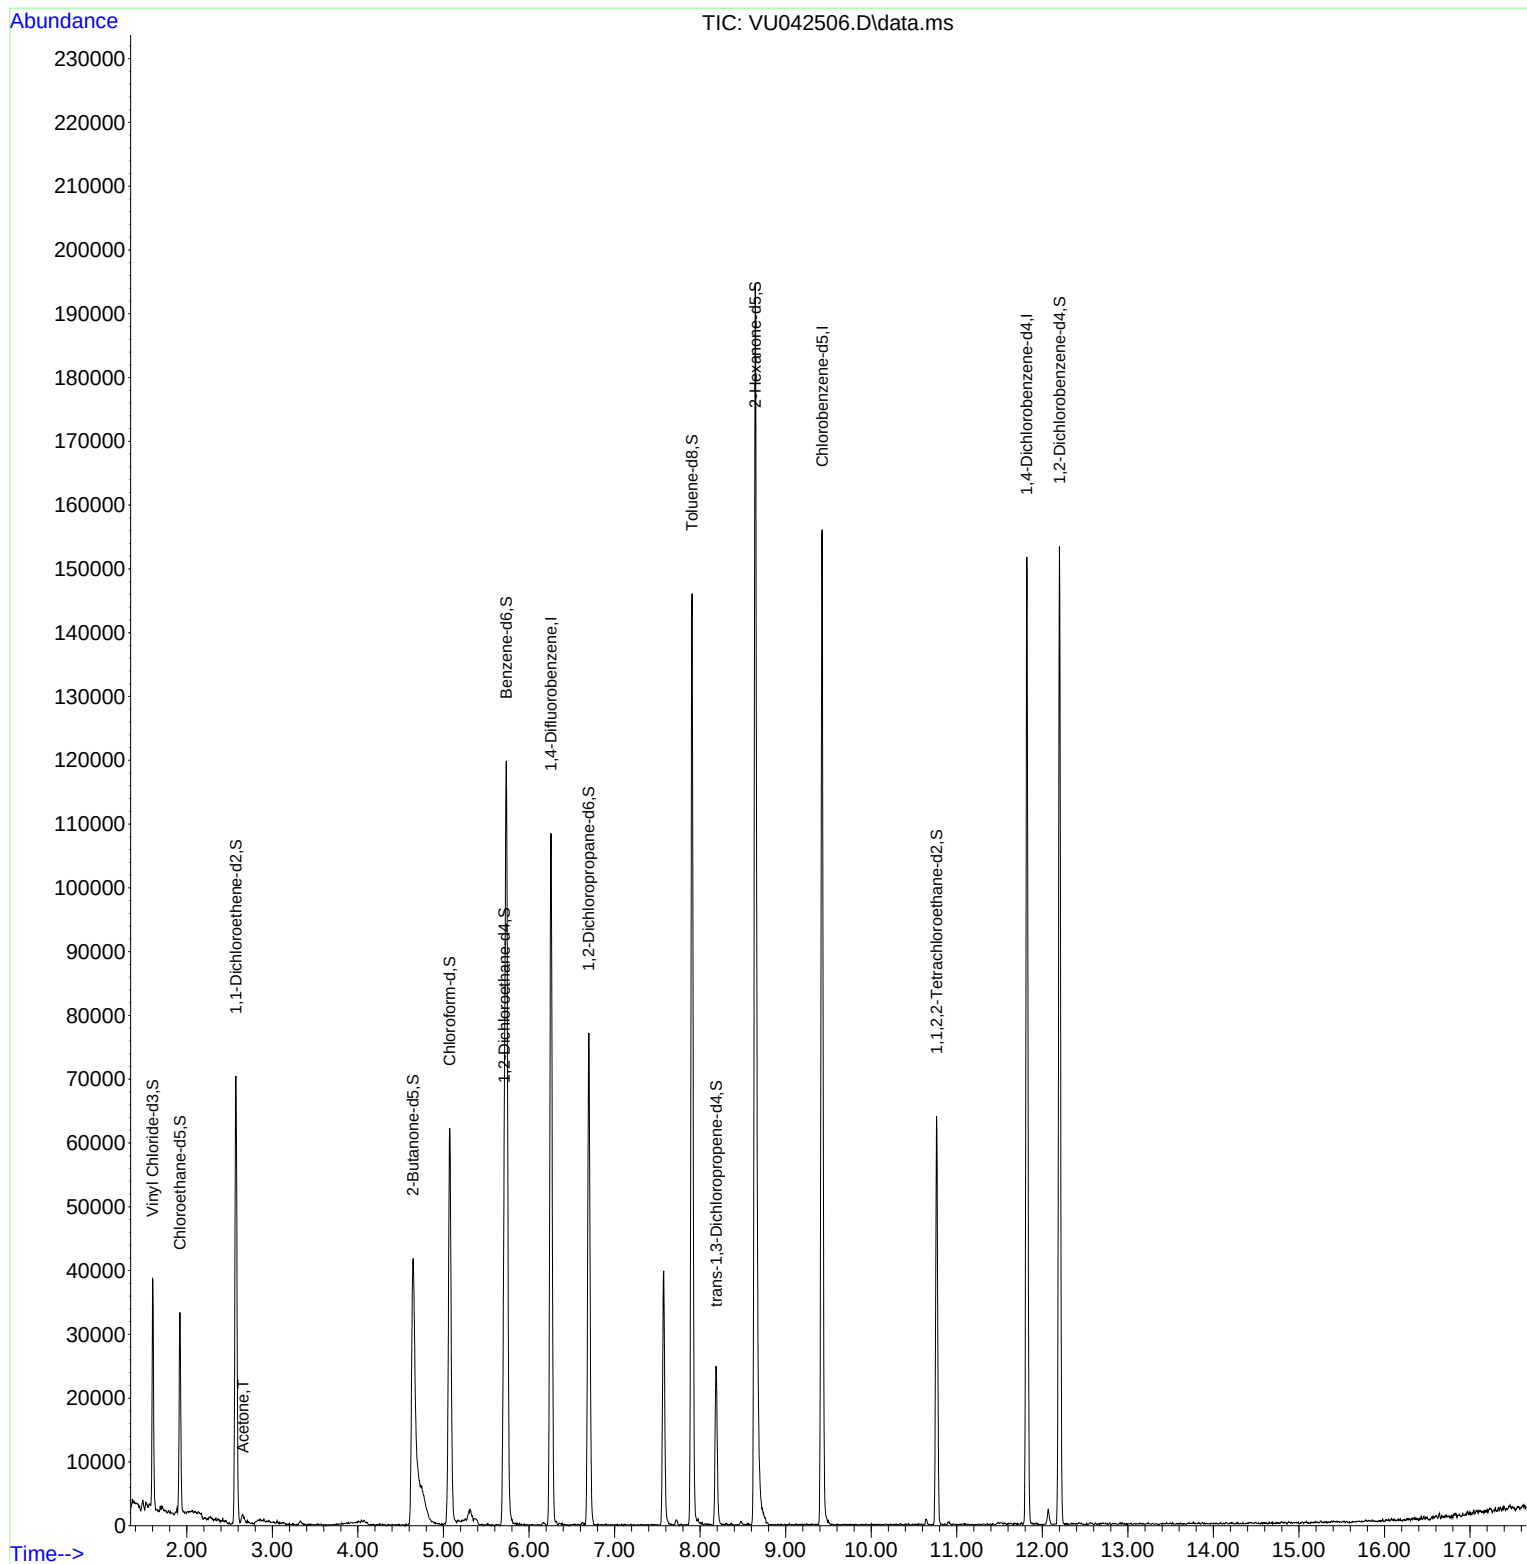

Abundance Scan 409 (2.655 min): VU042496.D\data.ms (-39

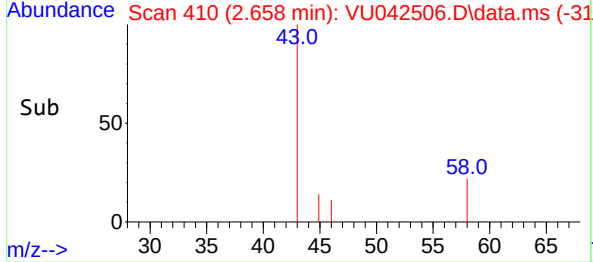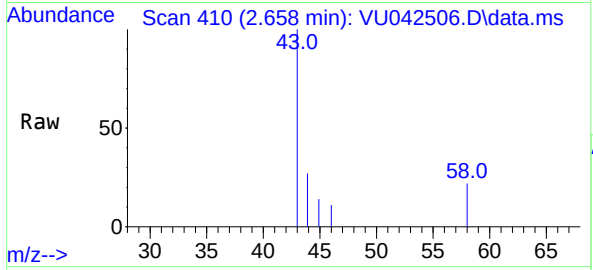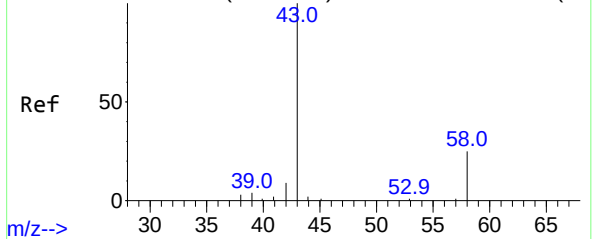

#13

Acetone

Concen: 1.67 ug/L

RT: 2.658 min Scan# 410

Delta R.T. -0.000 min

Lab File: VU042506.D


Acq: 05 Mar 2021 16:40

Tgt Ion: 43 Resp: 2372

Ion Ratio Lower Upper

43 100

58 18.3 0.0 55.8

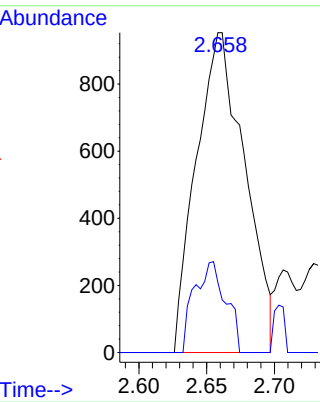

Instrument :

MSVOA_U

ClientSampleId :

C03T1