

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030521\
 Data File : VU042507.D
 Acq On : 05 Mar 2021 17:04
 Operator : SY/MD
 Sample : M1588-08
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C03T2

Quant Time: Mar 06 00:49:30 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Mar 05 00:31:48 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.260	114	82424	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.427	117	78989	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.819	152	38302	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	24850	4.52	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.40%
7) Chloroethane-d5	1.919	69	20841	5.01	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.20%
11) 1,1-Dichloroethene-d2	2.572	63	42641	3.44	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.80%
20) 2-Butanone-d5	4.642	46	88618	49.12	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.24%
24) Chloroform-d	5.073	84	54834	5.05	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.00%
26) 1,2-Dichloroethane-d4	5.713	65	35775	5.35	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.00%
32) Benzene-d6	5.735	84	98636	5.09	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.80%
36) 1,2-Dichloropropane-d6	6.700	67	32638	5.22	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.40%
41) Toluene-d8	7.906	98	91670	4.85	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.00%
43) trans-1,3-Dichloroprop...	8.185	79	13587	4.66	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	93.20%
46) 2-Hexanone-d5	8.645	63	73249	52.41	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	104.82%
57) 1,1,2,2-Tetrachloroeth...	10.764	84	28555	5.13	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.60%
64) 1,2-Dichlorobenzene-d4	12.201	152	36792	5.30	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.00%
Target Compounds						
13) Acetone	2.652	43	2072	1.49	ug/L	Qvalue 86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030521\
Data File : VU042507.D
Acq On : 05 Mar 2021 17:04
Operator : SY/MD
Sample : M1588-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C03T2

Quant Time: Mar 06 00:49:30 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Mar 05 00:31:48 2021
Response via : Initial Calibration

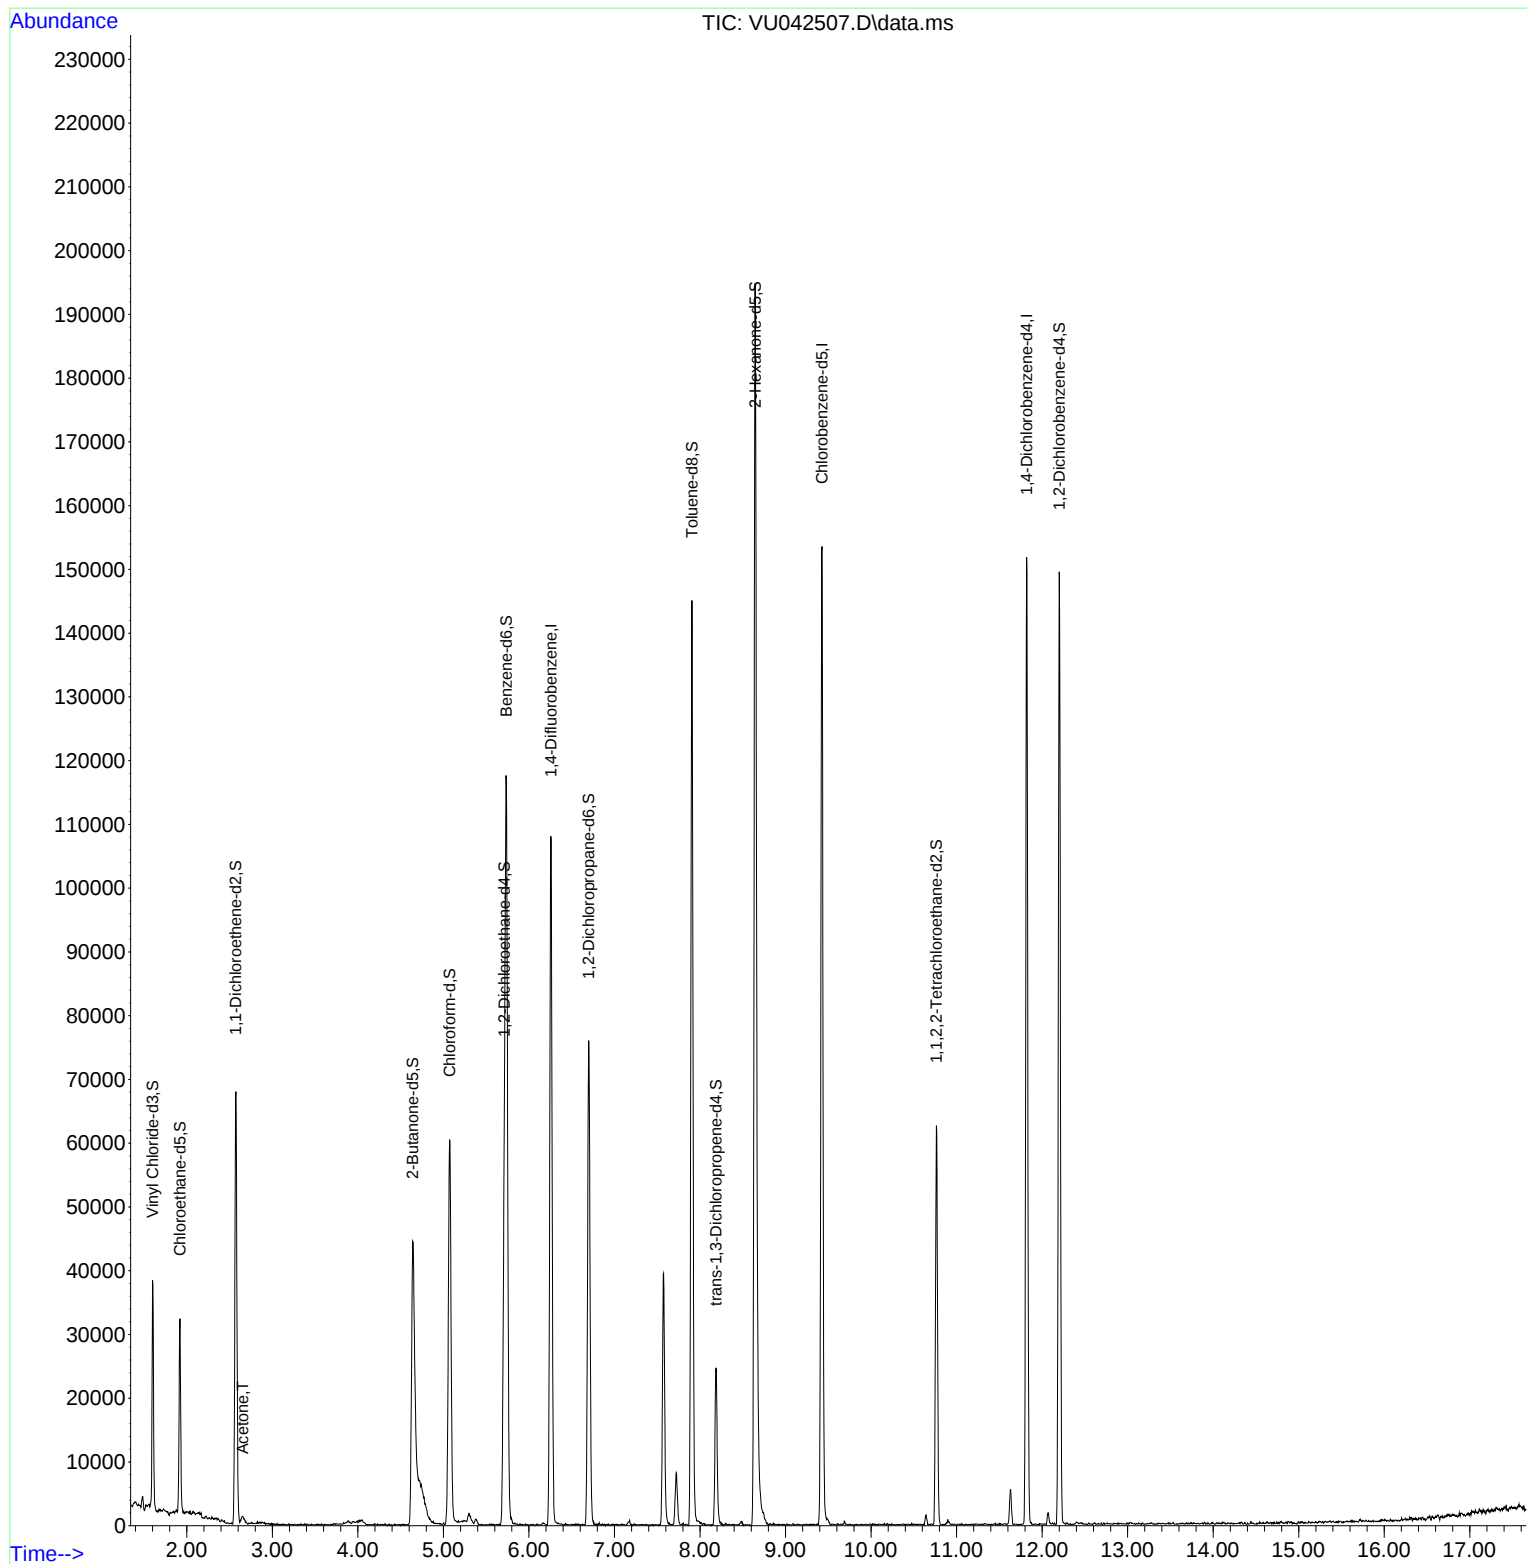

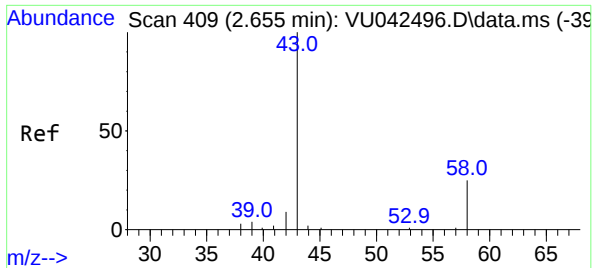

#13
 Acetone
 Concen: 1.49 ug/L
 RT: 2.652 min Scan# 408
 Delta R.T. -0.007 min
 Lab File: VU042507.D
 Acq: 05 Mar 2021 17:04

Instrument :
 MSVOA_U
 ClientSampleId :
 C03T2

Tgt Ion: 43 Resp: 2072

Ion	Ratio	Lower	Upper
43	100		
58	20.7	0.0	55.8

