

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030521\
 Data File : VU042511.D
 Acq On : 05 Mar 2021 18:40
 Operator : SY/MD
 Sample : M1588-12
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C03T6

Quant Time: Mar 06 00:50:56 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Mar 05 00:31:48 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	85888	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.426	117	81721	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.822	152	38464	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	23546	4.11	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery = 82.20%			
7) Chloroethane-d5	1.919	69	20989	4.84	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery = 96.80%			
11) 1,1-Dichloroethene-d2	2.575	63	41301	3.19	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery = 63.80%			
20) 2-Butanone-d5	4.645	46	85099	45.27	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery = 90.54%			
24) Chloroform-d	5.073	84	52922	4.67	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery = 93.40%			
26) 1,2-Dichloroethane-d4	5.713	65	35204	5.05	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery = 101.00%			
32) Benzene-d6	5.735	84	94547	4.72	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery = 94.40%			
36) 1,2-Dichloropropane-d6	6.700	67	32716	5.06	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery = 101.20%			
41) Toluene-d8	7.906	98	87198	4.46	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery = 89.20%			
43) trans-1,3-Dichloroprop...	8.185	79	12911	4.28	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery = 85.60%			
46) 2-Hexanone-d5	8.645	63	71671	49.57	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery = 99.14%			
57) 1,1,2,2-Tetrachloroeth...	10.764	84	27898	4.85	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery = 97.00%			
64) 1,2-Dichlorobenzene-d4	12.201	152	37943	5.44	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery = 108.80%			
Target Compounds					Qvalue	
13) Acetone	2.655	43	1145	0.79	ug/L	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030521\
Data File : VU042511.D
Acq On : 05 Mar 2021 18:40
Operator : SY/MD
Sample : M1588-12
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C03T6

Quant Time: Mar 06 00:50:56 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Mar 05 00:31:48 2021
Response via : Initial Calibration

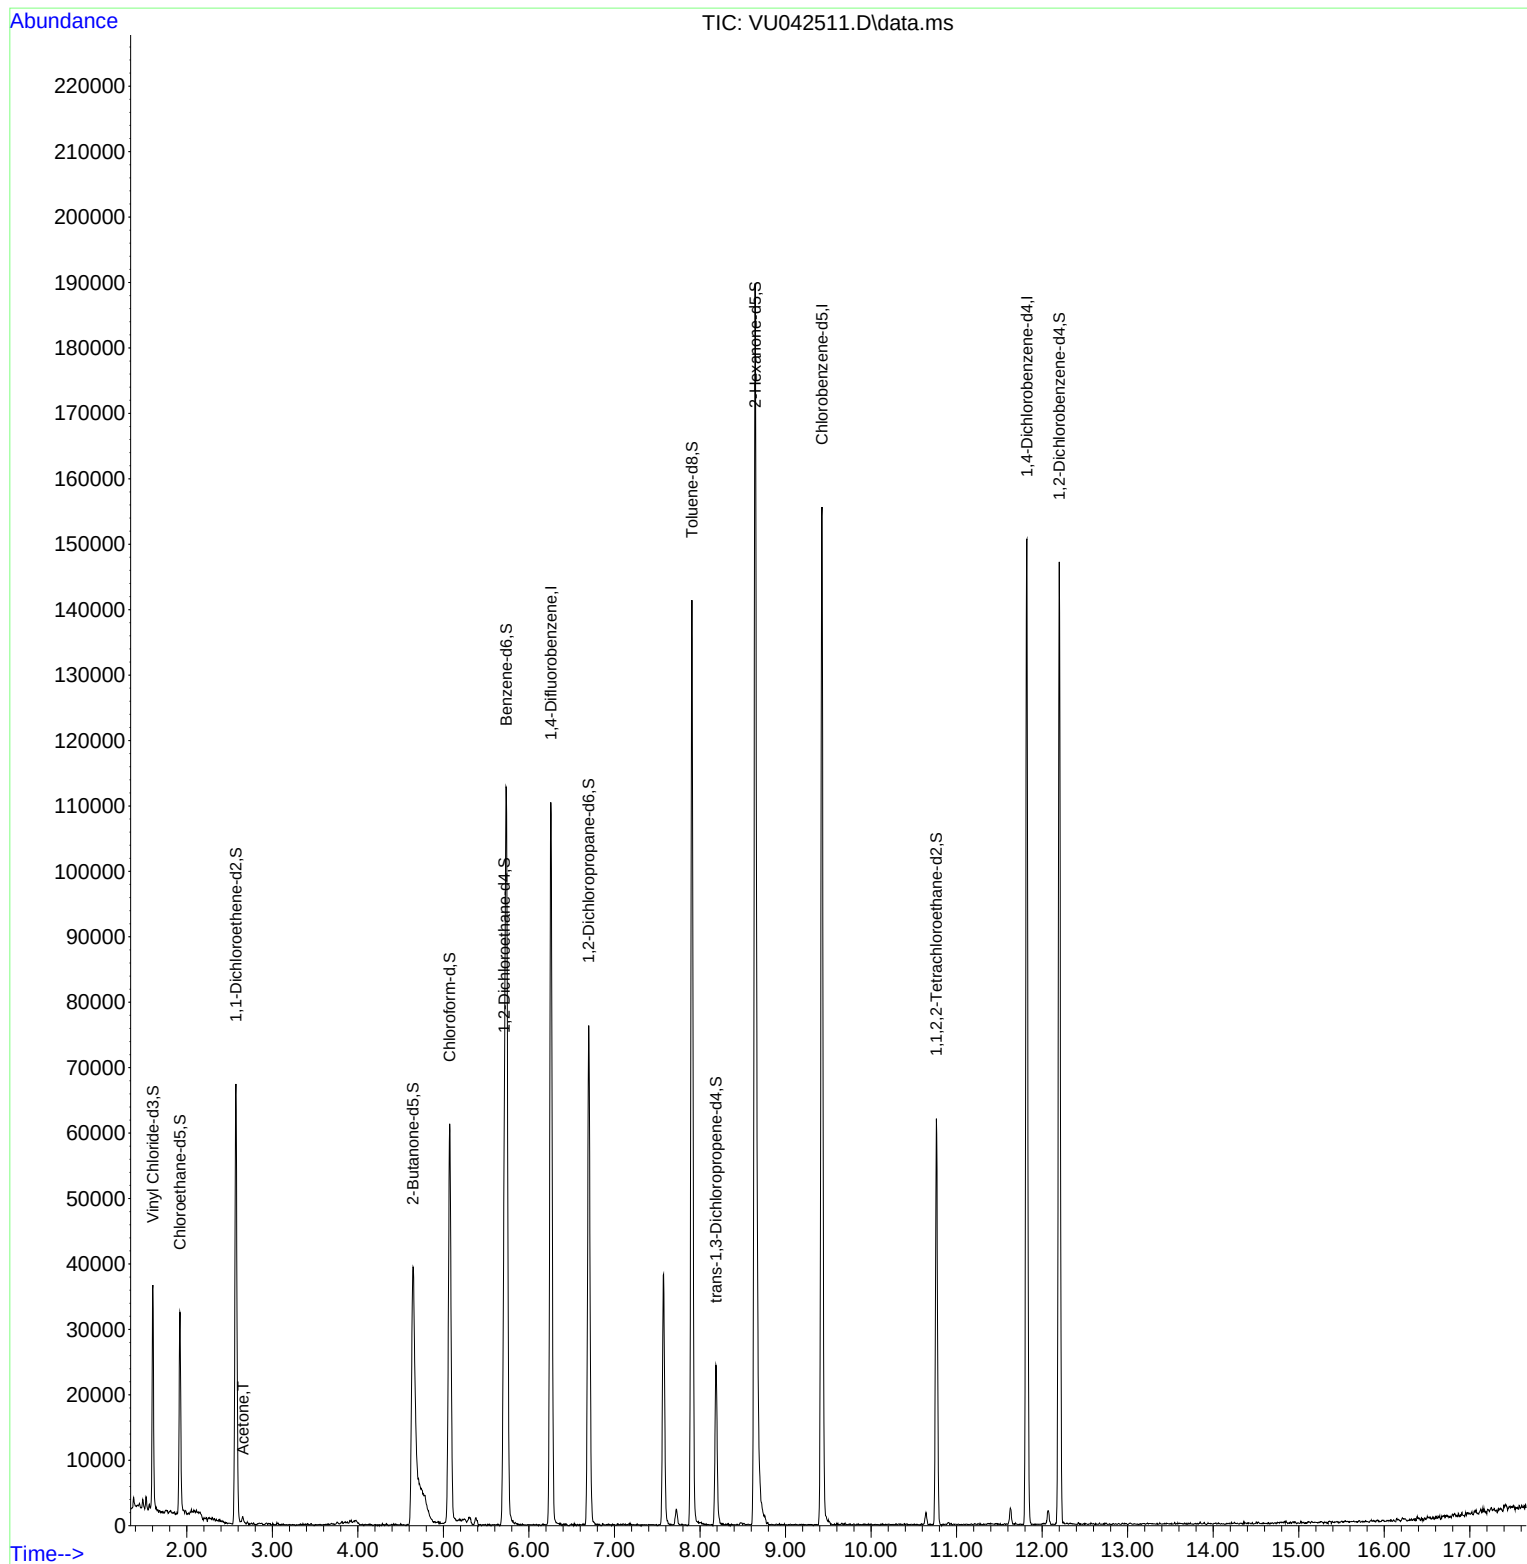

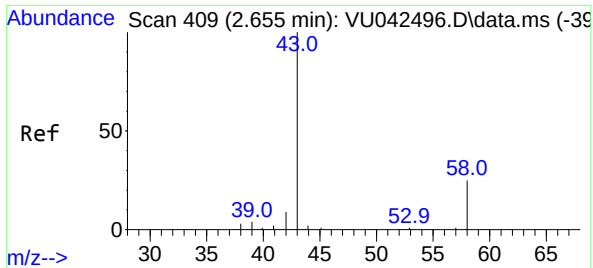

#13
 Acetone
 Concen: 0.79 ug/L
 RT: 2.655 min Scan# 409
 Delta R.T. -0.003 min
 Lab File: VU042511.D
 Acq: 05 Mar 2021 18:40

Instrument :
 MSVOA_U
 ClientSampleId :
 C03T6

Tgt Ion:	43	Resp:	1145
Ion	Ratio	Lower	Upper
43	100		
58	18.2	0.0	55.8

