

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030521\
 Data File : VU042512.D
 Acq On : 05 Mar 2021 19:04
 Operator : SY/MD
 Sample : M1588-13
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C03W0

Quant Time: Mar 06 00:51:15 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Mar 05 00:31:48 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.259	114	84158	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	80118	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.819	152	38414	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	23706	4.23	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	84.60%
7) Chloroethane-d5	1.919	69	20629	4.86	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.20%
11) 1,1-Dichloroethene-d2	2.575	63	39576	3.12	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	62.40%
20) 2-Butanone-d5	4.642	46	89679	48.68	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	97.36%
24) Chloroform-d	5.073	84	51390	4.63	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.60%
26) 1,2-Dichloroethane-d4	5.713	65	33842	4.96	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.20%
32) Benzene-d6	5.738	84	92939	4.73	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.60%
36) 1,2-Dichloropropane-d6	6.700	67	31018	4.90	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.00%
41) Toluene-d8	7.906	98	86918	4.53	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.60%
43) trans-1,3-Dichloroprop...	8.185	79	13029	4.40	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.00%
46) 2-Hexanone-d5	8.645	63	68335	48.21	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.42%
57) 1,1,2,2-Tetrachloroeth...	10.764	84	27665	4.90	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.00%
64) 1,2-Dichlorobenzene-d4	12.201	152	35240	5.06	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.20%
Target Compounds						Qvalue
3) Chloromethane	1.523	50	1571	0.21	ug/L	98
13) Acetone	2.655	43	2441	1.72	ug/L	89
29) 1,1,1-Trichloroethane	5.324	97	2041	0.18	ug/L #	77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030521\
Data File : VU042512.D
Acq On : 05 Mar 2021 19:04
Operator : SY/MD
Sample : M1588-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C03W0

Quant Time: Mar 06 00:51:15 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Mar 05 00:31:48 2021
Response via : Initial Calibration




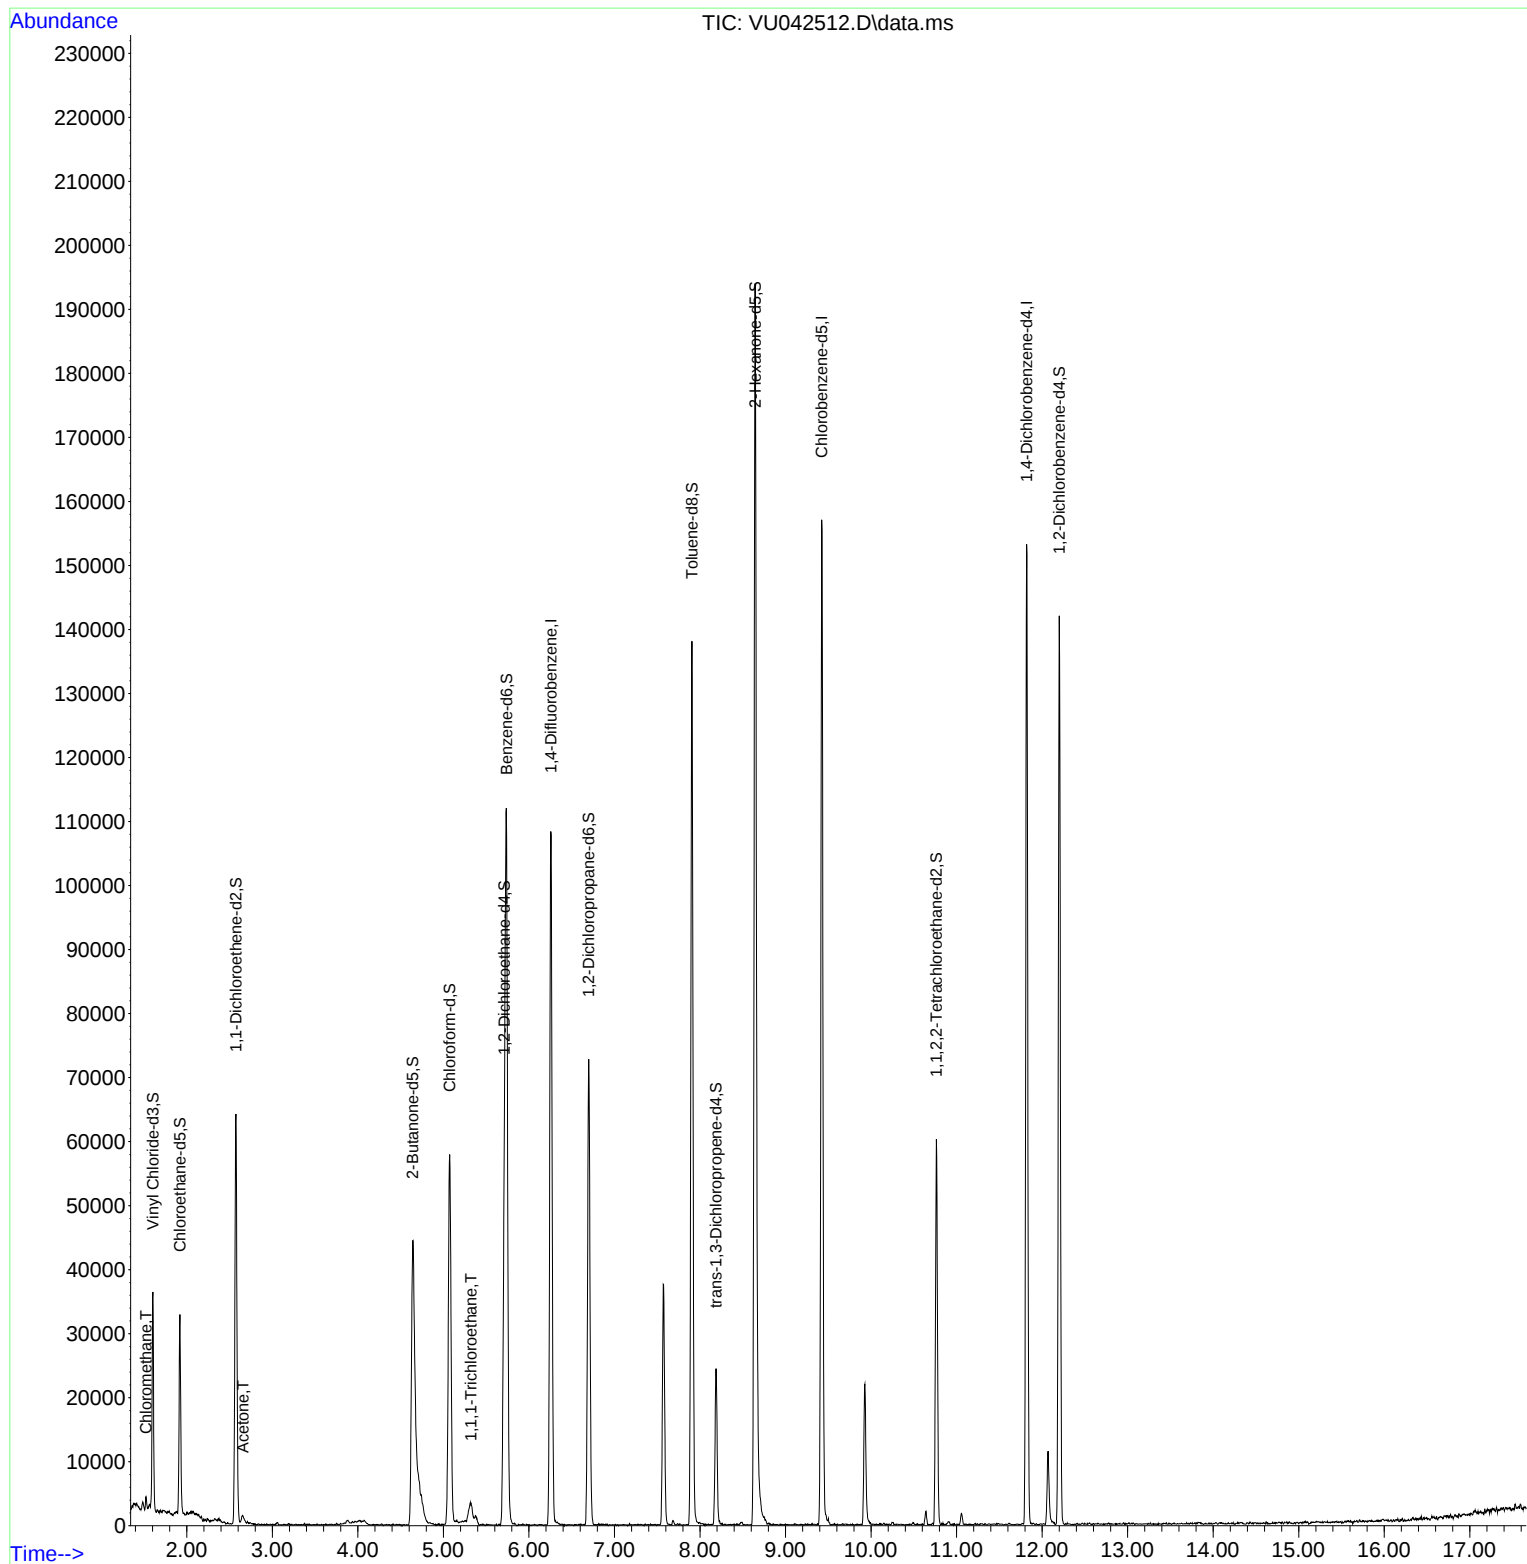


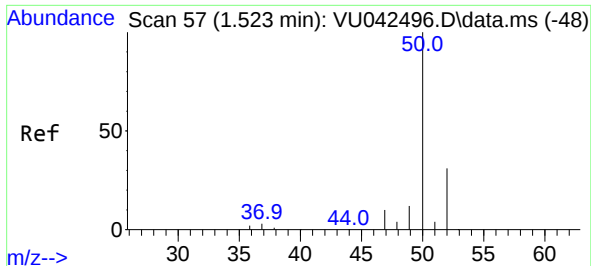

#3
Chloromethane
Concen: 0.21 ug/L
RT: 1.523 min Scan# 57
Delta R.T. 0.003 min
Lab File: VU042512.D
Acq: 05 Mar 2021 19:04




Instrument :
MSVOA_U
ClientSampled :
C03W0


Tgt Ion: 50 Resp: 1571
Ion Ratio Lower Upper
50 100
52 31.7 23.0 42.8

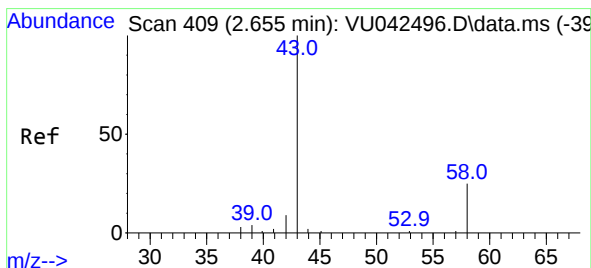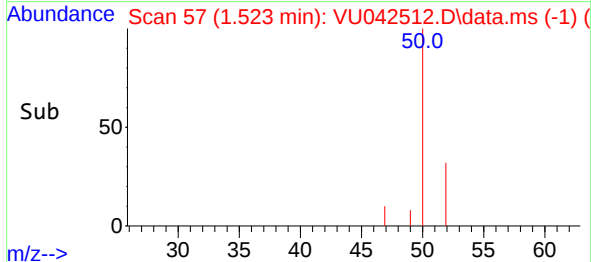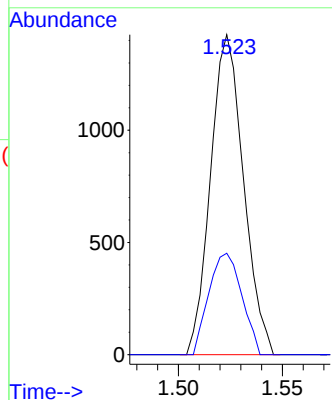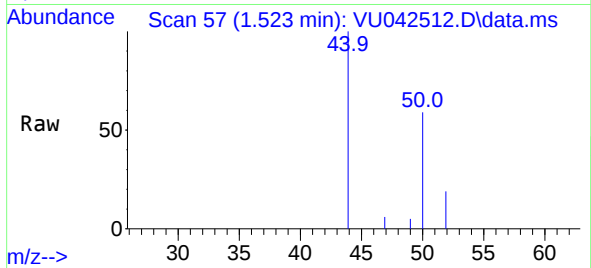

#13
Acetone
Concen: 1.72 ug/L
RT: 2.655 min Scan# 409
Delta R.T. -0.003 min
Lab File: VU042512.D
Acq: 05 Mar 2021 19:04

Tgt Ion: 43 Resp: 2441
Ion Ratio Lower Upper
43 100
58 22.0 0.0 55.8

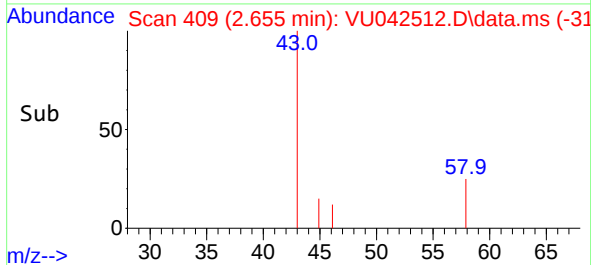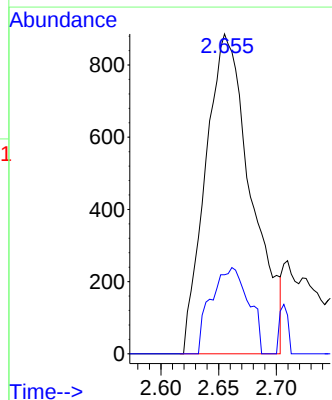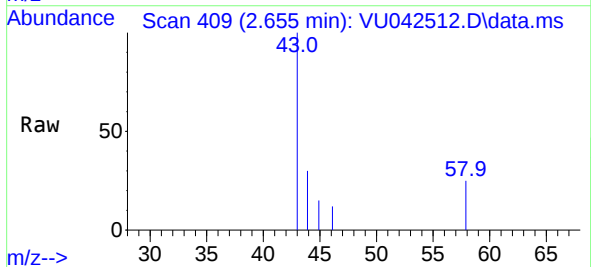

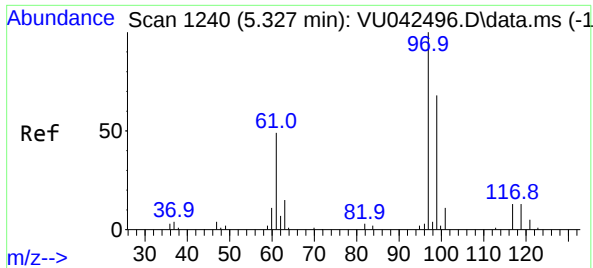

#29
1,1,1-Trichloroethane
Concen: 0.18 ug/L
RT: 5.324 min Scan# 1239
Delta R.T. -0.003 min
Lab File: VU042512.D
Acq: 05 Mar 2021 19:04

Instrument :
MSVOA_U
ClientSampleId :
C03W0

Tgt Ion: 97 Resp: 2041

Ion	Ratio	Lower	Upper
97	100		
99	55.6	50.8	76.2
61	18.6	35.8	53.6#

