


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030521\
 Data File : VU042495.D
 Acq On : 05 Mar 2021 08:58
 Operator : SY/MD
 Sample : BFB22
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB22

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Mar 05 00:31:48 2021

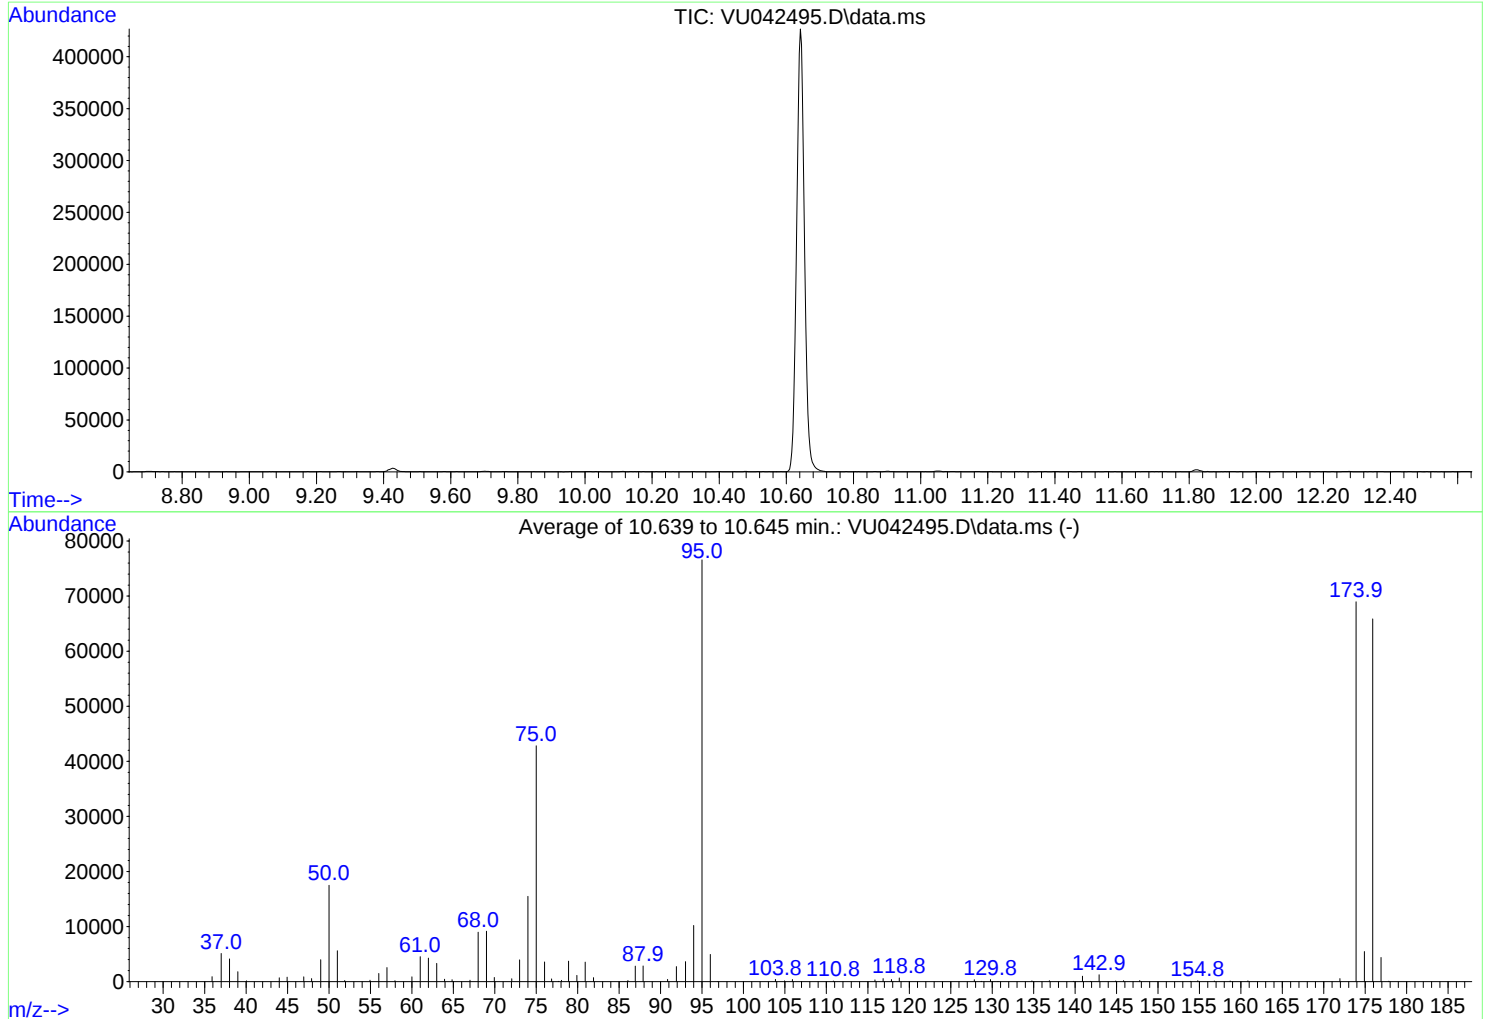

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.8	17493	PASS
75	95	30	80	55.9	42829	PASS
95	95	100	100	100.0	76584	PASS
96	95	5	9	6.4	4933	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	90.0	68960	PASS
175	174	5	9	7.9	5476	PASS
176	174	95	101	95.5	65872	PASS
177	176	5	9	6.7	4402	PASS

m/z	Abundance
35.90	842.0
37.00	5161.0
38.00	4146.0
39.00	1698.0
40.10	101.0
44.00	835.0
44.90	854.0
46.90	816.0
47.90	534.0
49.00	4143.0
50.00	17360.0
51.00	5412.0
51.90	227.0
55.00	301.0
56.00	1516.0
57.00	2546.0
58.00	162.0
60.00	939.0
61.00	4519.0
62.00	4272.0
63.00	3371.0
64.00	445.0
64.90	380.0
67.00	231.0
68.00	8696.0
69.00	9182.0
69.90	760.0
72.10	575.0
73.00	3944.0
74.00	14875.0
75.00	42472.0
76.00	3667.0
76.90	466.0
78.00	246.0
78.90	3700.0
79.90	1124.0
80.90	3501.0
81.90	699.0
86.00	141.0
86.90	2840.0
87.90	2752.0
90.80	390.0
91.90	2708.0
93.00	3665.0
94.00	9835.0
95.00	75344.0
96.00	5077.0
103.80	421.0
105.00	153.0
105.90	374.0
107.00	102.0
110.90	122.0
115.80	321.0
116.80	544.0
117.90	332.0
118.80	644.0
127.90	351.0
128.70	121.0
129.80	319.0
130.70	118.0
134.80	138.0
136.90	153.0
140.90	966.0
141.80	101.0
142.90	1197.0
144.90	137.0
145.90	147.0
147.80	210.0
154.80	212.0
157.00	112.0
158.70	115.0
160.80	158.0
172.00	561.0
173.90	65144.0
174.90	5011.0
175.90	62808.0
176.90	4240.0
177.90	126.0

Instrument :
MSVOA_U
ClientSampleId :
BFB22

m/z	Abundance
35.90	974.0
37.00	5324.0
38.00	4229.0
39.00	1888.0
40.00	142.0
44.00	902.0
45.00	817.0
46.90	899.0
47.90	573.0
49.00	4172.0
50.00	17960.0
51.00	5774.0
51.90	203.0
55.00	269.0
56.00	1511.0
57.00	2614.0
58.00	178.0
60.00	905.0
61.00	4684.0
62.00	4388.0
63.00	3390.0
64.00	451.0
64.80	368.0
67.00	263.0
68.00	9378.0
69.00	9497.0
69.90	778.0
72.00	536.0
73.00	4088.0
74.00	16012.0
75.00	44072.0
76.00	3709.0
76.90	532.0
78.10	252.0
78.90	3825.0
79.90	1181.0
80.90	3657.0
81.90	745.0
86.00	215.0
87.00	2909.0
87.90	2930.0
90.80	436.0
91.90	2872.0
93.00	3745.0
94.00	10533.0
95.00	79040.0
96.00	5057.0
103.90	397.0
104.90	133.0
105.90	400.0
110.90	134.0
115.80	333.0
116.80	562.0
117.80	388.0
118.80	702.0
127.80	340.0
128.70	103.0
129.80	371.0
134.80	152.0
136.90	181.0
139.80	100.0
140.90	1004.0
142.90	1276.0
144.90	129.0
145.80	199.0
147.80	202.0
153.90	108.0
154.80	183.0
156.80	131.0
158.70	146.0
160.90	160.0
171.90	565.0
173.90	71112.0
174.90	5713.0
175.90	67920.0
176.90	4553.0
177.80	122.0

Instrument :
MSVOA_U
ClientSampleId :
BFB22

m/z	Abundance
35.90	932.0
37.00	4850.0
38.00	3992.0
39.00	1871.0
40.00	186.0
44.00	906.0
45.00	768.0
47.00	887.0
47.90	531.0
49.00	3659.0
50.00	17160.0
51.00	5655.0
51.90	191.0
54.90	192.0
56.00	1441.0
57.00	2479.0
57.90	156.0
60.00	800.0
61.00	4421.0
62.00	4159.0
63.00	3171.0
63.90	420.0
64.80	270.0
67.00	267.0
68.00	8849.0
69.00	8800.0
70.00	695.0
72.00	448.0
73.00	3833.0
74.00	15594.0
75.00	41944.0
76.00	3398.0
76.80	492.0
77.70	219.0
78.10	238.0
78.90	3608.0
79.90	1103.0
80.90	3465.0
81.90	760.0
86.10	239.0
87.00	2732.0
87.90	2878.0
90.90	433.0
91.90	2622.0
93.00	3518.0
94.00	10221.0
95.00	75368.0
96.00	4665.0
96.90	102.0
103.90	375.0
104.90	128.0
105.90	387.0
110.80	115.0
115.90	328.0
116.90	546.0
117.80	401.0
118.80	623.0
127.80	342.0
129.80	414.0
134.80	150.0
136.90	178.0
139.80	111.0
140.90	973.0
141.90	107.0
142.90	1272.0
144.90	102.0
145.80	199.0
147.80	177.0
153.90	107.0
154.80	172.0
156.70	146.0
158.70	129.0
160.90	127.0
171.90	545.0
173.90	70624.0
174.90	5705.0
175.90	66888.0
176.90	4414.0

Instrument :
MSVOA_U
ClientSampleId :
BFB22

m/z	Abundance
44.00	174.0

Instrument :
MSVOA_U
ClientSampleId :
BFB22