

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030524\
 Data File : VU057988.D
 Acq On : 05 Mar 2024 13:31
 Operator : MD/SY
 Sample : VU0305WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Mar 06 01:48:22 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM030524.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Mar 06 01:33:52 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.257	114	5125	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.418	117	7533	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.808	152	2287	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.597	65	3203	0.535	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	106.000%
4) 1,2-Dichloroethane-d4	5.685	65	1933	0.545	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	108.000%
7) 1,2-Dichloropropane-d6	6.687	67	2385	0.580	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	116.000%
8) Toluene-d8	7.887	98	6028	0.536	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	108.000%
10) 1,1,2,2-Tetrachloroeth...	10.745	84	1479	0.570	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	114.000%
Target Compounds						
13) 1,2-Dibromo-3-chloropr...	12.750	75	16	0.043	ug/L	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030524\
Data File : VU057988.D
Acq On : 05 Mar 2024 13:31
Operator : MD/SY
Sample : VU0305WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: Mar 06 01:48:22 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM030524.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Mar 06 01:33:52 2024
Response via : Initial Calibration

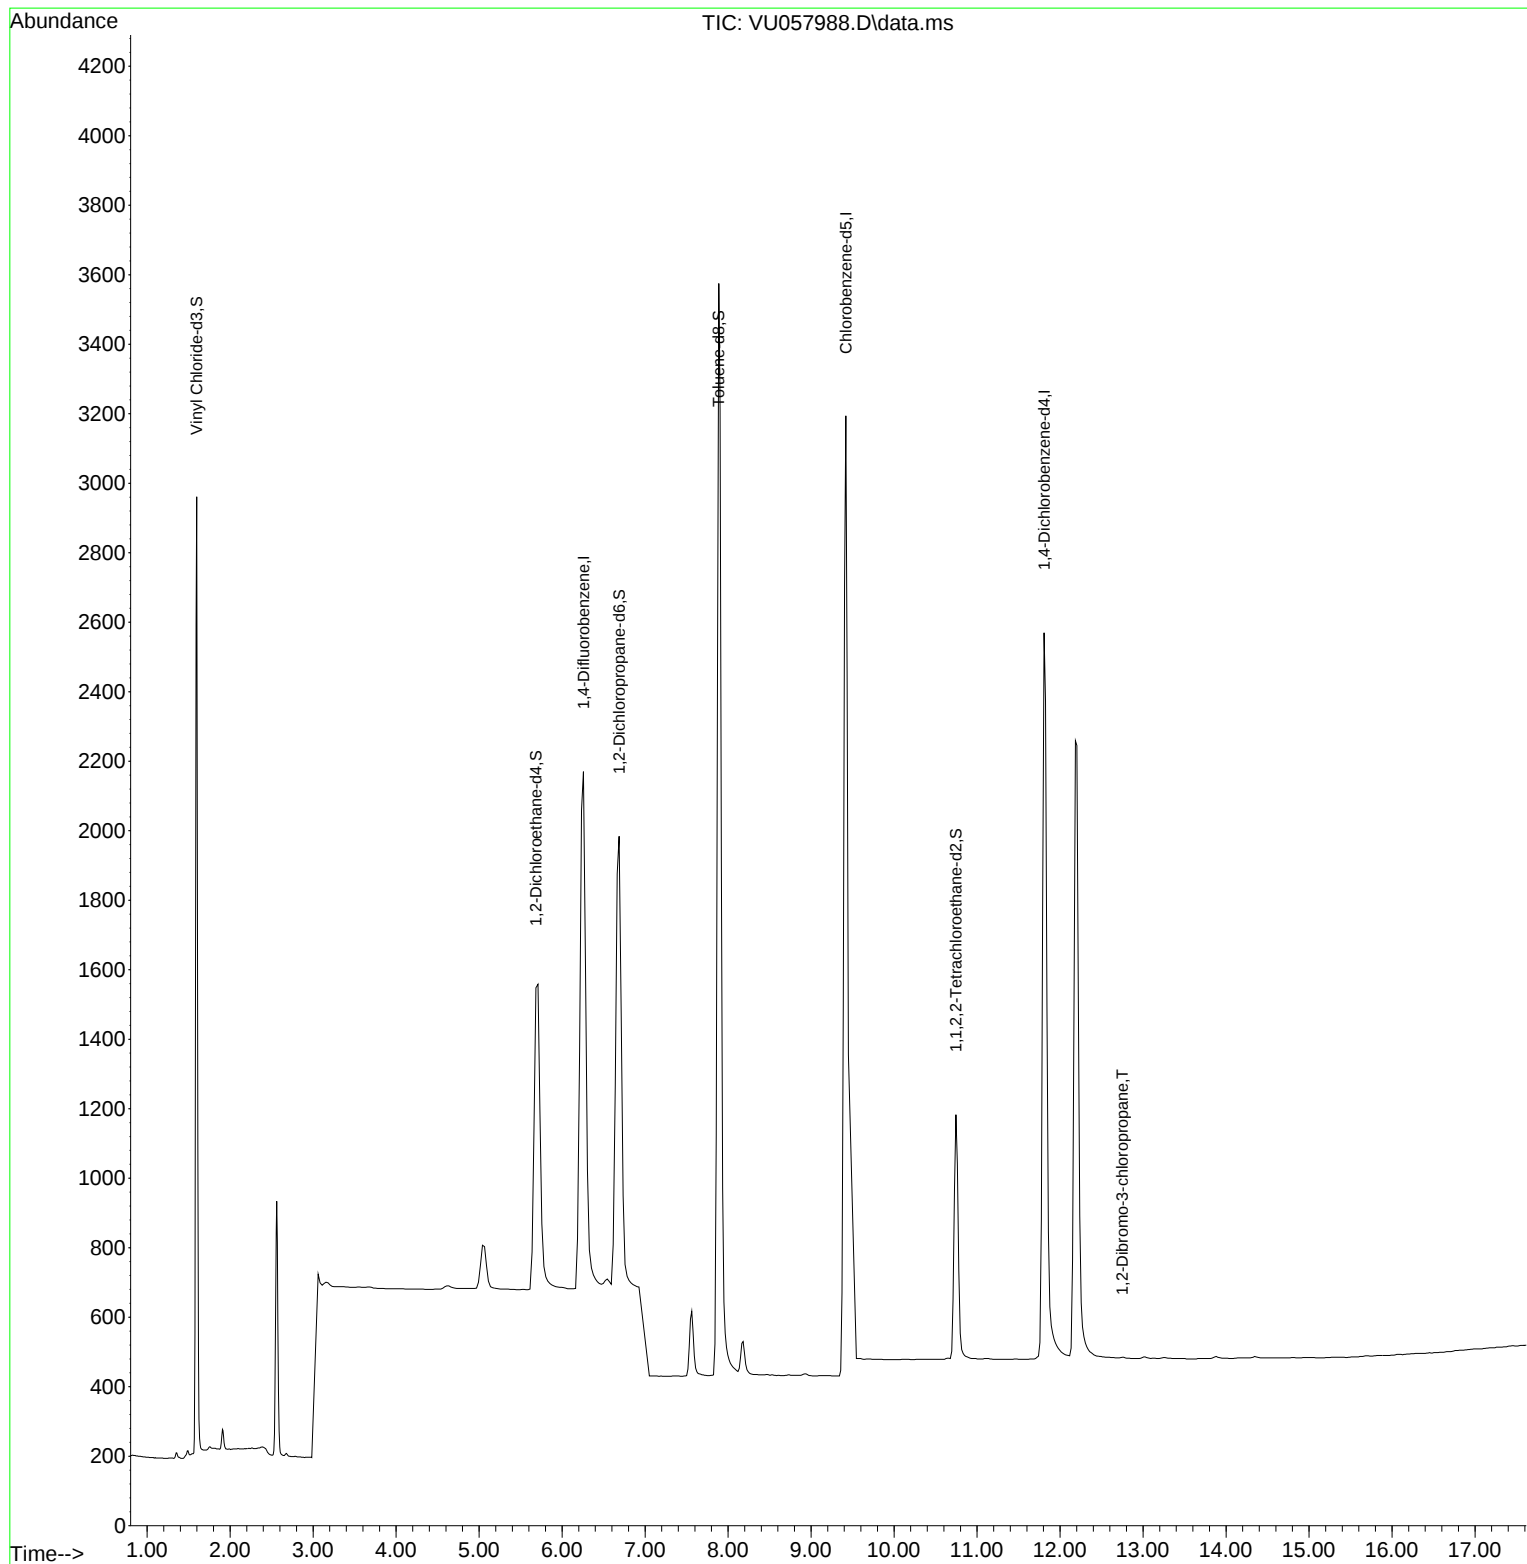

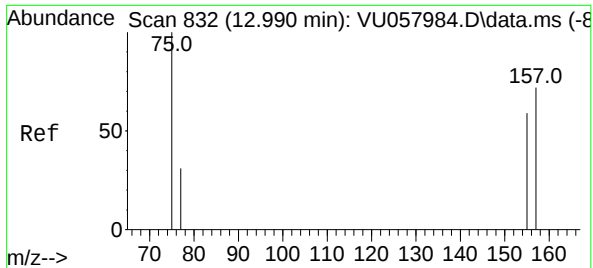

#13
1,2-Dibromo-3-chloropropane
Concen: 0.043 ug/L
RT: 12.750 min Scan# 81
Delta R.T. -0.240 min
Lab File: VU057988.D
Acq: 05 Mar 2024 13:31

Instrument :
MSVOA_U
ClientSampleId :

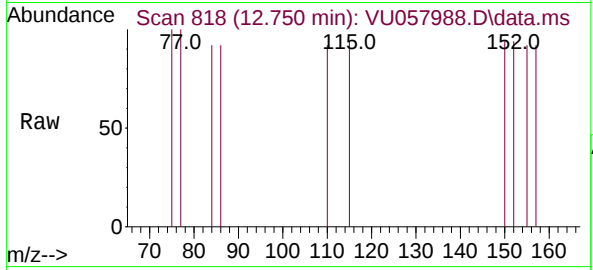

Tgt Ion: 75 Resp: 16

Ion	Ratio	Lower	Upper
75	100		
157	92.2	66.6	100.0
155	92.2	62.0	93.0

