


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030524\
Data File : VU057981.D
Acq On : 05 Mar 2024 09:01
Operator : MD/SY
Sample : BFB001
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB001

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM030524.M
Title : TRACE VOA SOM01.0
Last Update : Wed Mar 06 01:33:52 2024

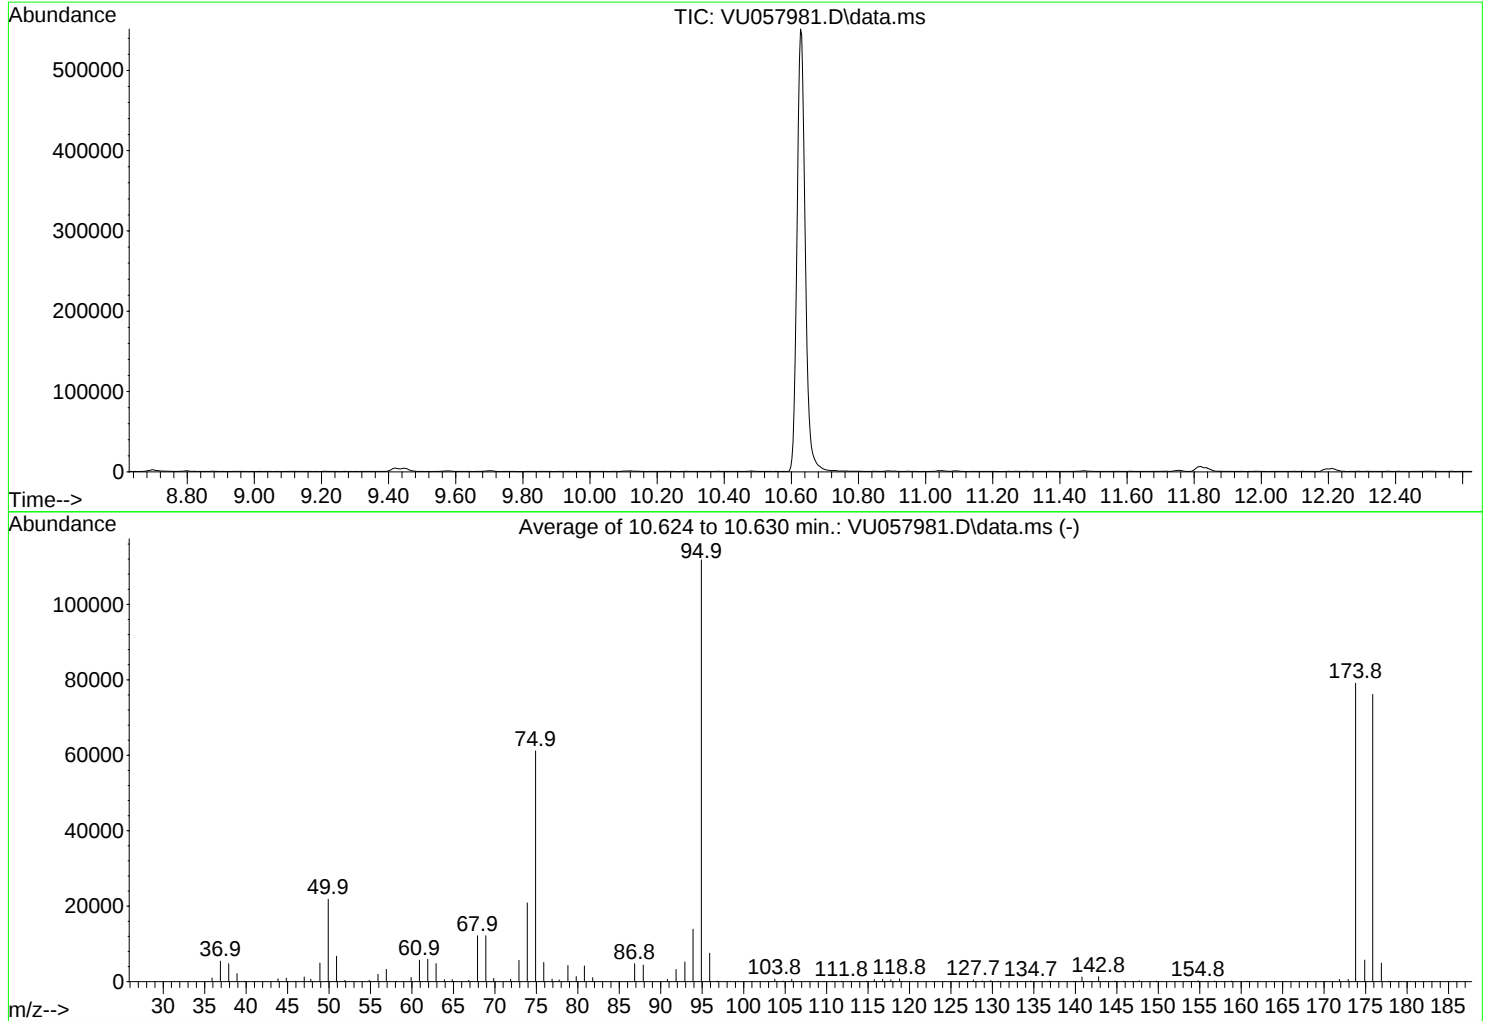

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	21824	PASS
75	95	30	80	54.7	61176	PASS
95	95	100	100	100.0	111805	PASS
96	95	5	9	6.7	7539	PASS
173	174	0.00	2	0.7	577	PASS
174	95	50	120	70.7	79088	PASS
175	174	5	9	7.2	5724	PASS
176	174	95	101	96.2	76112	PASS
177	176	5	9	6.4	4904	PASS

Scan 2890 (10.582 min): VU057981.D\data.ms
BFB001

m/z	Abundance
39.90	239.0
43.80	312.0

Instrument :
MSVOA_U
ClientSampleId :
BFB001

m/z	Abundance
35.90	916.0
36.90	5205.0
37.90	4707.0
38.90	2040.0
39.80	368.0
43.90	1045.0
44.80	950.0
45.90	117.0
47.00	1153.0
47.80	740.0
48.90	4870.0
49.90	21104.0
50.90	6543.0
51.90	354.0
54.80	264.0
55.90	1886.0
56.90	3137.0
59.90	1140.0
60.90	5580.0
61.90	5970.0
62.90	4602.0
63.90	442.0
64.80	511.0
66.90	374.0
67.90	11685.0
68.90	11624.0
69.80	837.0
71.90	564.0
72.90	5423.0
73.90	20008.0
74.90	59024.0
75.90	4918.0
76.90	626.0
77.80	467.0
78.80	4060.0
79.80	1210.0
80.80	4220.0
81.80	1103.0
86.80	4784.0
87.90	4109.0
90.80	593.0
91.90	3293.0
92.90	4997.0
93.90	13602.0
94.90	106600.0
95.90	7441.0
96.80	133.0
103.80	603.0
104.80	177.0
105.80	626.0
106.80	109.0
111.80	147.0
112.90	130.0
114.80	143.0
115.70	549.0
116.70	659.0
117.80	504.0
118.80	700.0
127.70	484.0
128.70	263.0
129.90	303.0
130.60	141.0
134.70	159.0
136.80	159.0
139.80	114.0
140.80	1044.0
142.80	1215.0
143.80	116.0
144.80	190.0
145.80	149.0
147.70	232.0
149.80	156.0
154.80	238.0
156.80	173.0
158.80	178.0
160.70	124.0
171.80	657.0
172.90	525.0
173.80	73872.0
174.90	5510.0
175.80	71504.0
176.90	4671.0
177.80	138.0

Instrument :
MSVOA_U
ClientSampleId :
BFB001

m/z	Abundance
35.90	971.0
36.90	5556.0
37.90	4851.0
38.90	2192.0
39.80	393.0
43.90	1098.0
44.90	975.0
45.90	142.0
47.00	1263.0
47.80	634.0
48.90	5076.0
49.90	22472.0
50.90	6886.0
51.90	353.0
54.90	356.0
55.90	2034.0
56.90	3380.0
58.10	120.0
59.90	1143.0
60.90	5858.0
61.90	6094.0
62.90	4937.0
63.90	534.0
64.80	548.0
66.80	360.0
67.90	12435.0
68.90	12603.0
69.80	872.0
71.90	649.0
72.90	5833.0
73.90	21536.0
74.90	62992.0
75.90	5226.0
76.90	695.0
77.70	483.0
78.80	4402.0
79.80	1405.0
80.80	4220.0
81.80	1109.0
82.80	122.0
86.80	4876.0
87.90	4583.0
90.80	632.0
91.80	3293.0
92.90	5352.0
93.90	14398.0
94.90	114984.0
95.90	7694.0
96.80	145.0
103.80	697.0
104.70	190.0
105.80	654.0
110.70	105.0
111.80	153.0
112.90	122.0
114.80	145.0
115.80	549.0
116.70	657.0
117.80	544.0
118.80	807.0
127.70	493.0
128.80	242.0
129.80	313.0
130.70	158.0
134.60	167.0
136.90	180.0
140.80	1301.0
142.80	1387.0
144.80	169.0
145.90	158.0
146.90	100.0
147.70	269.0
149.70	170.0
154.80	260.0
156.80	176.0
158.80	171.0
160.70	156.0
171.80	591.0
172.90	575.0
173.80	81592.0
174.90	5920.0
175.90	78312.0
176.90	5073.0
177.80	149.0

Instrument :
MSVOA_U
ClientSampleId :
BFB001

m/z	Abundance
35.90	1024.0
36.90	5519.0
37.90	4719.0
38.90	2162.0
39.80	381.0
43.90	1028.0
44.90	888.0
45.90	149.0
47.00	1219.0
47.80	580.0
48.90	4882.0
49.90	21896.0
50.90	6750.0
51.90	330.0
54.90	404.0
55.90	1961.0
56.90	3313.0
58.10	136.0
59.90	1097.0
60.90	5627.0
61.90	5699.0
62.90	4857.0
63.90	574.0
64.90	537.0
66.80	329.0
67.90	12354.0
68.90	12317.0
69.90	835.0
71.90	675.0
72.90	5724.0
73.90	21096.0
74.90	61512.0
75.90	5091.0
76.90	696.0
77.70	445.0
78.80	4370.0
79.80	1447.0
80.80	4058.0
81.80	1038.0
82.80	137.0
86.90	4626.0
87.90	4502.0
90.80	586.0
91.80	3045.0
92.90	5332.0
93.90	13804.0
94.90	113832.0
95.90	7481.0
96.80	184.0
103.70	725.0
104.70	187.0
105.80	631.0
109.70	111.0
110.70	130.0
111.80	139.0
114.80	151.0
115.80	539.0
116.80	634.0
117.70	541.0
118.80	847.0
127.70	435.0
128.80	190.0
129.70	342.0
130.80	139.0
134.70	179.0
136.90	199.0
140.80	1374.0
141.70	119.0
142.80	1353.0
144.80	135.0
145.90	188.0
147.70	263.0
149.70	153.0
154.80	220.0
156.80	136.0
158.80	144.0
160.70	152.0
171.90	534.0
172.90	631.0
173.80	81800.0
174.90	5743.0
175.90	78520.0
176.90	4969.0
177.80	143.0

Instrument :
MSVOA_U
ClientSampleId :
BFB001