


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030619\
 Data File : VU029822.D
 Acq On : 05 Mar 2019 15:03
 Operator : JC/SP
 Sample : BFB56
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB56

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR022119WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Mar 06 02:51:24 2019

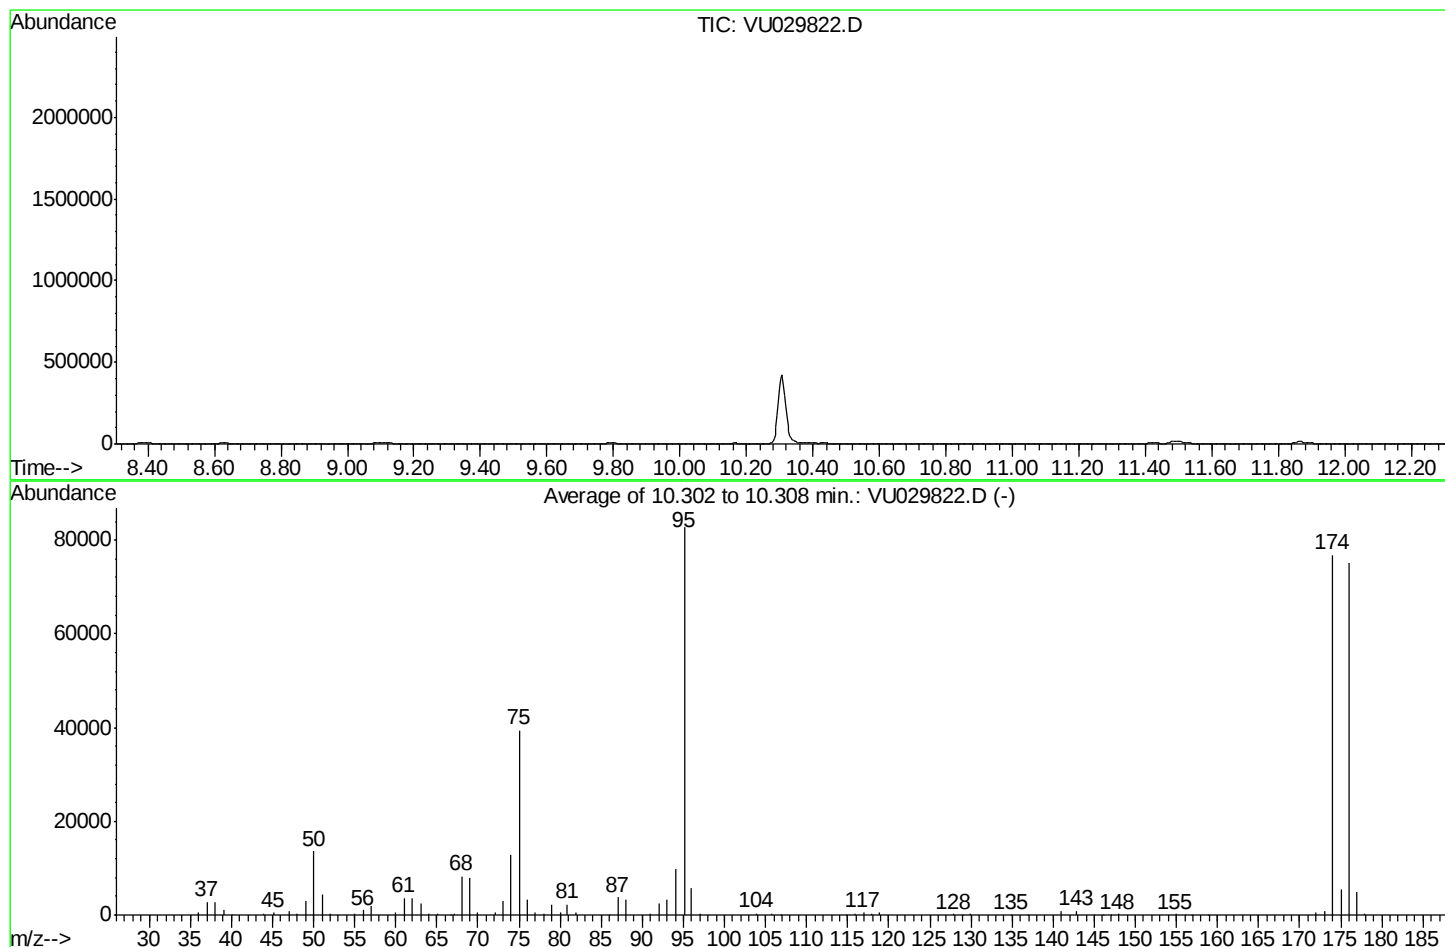

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2852

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	13571	PASS
75	95	30	80	47.7	39440	PASS
95	95	100	100	100.0	82730	PASS
96	95	5	9	7.1	5864	PASS
173	174	0.00	2	1.0	803	PASS
174	95	50	120	92.9	76842	PASS
175	174	5	9	7.3	5575	PASS
176	174	95	101	97.8	75146	PASS
177	176	5	9	6.6	4970	PASS

m/z	Abundance
36.00	569.0
37.00	2851.0
38.10	2628.0
39.10	1183.0
40.00	2239.0
43.90	779.0
45.10	481.0
47.00	623.0
48.00	293.0
49.00	2877.0
50.00	13158.0
51.00	4364.0
52.00	221.0
55.00	217.0
56.00	1016.0
57.00	1849.0
60.00	758.0
61.00	3413.0
62.00	3395.0
63.00	2382.0
64.00	338.0
65.10	347.0
66.70	150.0
67.10	164.0
68.00	8145.0
69.00	8015.0
70.00	638.0
72.00	412.0
73.00	3054.0
74.00	12539.0
75.00	38328.0
76.00	3327.0
77.00	443.0
78.00	362.0
78.90	2047.0
80.00	647.0
80.90	2142.0
81.90	412.0
86.00	153.0
87.00	3760.0
88.00	3206.0
90.90	303.0
92.00	2344.0
93.00	3205.0
94.00	9510.0
95.10	79944.0
96.00	5750.0
97.10	163.0
103.90	375.0
105.80	276.0
106.90	121.0
114.80	119.0
115.90	246.0
116.90	433.0
117.80	328.0
118.90	462.0
127.90	243.0
130.00	209.0
134.90	124.0
136.90	136.0
140.90	795.0
142.90	857.0
144.90	106.0
147.90	159.0
155.00	164.0
156.90	160.0
171.90	585.0
172.90	726.0
174.00	73520.0
175.00	5384.0
176.00	72040.0
177.00	4651.0
177.90	190.0
207.00	153.0

Instrument :
MSVOA_U
ClientSampleId :
BFB56

m/z	Abundance
36.00	531.0
37.00	2893.0
38.00	2956.0
39.00	1163.0
40.00	2315.0
43.90	831.0
45.10	517.0
47.00	764.0
48.00	337.0
49.00	3169.0
50.00	13993.0
51.00	4554.0
52.00	212.0
55.00	217.0
56.00	1044.0
57.00	2025.0
60.00	709.0
61.00	3777.0
62.00	3696.0
63.00	2622.0
64.10	376.0
65.10	307.0
67.10	221.0
68.00	8702.0
69.00	8322.0
70.00	697.0
72.10	446.0
73.00	3192.0
74.00	13288.0
75.00	40848.0
76.00	3542.0
77.00	479.0
78.00	337.0
78.90	2208.0
80.00	721.0
80.90	2284.0
81.90	444.0
87.00	3970.0
88.00	3604.0
90.90	286.0
92.00	2532.0
93.00	3353.0
94.00	10281.0
95.10	85632.0
96.00	6164.0
97.00	199.0
103.90	370.0
105.80	293.0
106.90	150.0
115.90	259.0
116.90	476.0
117.90	390.0
118.90	457.0
127.90	254.0
128.90	121.0
130.00	264.0
135.00	155.0
136.90	131.0
140.90	824.0
142.90	944.0
145.00	152.0
146.10	130.0
147.10	114.0
147.90	223.0
155.00	196.0
156.00	105.0
156.90	150.0
158.80	161.0
172.00	651.0
173.00	824.0
174.00	79264.0
175.00	5724.0
176.00	77688.0
177.00	5069.0
177.90	193.0
207.00	164.0

Instrument :
MSVOA_U
ClientSampleId :
BFB56

m/z	Abundance
36.00	466.0
37.00	2765.0
38.00	2894.0
39.00	1054.0
40.00	2413.0
44.00	806.0
45.10	507.0
47.00	919.0
48.00	344.0
49.00	3045.0
50.00	13564.0
51.00	4458.0
52.00	156.0
55.00	197.0
56.00	952.0
57.00	1966.0
59.90	603.0
61.00	3759.0
62.00	3503.0
63.00	2667.0
64.10	365.0
65.00	248.0
67.10	253.0
68.00	8169.0
69.00	7595.0
70.00	657.0
72.10	406.0
73.00	3118.0
74.00	12742.0
75.00	39144.0
76.00	3387.0
76.90	490.0
78.00	269.0
79.00	2185.0
80.00	692.0
80.90	2273.0
81.90	464.0
87.00	3752.0
88.00	3403.0
90.90	252.0
92.00	2363.0
93.00	3265.0
94.00	9722.0
95.10	82616.0
96.00	5678.0
97.00	165.0
103.90	334.0
105.80	343.0
106.90	154.0
115.90	216.0
116.90	517.0
117.90	379.0
118.90	437.0
127.90	275.0
128.90	122.0
129.90	295.0
134.90	164.0
136.90	127.0
141.00	839.0
142.90	934.0
145.00	182.0
146.00	129.0
147.90	237.0
154.90	196.0
156.00	112.0
156.90	123.0
158.80	175.0
172.00	631.0
173.10	861.0
174.00	77744.0
175.00	5617.0
176.00	75712.0
177.00	5192.0
177.80	185.0
207.10	191.0

Instrument :
MSVOA_U
ClientSampleId :
BFB56

m/z	Abundance
40.00	2228.0
44.00	469.0
207.00	226.0

Instrument :
MSVOA_U
ClientSampleId :
BFB56