

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU030620\
 Data File : VU037104.D
 Acq On : 06 Mar 2020 13:14
 Operator : JC/MD
 Sample : L1780-20
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Quant Time: Mar 07 01:21:43 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 06 23:54:55 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	262014	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	248627	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	85931	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	92706	42.13	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	84.26%
7) Chloroethane-d5	1.93	69	85592	47.01	ug/L	0.02
Spiked Amount	50.000	Range	70 - 130	Recovery	=	94.02%
11) 1,1-Dichloroethene-d2	2.59	63	122513	33.25	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	66.50%
21) 2-Butanone-d5	4.67	46	136783	92.68	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	92.68%
24) Chloroform-d	5.11	84	154881	46.10	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.20%
26) 1,2-Dichloroethane-d4	5.74	65	106374	46.78	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.56%
32) Benzene-d6	5.76	84	332009	46.18	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.36%
36) 1,2-Dichloropropane-d6	6.72	67	110283	47.34	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	94.68%
41) Toluene-d8	7.92	98	297222	44.56	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	89.12%
43) trans-1,3-Dichloropropene-	8.20	79	44120	40.76	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	81.52%
47) 2-Hexanone-d5	8.66	63	92336	81.07	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	81.07%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	147812	45.01	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	90.02%
64) 1,2-Dichlorobenzene-d4	12.21	152	83965	49.98	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	99.96%

Target Compounds


					Ovalue
63) 1,4-Dichlorobenzene	11.85	146	5453	1.980 ug/L	97
65) 1,2-Dichlorobenzene	12.23	146	4845	1.741 ug/L	92
68) 1,2,4-trichlorobenzene	13.87	180	1565	1.181 ug/L #	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU030620\
Data File : VU037104.D
Acq On : 06 Mar 2020 13:14
Operator : JC/MD
Sample : L1780-20
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Time: Mar 07 01:21:43 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 06 23:54:55 2020
Response via : Initial Calibration




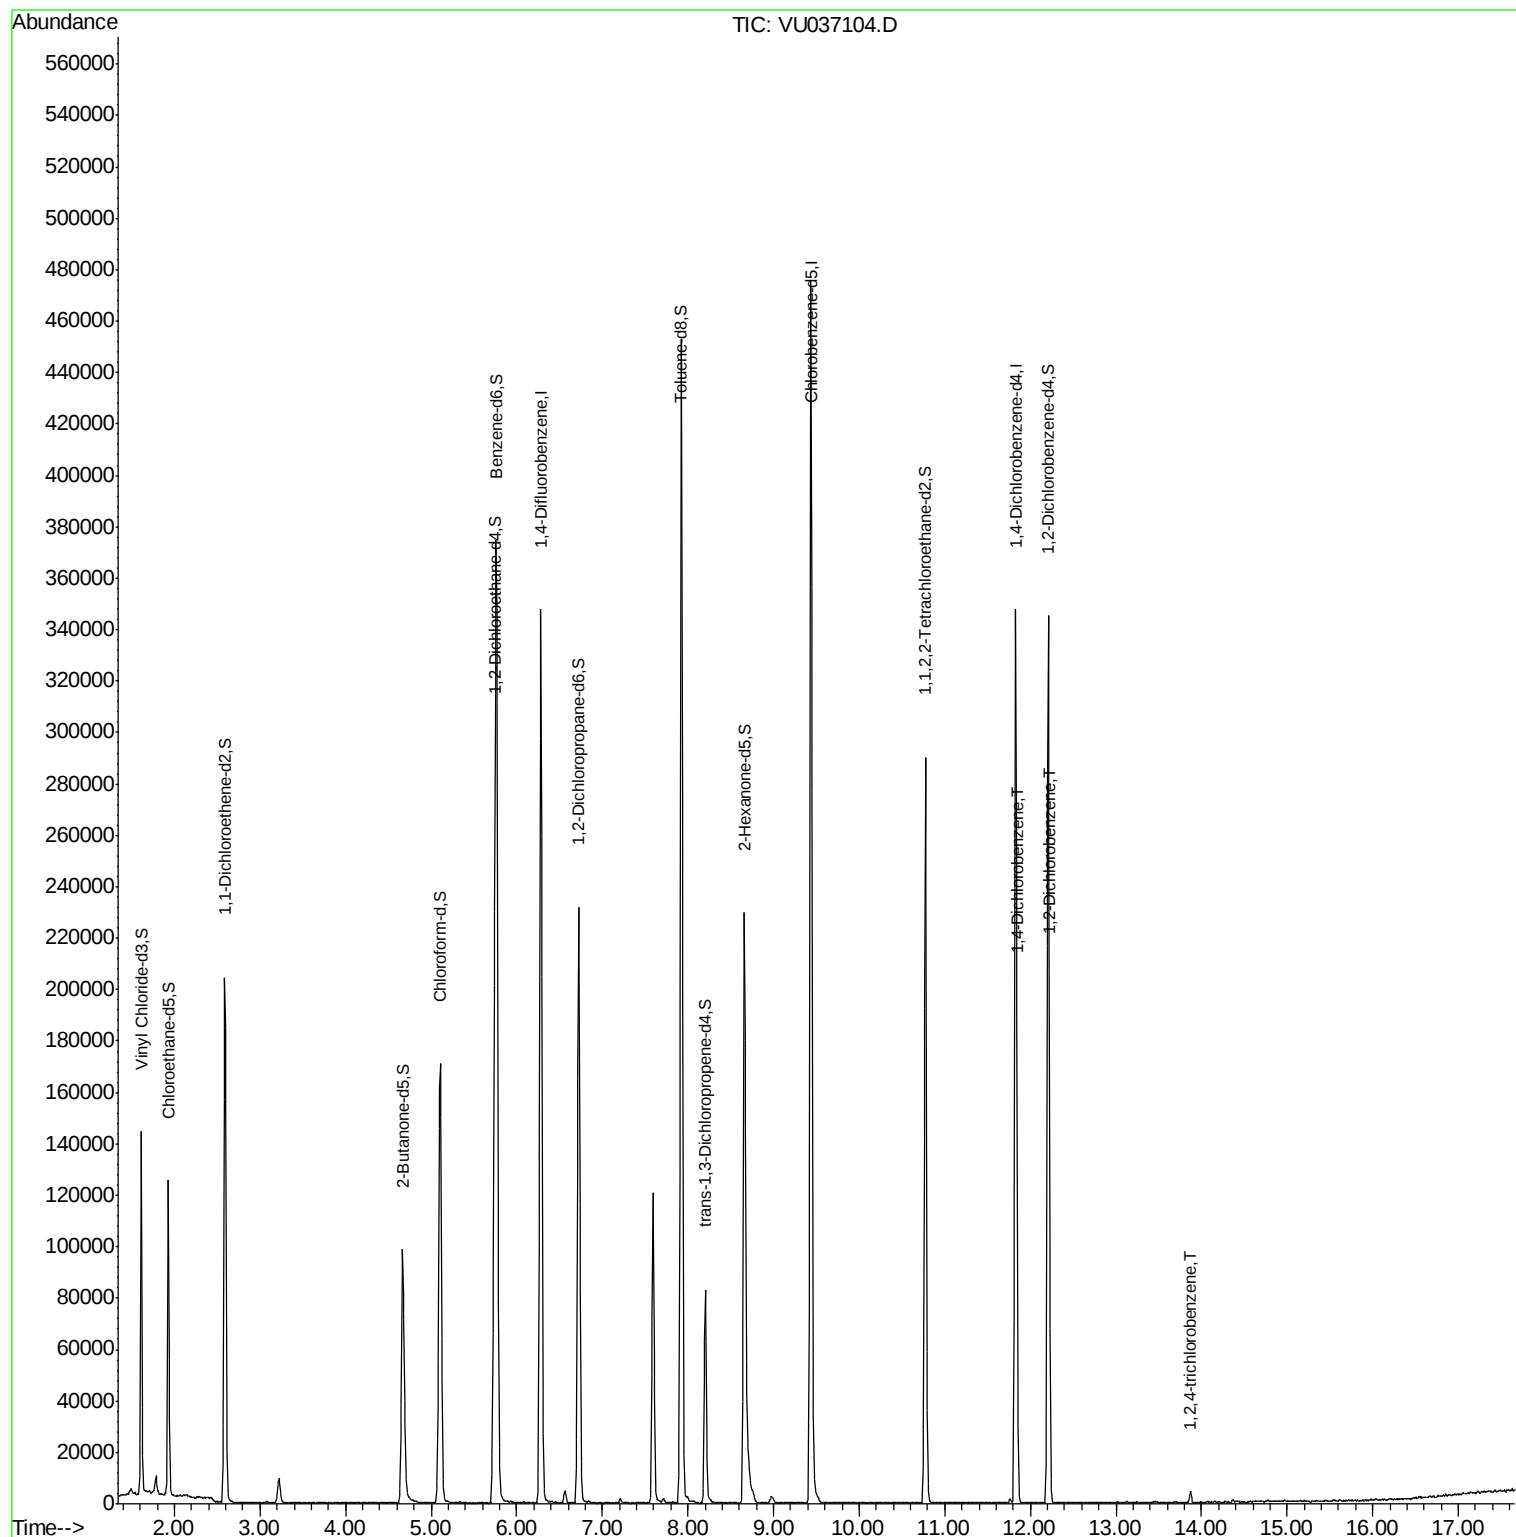


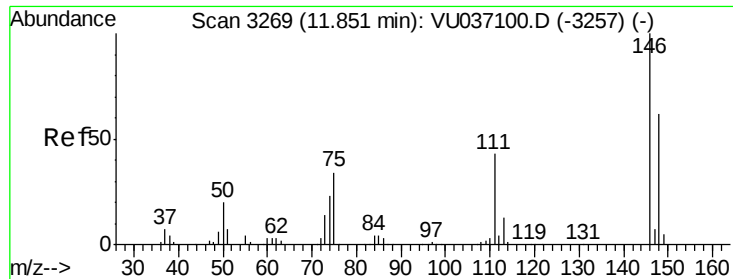

#63
 1,4-Dichlorobenzene
 Concen: 1.980 ug/L
 RT: 11.85 min Scan# 3269
 Delta R.T. 0.00 min
 Lab File: VU037104.D
 Acq: 06 Mar 2020 13:14




Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01


Tot Ion:146 Resp: 5453
 Ion Ratio Lower Upper
 146 100
 111 43.8 29.8 55.4
 148 61.7 45.1 83.9

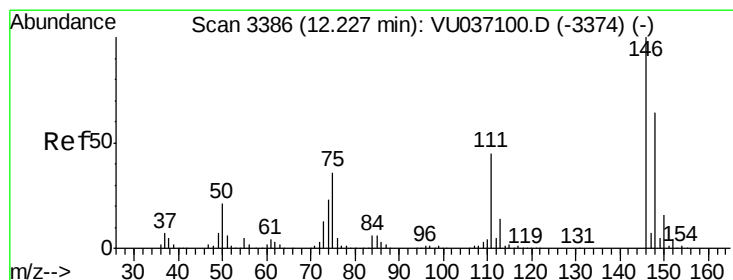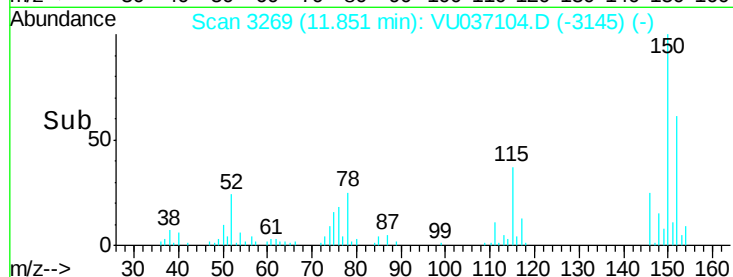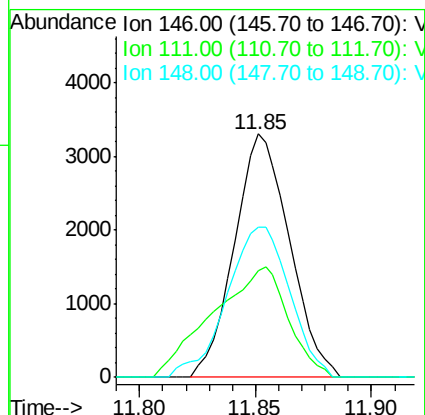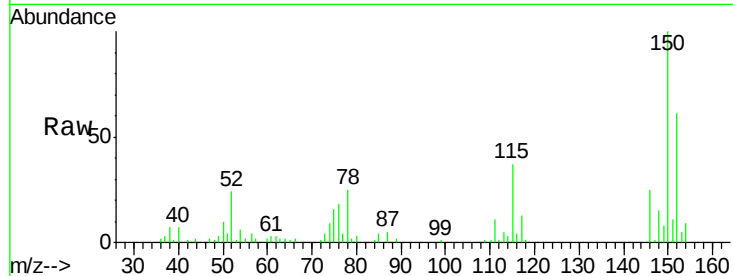

#65
 1,2-Dichlorobenzene
 Concen: 1.741 ug/L
 RT: 12.23 min Scan# 3387
 Delta R.T. 0.00 min
 Lab File: VU037104.D
 Acq: 06 Mar 2020 13:14

Tgt Ion:146 Resp: 4845
 Ion Ratio Lower Upper
 146 100
 111 50.3 35.4 53.0
 148 68.3 50.5 75.7

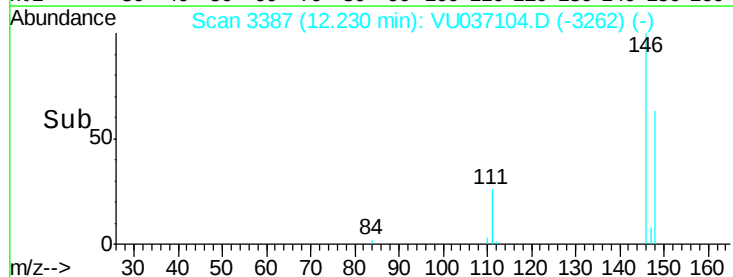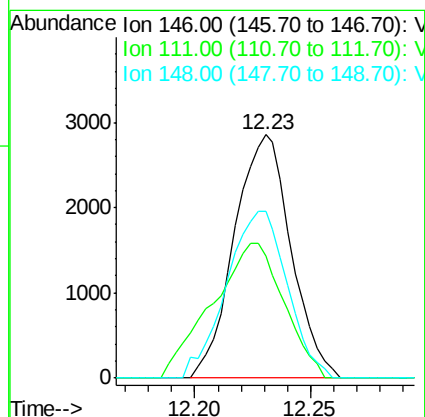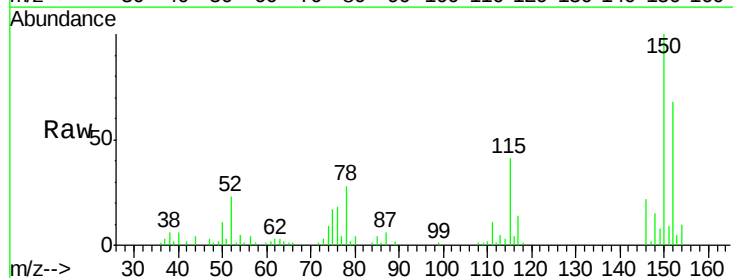

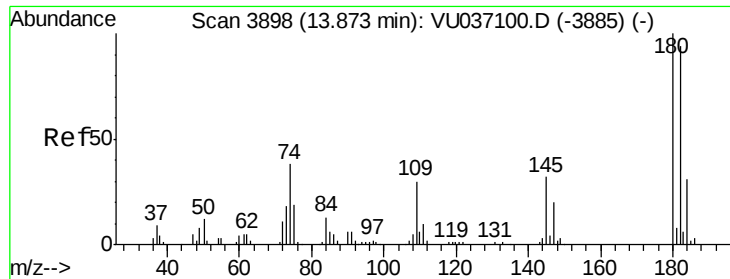

#68

1,2,4-trichlorobenzene

Concen: 1.181 ug/L

RT: 13.87 min Scan# 3898

Delta R.T. 0.00 min

Lab File: VU037104.D

Acq: 06 Mar 2020 13:14

Instrument :

MSVOA_U

ClientSampleId :

VHBLK01


Tot Ion:180 Resp: 1565

Ion Ratio Lower Upper

180 100

182 91.5 75.3 112.9

145 19.8 26.2 39.4#

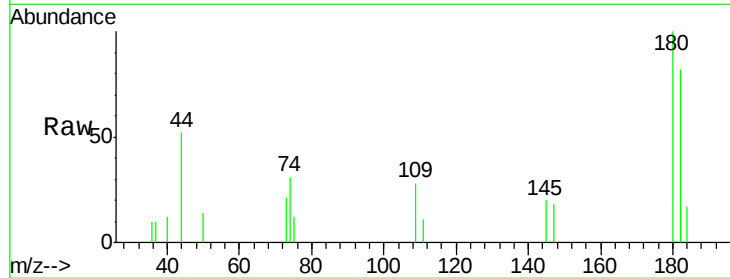

Abundance Ion 180.00 (179.70 to 180.70): V

Ion 182.00 (181.70 to 182.70): V

Ion 145.00 (144.70 to 145.70): V

