

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030624\
 Data File : VU057993.D
 Acq On : 06 Mar 2024 09:36
 Operator : MD/SY
 Sample : VU0306WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Mar 07 03:35:51 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM030524.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Mar 06 01:33:52 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.258	114	5175	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.419	117	7555	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.808	152	2321	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.597	65	3087	0.511	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	102.000%
4) 1,2-Dichloroethane-d4	5.685	65	1857	0.518	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	104.000%
7) 1,2-Dichloropropane-d6	6.687	67	2279	0.553	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	110.000%
8) Toluene-d8	7.888	98	5809	0.515	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	102.000%
10) 1,1,2,2-Tetrachloroeth...	10.746	84	1414	0.544	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	108.000%
Target Compounds						
13) 1,2-Dibromo-3-chloropr...	12.751	75	19	0.050	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030624\
Data File : VU057993.D
Acq On : 06 Mar 2024 09:36
Operator : MD/SY
Sample : VU0306WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: Mar 07 03:35:51 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM030524.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Mar 06 01:33:52 2024
Response via : Initial Calibration

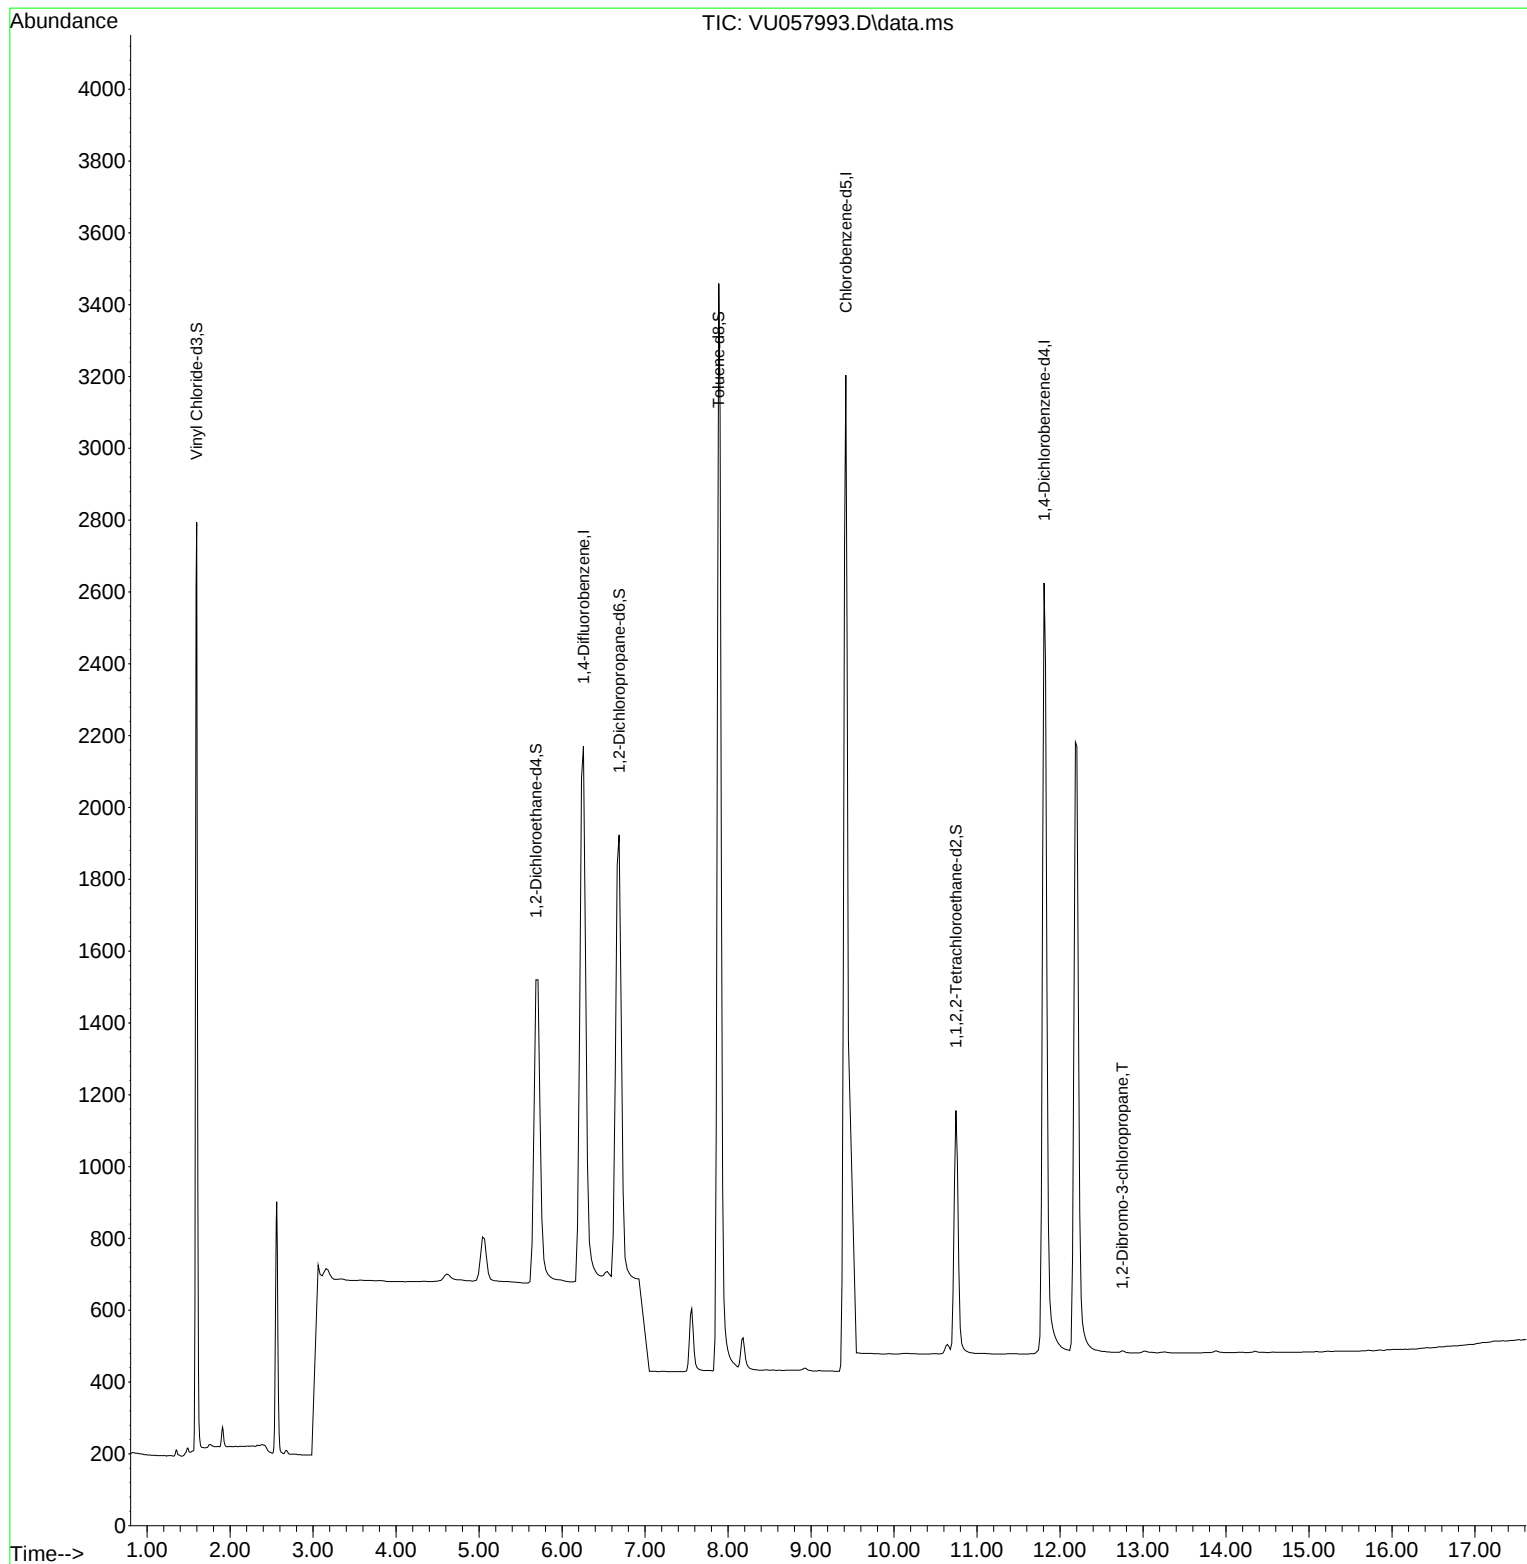

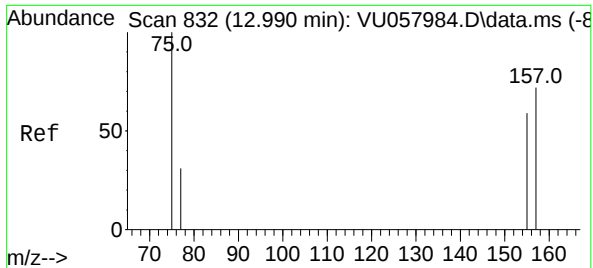

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.050 ug/L
 RT: 12.751 min Scan# 81
 Delta R.T. -0.239 min
 Lab File: VU057993.D
 Acq: 06 Mar 2024 09:36

Instrument :
 MSVOA_U
 ClientSampleId :

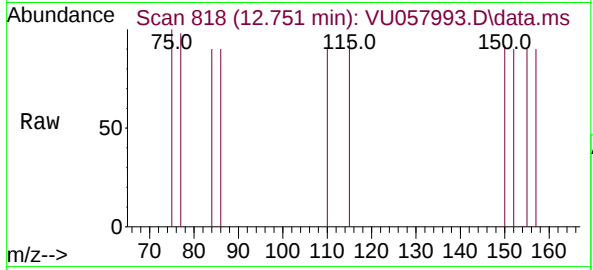

Tgt Ion: 75 Resp: 19

Ion	Ratio	Lower	Upper
75	100		
157	90.4	66.6	100.0
155	90.4	62.0	93.0

