


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030624\
Data File : VU057991.D
Acq On : 06 Mar 2024 08:32
Operator : MD/SY
Sample : BFB002
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB002

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM030524.M
Title : TRACE VOA SOM01.0
Last Update : Wed Mar 06 01:33:52 2024

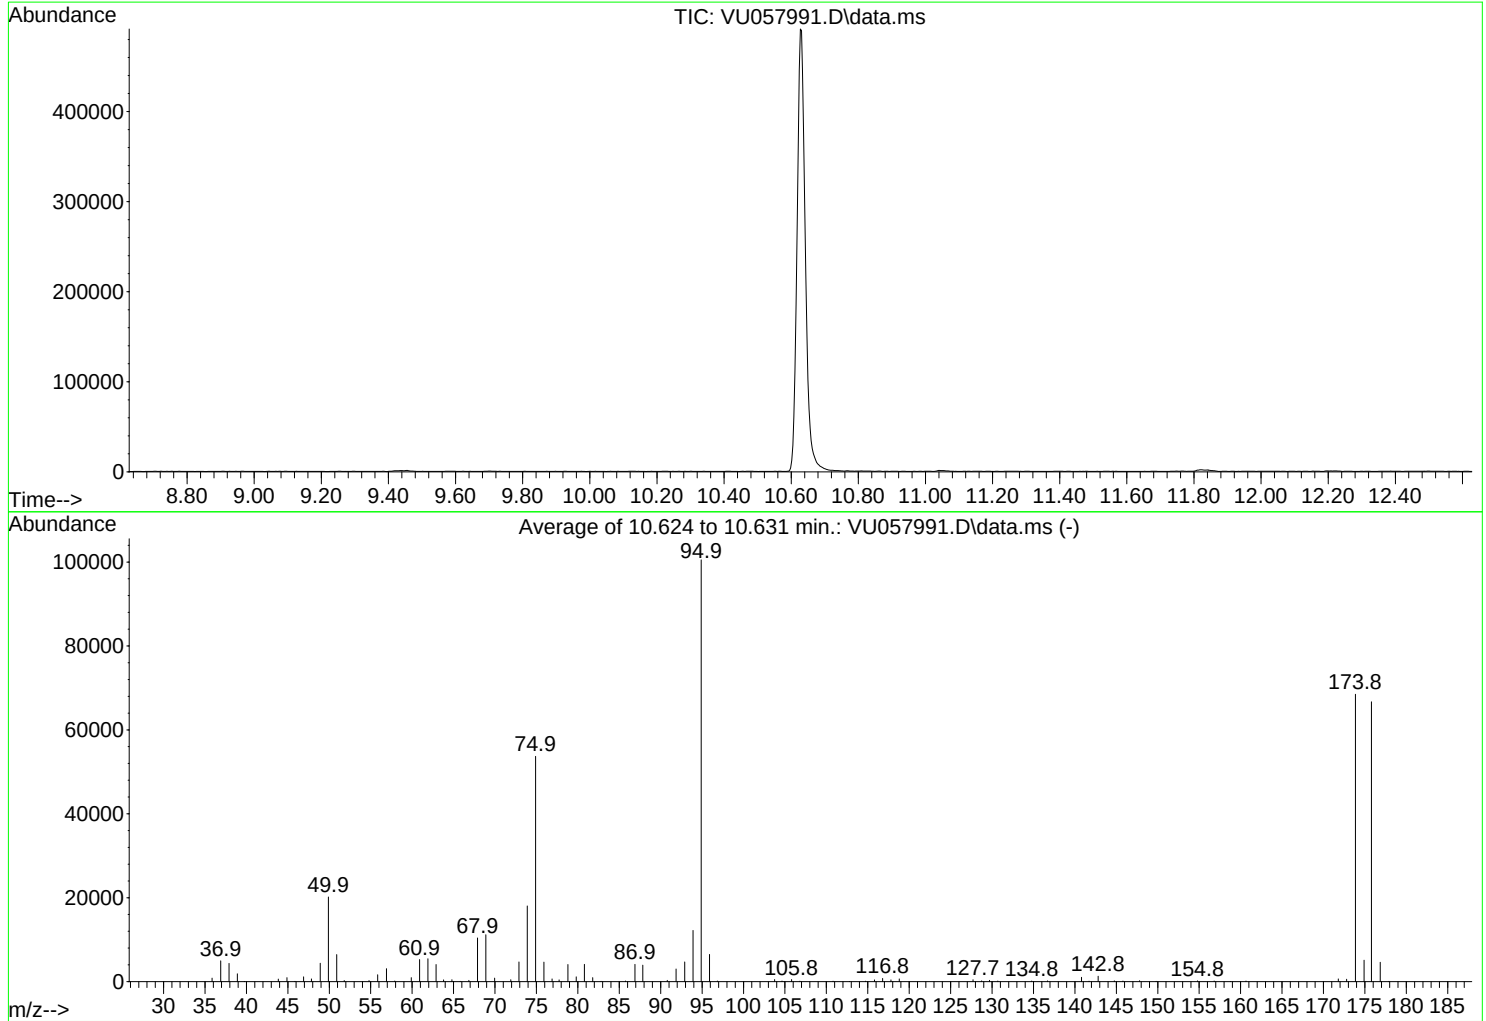

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2891

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.1	20189	PASS
75	95	30	80	53.4	53693	PASS
95	95	100	100	100.0	100525	PASS
96	95	5	9	6.5	6500	PASS
173	174	0.00	2	0.8	573	PASS
174	95	50	120	68.1	68491	PASS
175	174	5	9	7.4	5095	PASS
176	174	95	101	97.4	66693	PASS
177	176	5	9	6.9	4608	PASS

m/z	Abundance
39.70	258.0
43.80	369.0

Instrument :
MSVOA_U
ClientSampleId :
BFB002

m/z	Abundance
35.90	852.0
36.90	4551.0
37.90	4326.0
38.90	1788.0
39.80	296.0
43.90	919.0
44.90	848.0
45.80	109.0
46.90	1081.0
47.80	563.0
48.90	4353.0
49.90	19272.0
50.90	6104.0
51.80	257.0
54.80	276.0
55.80	1613.0
56.90	2923.0
57.90	128.0
59.90	909.0
60.90	5104.0
61.90	5229.0
62.90	3917.0
63.80	407.0
64.80	446.0
66.80	274.0
67.90	9970.0
68.90	10573.0
69.90	802.0
71.90	425.0
72.90	4530.0
73.90	16752.0
74.90	50648.0
75.90	4389.0
76.90	585.0
77.80	416.0
78.80	3710.0
79.80	1131.0
80.80	3913.0
81.80	848.0
85.80	147.0
86.90	3912.0
87.90	3837.0
90.80	286.0
91.90	2781.0
92.90	4501.0
93.90	11605.0
94.90	94600.0
95.90	6318.0
96.80	161.0
103.80	504.0
104.70	115.0
104.90	115.0
105.80	521.0
106.80	110.0
110.80	140.0
114.90	103.0
115.80	348.0
116.80	734.0
117.80	387.0
118.80	598.0
127.70	416.0
128.70	204.0
129.70	277.0
130.70	137.0
134.80	124.0
136.70	176.0
140.80	948.0
141.70	104.0
142.80	1213.0
144.70	151.0
145.80	129.0
147.80	203.0
154.90	180.0
156.80	170.0
160.60	149.0
171.80	561.0
172.80	550.0
173.80	63200.0
174.90	4734.0
175.80	61336.0
176.80	4139.0

Instrument :
MSVOA_U
ClientSampleId :
BFB002

m/z	Abundance
35.90	904.0
36.90	5167.0
37.90	4476.0
38.90	1952.0
39.80	306.0
43.90	992.0
44.90	999.0
45.90	127.0
46.90	1206.0
47.80	699.0
48.90	4600.0
49.90	20848.0
50.90	6676.0
51.80	274.0
54.80	284.0
55.80	1696.0
56.90	3202.0
57.90	139.0
59.90	996.0
60.90	5437.0
61.90	5676.0
62.90	4267.0
63.80	418.0
64.80	483.0
65.80	103.0
66.80	333.0
67.90	10728.0
68.90	11632.0
70.00	887.0
71.90	456.0
72.90	4826.0
73.90	18592.0
74.90	55472.0
75.90	4797.0
76.90	680.0
77.70	436.0
78.80	4228.0
79.80	1171.0
80.80	4181.0
81.80	974.0
82.80	124.0
85.70	154.0
86.90	4309.0
87.90	4043.0
90.80	301.0
91.80	3147.0
92.90	4863.0
93.90	12625.0
94.90	103896.0
95.90	6680.0
96.80	178.0
103.70	496.0
104.70	144.0
105.80	516.0
106.80	131.0
110.80	130.0
114.70	112.0
115.80	423.0
116.80	825.0
117.80	432.0
118.80	675.0
127.70	488.0
128.70	213.0
129.70	302.0
130.70	158.0
134.80	157.0
136.70	206.0
140.80	1108.0
141.70	129.0
142.80	1348.0
144.70	172.0
145.80	161.0
147.80	226.0
149.80	118.0
154.80	167.0
156.80	183.0
158.80	103.0
160.70	153.0
171.80	671.0
172.80	573.0
173.80	70520.0
174.90	5245.0
175.80	68760.0
176.90	4793.0
177.90	125.0

Instrument :
MSVOA_U
ClientSampleId :
BFB002

m/z	Abundance
35.80	815.0
36.90	5115.0
37.90	4299.0
38.90	1891.0
39.80	324.0
43.90	987.0
44.90	997.0
46.90	1158.0
47.90	709.0
48.90	4229.0
49.90	20448.0
50.90	6538.0
51.80	278.0
54.80	276.0
55.90	1592.0
56.90	3102.0
57.90	164.0
59.90	1013.0
60.90	5262.0
61.90	5461.0
62.90	4107.0
63.80	416.0
64.80	477.0
65.80	109.0
66.90	332.0
67.90	10565.0
68.90	11329.0
69.90	841.0
71.90	499.0
72.90	4713.0
73.90	18832.0
74.90	54960.0
75.90	4799.0
76.90	687.0
77.80	457.0
78.80	4311.0
79.80	1144.0
80.80	4234.0
81.80	1001.0
82.80	162.0
85.70	133.0
86.90	4163.0
87.80	3901.0
90.80	346.0
91.80	3112.0
92.90	4742.0
93.90	12424.0
94.90	103080.0
95.90	6502.0
96.90	180.0
103.70	525.0
104.60	157.0
105.80	490.0
106.80	130.0
110.80	117.0
112.80	105.0
114.70	117.0
115.80	443.0
116.80	781.0
117.80	447.0
118.80	673.0
127.70	487.0
128.80	165.0
129.70	325.0
130.70	152.0
134.80	181.0
136.70	220.0
140.80	1075.0
141.70	151.0
142.80	1312.0
144.80	204.0
145.80	137.0
147.80	258.0
149.80	149.0
154.70	181.0
156.80	156.0
160.70	154.0
171.80	667.0
172.80	597.0
173.90	71752.0
174.90	5305.0
175.80	69984.0
176.90	4892.0
177.90	157.0

Instrument :
MSVOA_U
ClientSampleId :
BFB002