

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU030719\
Data File : VU029837.D
Acq On : 06 Mar 2019 13:40
Operator : JC/SP
Sample : VU0307WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0307WBL01

Quant Time: Mar 08 01:40:12 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U030719DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Fri Mar 08 00:30:10 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene	5.74	96	62882	1.00	ug/l	0.00

System Monitoring Compounds

57) 4-Bromofluorobenzene	10.31	95	18390	0.81	ug/l	0.00
Spiked Amount	1.000		Recovery	=	81.00%	
68) 1,2-Dichlorobenzene-d4	11.86	152	21386	0.82	ug/l	0.00
Spiked Amount	1.000		Recovery	=	82.00%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU030719\
Data File : VU029837.D
Acq On : 06 Mar 2019 13:40
Operator : JC/SP
Sample : VU0307WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0307WBL01

Quant Time: Mar 08 01:40:12 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\524U030719DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Fri Mar 08 00:30:10 2019
Response via : Initial Calibration

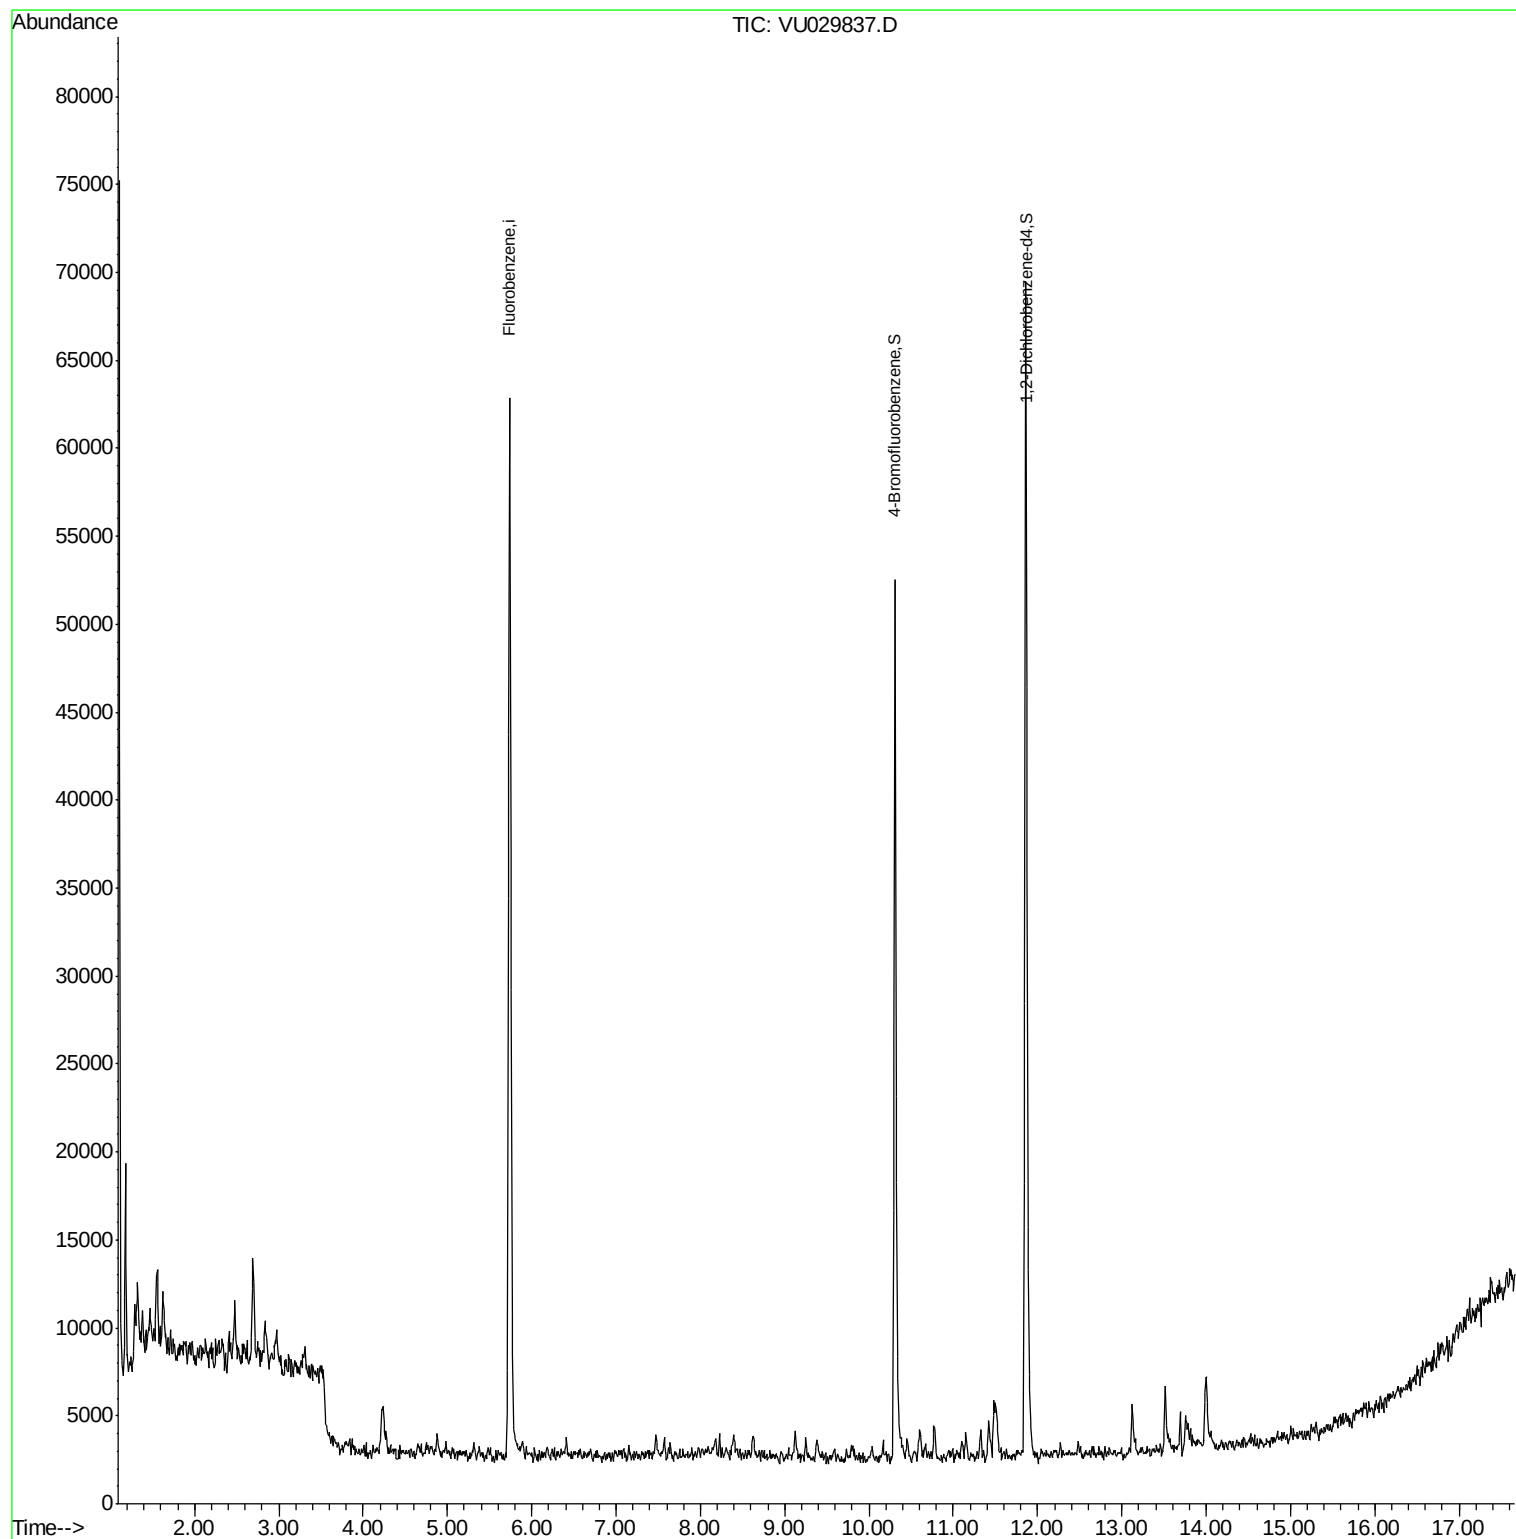

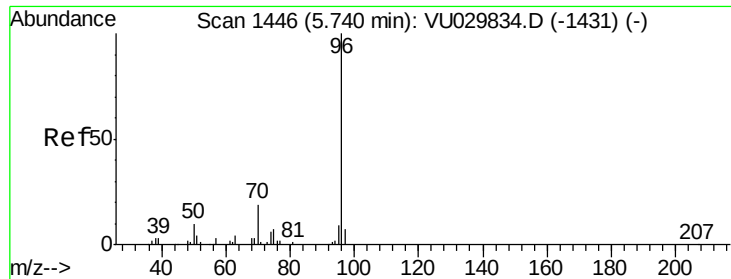

#1

Fluorobenzene

Concen: 1.000 ug/l

RT: 5.74 min Scan# 1445

Delta R.T. -0.00 min

Lab File: VU029837.D

Acq: 06 Mar 2019 13:40

Instrument :

MSVOA_U

ClientSampleId :

VU0307WBL01

Tgt Ion: 96 Resp: 62882


Ion Ratio Lower Upper

96 100

70 18.8 14.4 21.6

95 8.7 7.0 10.6

97 6.5 0.0 0.0#



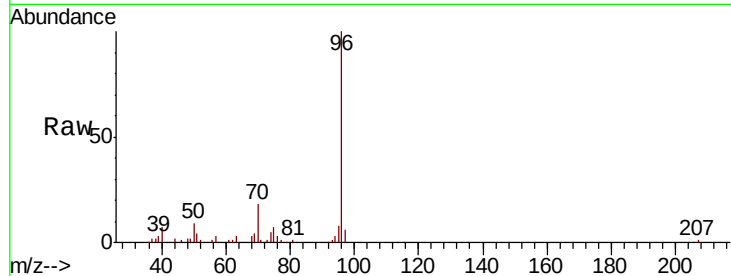


Abundance Ion 96.00 (95.70 to 96.70): VU0

Ion 70.00 (69.70 to 70.70): VU0

Ion 95.00 (94.70 to 95.70): VU0

Ion 97.00 (96.70 to 97.70): VU0

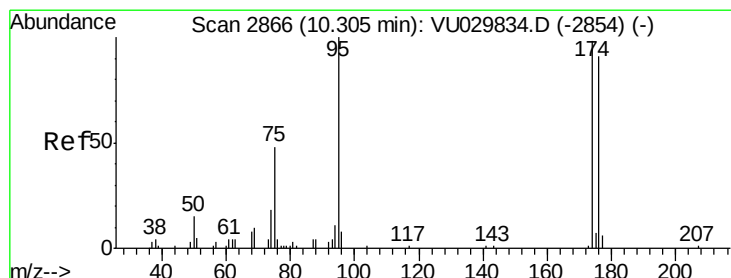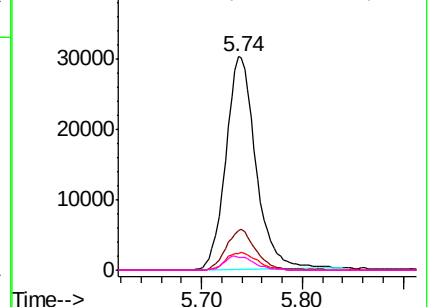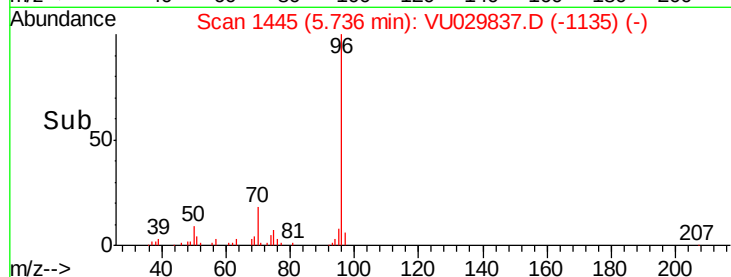

#57

4-Bromofluorobenzene

Concen: N.D. ug/l

RT: 10.31 min Scan# 2867

Delta R.T. 0.00 min

Lab File: VU029837.D

Acq: 06 Mar 2019 13:40


Tgt Ion: 95 Resp: 18390

Ion Ratio Lower Upper

95 100

174 93.3 76.5 114.7



176 95.6 74.2 111.2

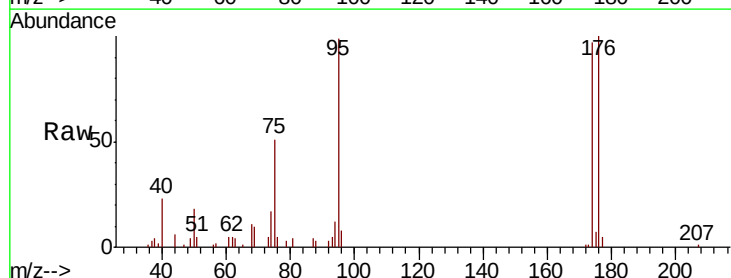


Abundance Ion 95.00 (94.70 to 95.70): VU0

Ion 174.00 (173.70 to 174.70): V

Ion 176.00 (175.70 to 176.70): V

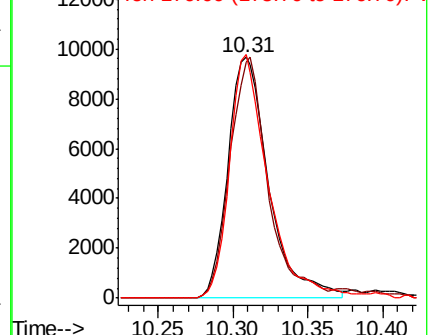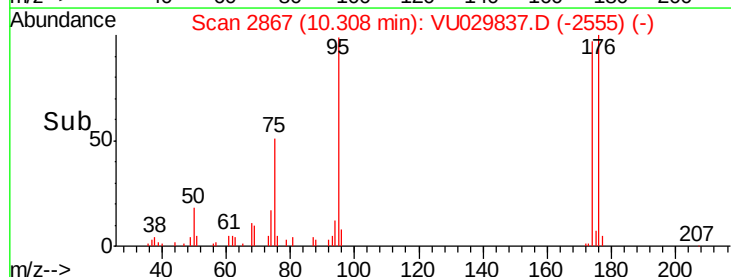

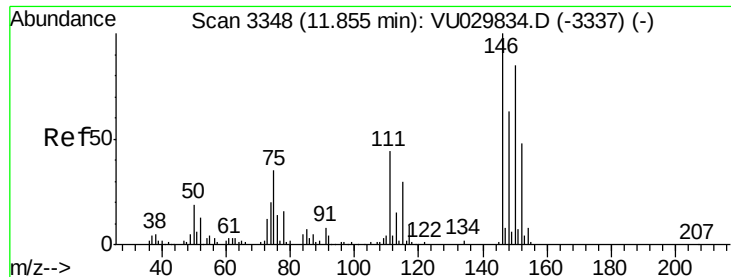

#68
 1,2-Dichlorobenzene-d4
 Concen: N.D. ug/l
 RT: 11.86 min Scan# 3350
 Delta R.T. 0.01 min
 Lab File: VU029837.D
 Acq: 06 Mar 2019 13:40

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0307WBL01

Tgt Ion:152 Resp: 21386
 Ion Ratio Lower Upper
 152 100
 115 61.4 0.0 124.0
 150 158.5 0.0 631.2

