


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU030719\
Data File : VU029829.D
Acq On : 06 Mar 2019 08:52
Operator : JC/SP
Sample : BFB
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U030719DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Fri Mar 08 00:30:10 2019

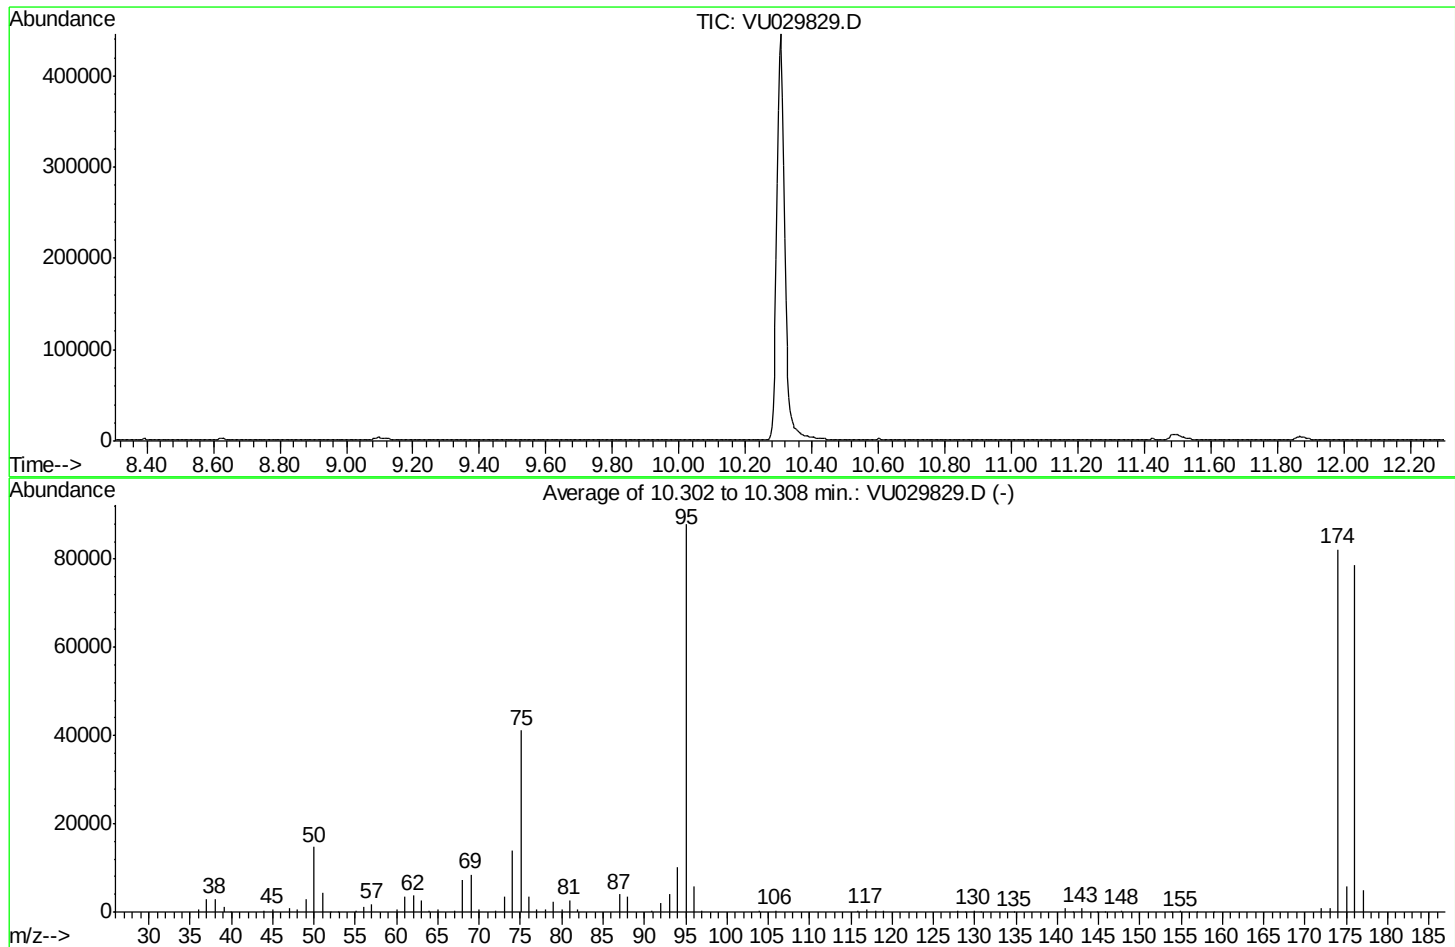

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2852

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	14702	PASS
75	95	30	60	46.9	41178	PASS
95	95	100	100	100.0	87880	PASS
96	95	5	9	6.7	5894	PASS
173	174	0.00	2	1.0	787	PASS
174	95	50	100	93.5	82130	PASS
175	174	5	9	7.1	5865	PASS
176	174	95	101	95.7	78613	PASS
177	176	5	9	6.3	4983	PASS