
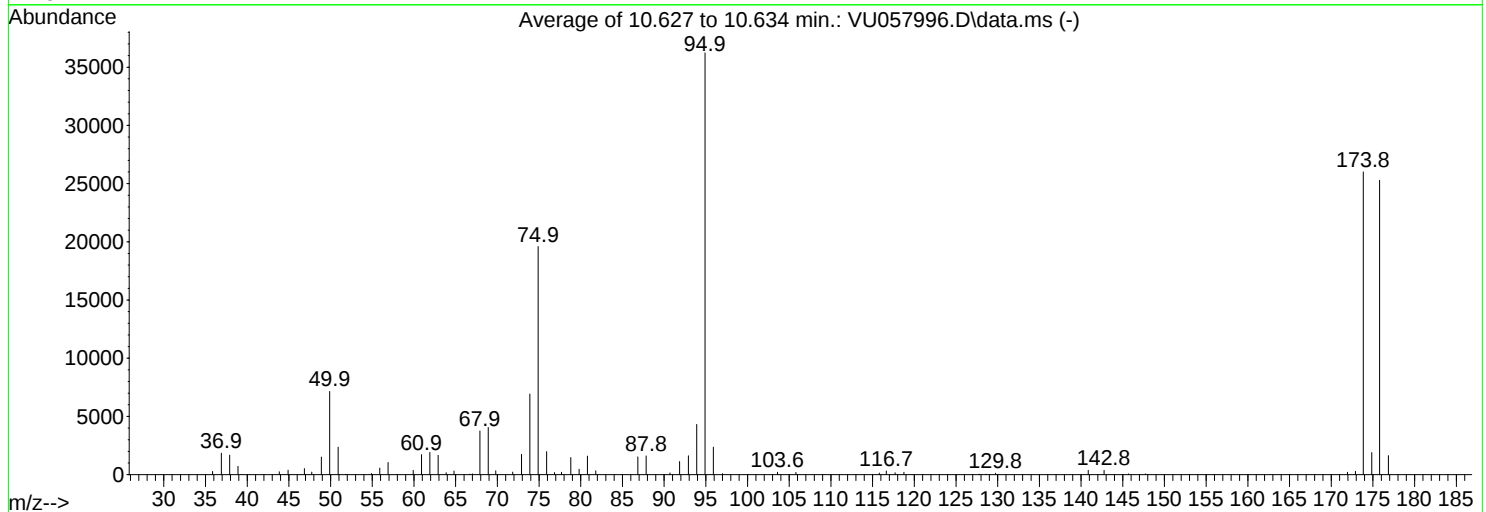


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030724\
Data File : VU057996.D
Acq On : 06 Mar 2024 12:14
Operator : MD/SY
Sample : BFB117
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB117

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Mar 07 03:58:14 2024

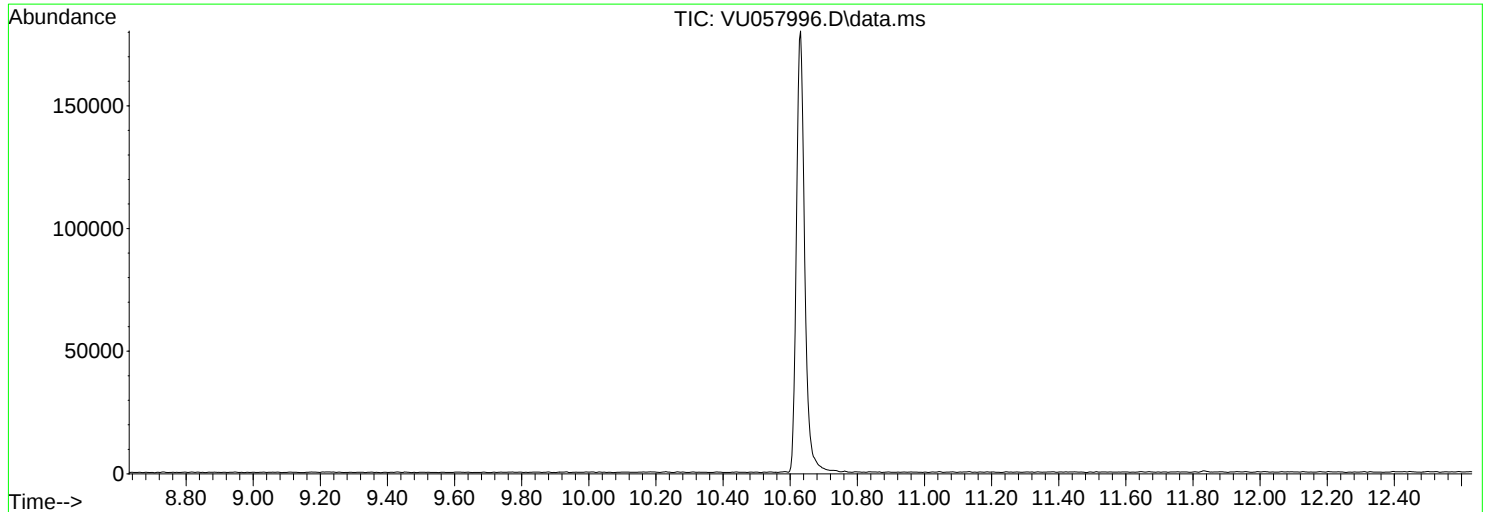

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2892

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	7154	PASS
75	95	30	80	54.1	19603	PASS
95	95	100	100	100.0	36232	PASS
96	95	5	9	6.5	2365	PASS
173	174	0.00	2	1.1	287	PASS
174	95	50	120	71.8	26005	PASS
175	174	5	9	7.3	1893	PASS
176	174	95	101	97.3	25296	PASS
177	176	5	9	6.5	1637	PASS

m/z	Abundance
39.80	341.0
43.90	532.0

Instrument :
MSVOA_U
ClientSampleId :
BFB117

m/z	Abundance
35.90	268.0
36.90	1981.0
37.90	1620.0
38.90	718.0
39.80	321.0
43.90	768.0
44.90	406.0
46.90	446.0
47.70	222.0
48.90	1512.0
49.90	7223.0
50.90	2543.0
54.90	148.0
55.90	612.0
56.90	1020.0
59.90	407.0
60.90	1875.0
61.90	1920.0
62.90	1725.0
63.90	153.0
64.80	291.0
67.00	115.0
67.90	3860.0
68.90	4102.0
69.80	339.0
71.80	217.0
72.90	1774.0
73.90	7111.0
74.90	19776.0
75.90	1974.0
76.90	164.0
77.70	198.0
78.80	1540.0
79.80	502.0
80.80	1659.0
81.80	359.0
86.90	1596.0
87.80	1510.0
90.70	179.0
91.90	1195.0
92.90	1657.0
93.90	4316.0
94.90	36624.0
95.90	2473.0
97.00	115.0
103.60	196.0
105.80	177.0
115.80	138.0
116.70	333.0
117.70	186.0
118.70	178.0
127.80	125.0
128.60	108.0
129.70	115.0
140.80	409.0
142.70	366.0
145.70	115.0
147.70	121.0
171.90	197.0
172.90	270.0
173.80	25528.0
174.80	1947.0
175.80	25000.0
176.80	1814.0

Instrument :
MSVOA_U
ClientSampleId :
BFB117

m/z	Abundance
35.80	289.0
36.90	1886.0
37.90	1742.0
38.90	762.0
39.80	271.0
43.80	797.0
44.90	408.0
46.80	547.0
47.70	220.0
48.90	1570.0
49.90	7380.0
50.90	2407.0
54.90	130.0
55.90	575.0
56.90	1061.0
59.90	384.0
60.90	1742.0
61.90	1988.0
62.90	1716.0
63.90	177.0
64.80	340.0
67.00	117.0
67.90	3889.0
68.90	4176.0
69.80	347.0
71.90	212.0
72.90	1835.0
73.90	7164.0
74.90	20088.0
75.90	2054.0
76.80	166.0
77.70	211.0
78.80	1531.0
79.80	481.0
80.80	1657.0
81.80	340.0
86.90	1622.0
87.90	1664.0
90.70	163.0
91.90	1145.0
92.90	1633.0
93.90	4376.0
94.90	37304.0
95.90	2443.0
97.00	120.0
103.60	218.0
105.80	186.0
115.80	137.0
116.70	330.0
117.70	178.0
118.80	209.0
129.80	132.0
140.80	373.0
142.80	355.0
145.70	115.0
147.70	106.0
172.00	215.0
172.90	301.0
173.80	26824.0
174.90	1950.0
175.80	26064.0
176.80	1639.0

Instrument :
MSVOA_U
ClientSampleId :
BFB117

m/z	Abundance
35.80	286.0
36.90	1651.0
37.90	1684.0
38.90	671.0
39.80	230.0
43.80	759.0
44.90	333.0
46.80	582.0
47.80	217.0
48.90	1464.0
49.90	6859.0
50.90	2138.0
51.80	101.0
55.90	517.0
56.90	1057.0
59.90	337.0
60.90	1537.0
61.90	1836.0
62.90	1565.0
63.80	189.0
64.80	321.0
66.70	112.0
67.90	3512.0
68.90	3905.0
69.80	312.0
71.90	236.0
72.90	1613.0
73.90	6510.0
74.90	18944.0
75.90	1894.0
76.80	198.0
77.70	201.0
78.80	1335.0
79.80	416.0
80.80	1477.0
81.80	279.0
86.80	1357.0
87.90	1643.0
90.70	120.0
91.80	1027.0
92.90	1558.0
93.90	4243.0
94.90	34768.0
95.90	2178.0
103.60	205.0
105.80	199.0
115.80	135.0
116.60	266.0
117.70	136.0
118.80	239.0
129.80	145.0
140.90	330.0
142.80	401.0
172.00	219.0
172.90	289.0
173.90	25664.0
174.90	1781.0
175.80	24824.0
176.90	1458.0

Instrument :
MSVOA_U
ClientSampleId :
BFB117