


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU030819\
Data File : VU029843.D
Acq On : 07 Mar 2019 09:13
Operator : JC/SP
Sample : BFB
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U030719DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Fri Mar 08 00:30:10 2019

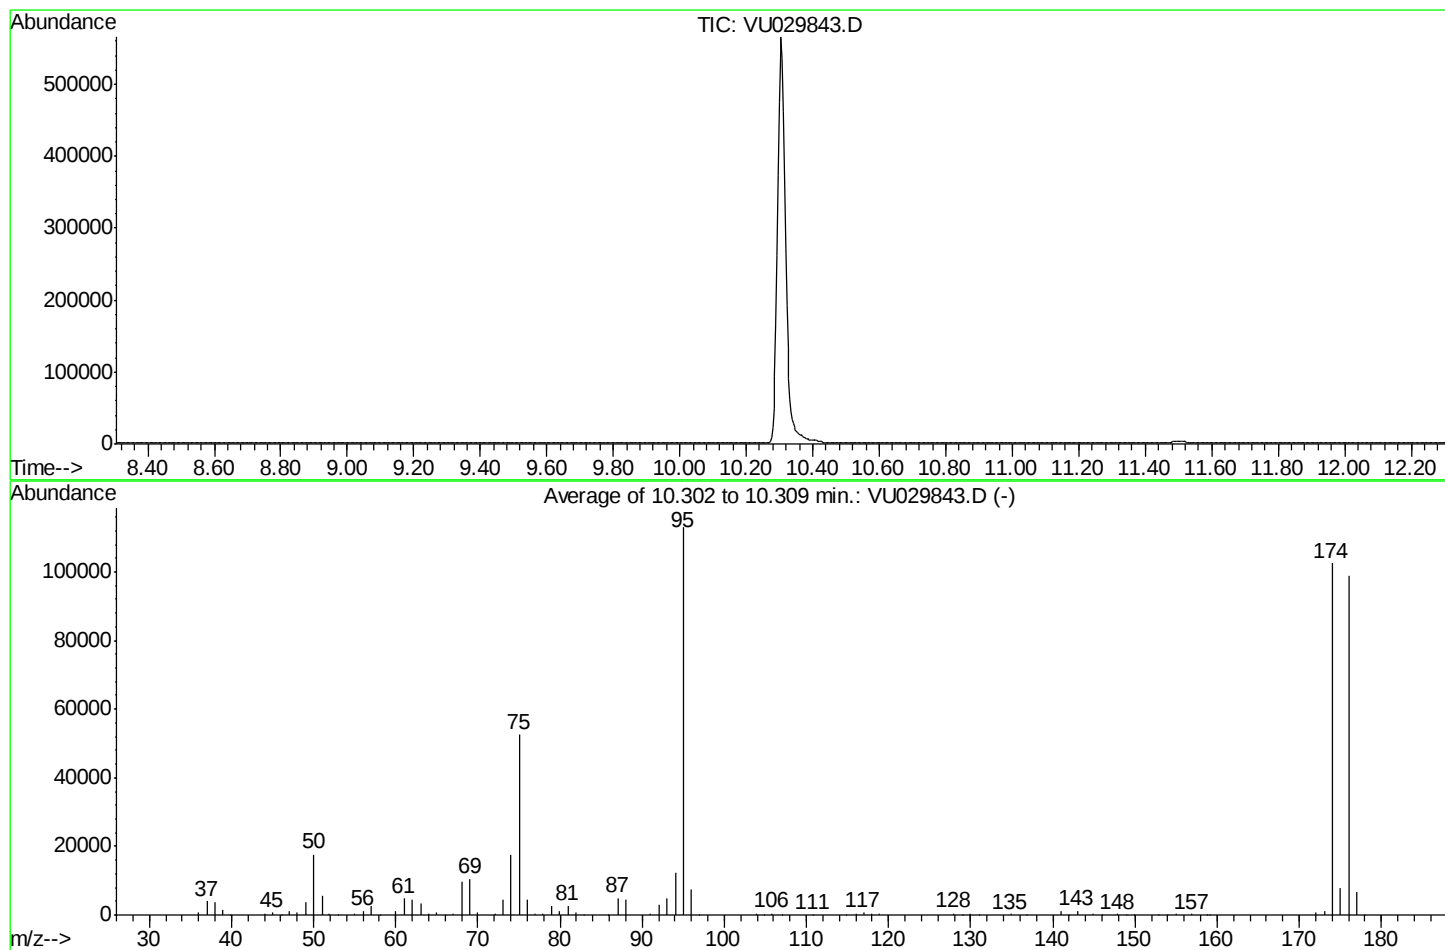

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2852

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	17720	PASS
75	95	30	60	46.5	52557	PASS
95	95	100	100	100.0	112992	PASS
96	95	5	9	6.6	7436	PASS
173	174	0.00	2	1.0	1012	PASS
174	95	50	100	90.7	102536	PASS
175	174	5	9	7.6	7769	PASS
176	174	95	101	96.5	98968	PASS
177	176	5	9	6.7	6623	PASS