

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030821\
 Data File : VU042519.D
 Acq On : 08 Mar 2021 11:17
 Operator : SY/MD
 Sample : M1588-16
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C03W3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC: VU042519.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	75	82	95	rVB	35216	40597	10.47%	1.150%
2	1.919	172	180	197	rVB	32231	42159	10.88%	1.195%
3	2.584	372	387	401	rBV4	205434	387028	99.85%	10.968%
4	2.649	401	407	416	rVV2	2433	4555	1.18%	0.129%
5	3.880	776	790	802	rBV3	6036	14130	3.65%	0.400%
6	4.645	1012	1028	1083	rBV	44312	158783	40.96%	4.500%
7	5.073	1145	1161	1180	rBV	60402	135838	35.04%	3.849%
8	5.327	1223	1240	1255	rBV2	161493	369744	95.39%	10.478%
9	5.732	1346	1366	1386	rBV2	117932	312925	80.73%	8.868%
10	6.256	1516	1529	1552	rBV2	121991	231773	59.79%	6.568%
11	6.700	1653	1667	1686	rBV	75293	145970	37.66%	4.137%
12	7.575	1927	1939	1954	rBV2	41649	72406	18.68%	2.052%
13	7.722	1972	1985	1999	rBV2	9196	17666	4.56%	0.501%
14	7.906	2028	2042	2058	rBV	150100	259163	66.86%	7.344%
15	8.189	2116	2130	2143	rBV3	25588	43949	11.34%	1.245%
16	8.645	2258	2272	2305	rBV	197302	387613	100.00%	10.984%
17	9.423	2501	2514	2533	rBV	172862	289130	74.59%	8.193%
18	10.642	2885	2893	2902	rBV3	3370	4884	1.26%	0.138%
19	10.764	2919	2931	2946	rBV2	62695	101032	26.07%	2.863%
20	11.819	3248	3259	3278	rVB	169103	270901	69.89%	7.677%
21	12.201	3366	3378	3392	rVB	148750	238570	61.55%	6.761%




Sum of corrected areas: 3528816

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030821\
Data File : VU042519.D
Acq On : 08 Mar 2021 11:17
Operator : SY/MD
Sample : M1588-16
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C03W3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

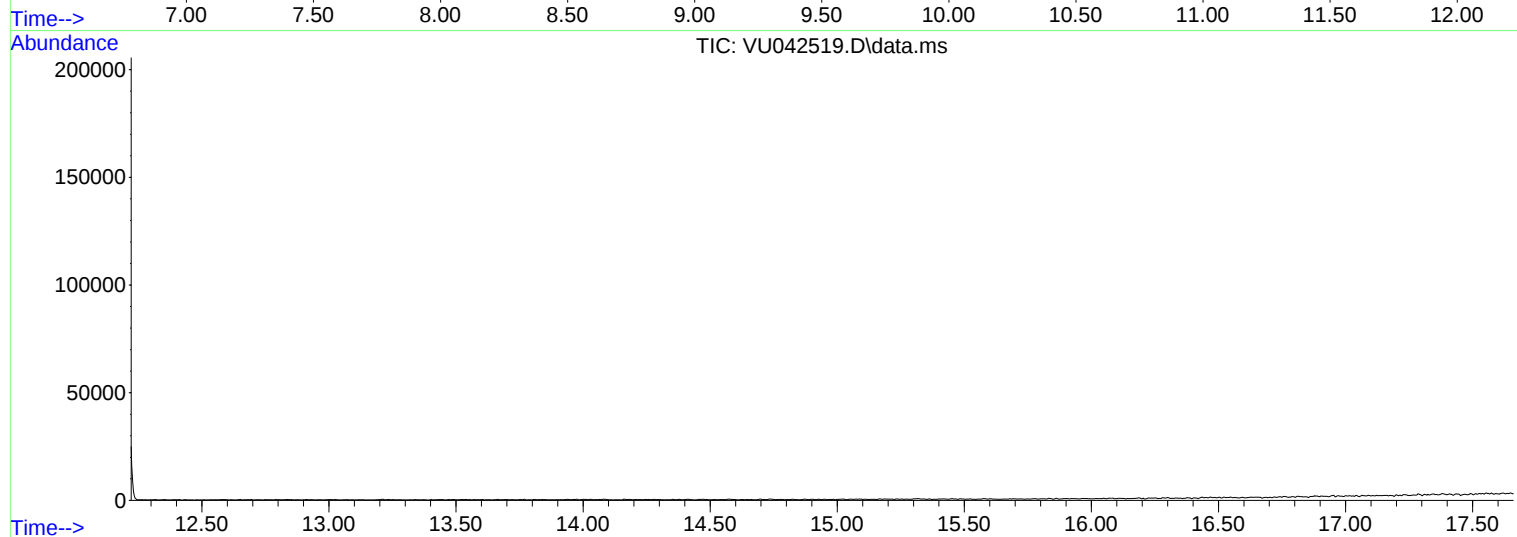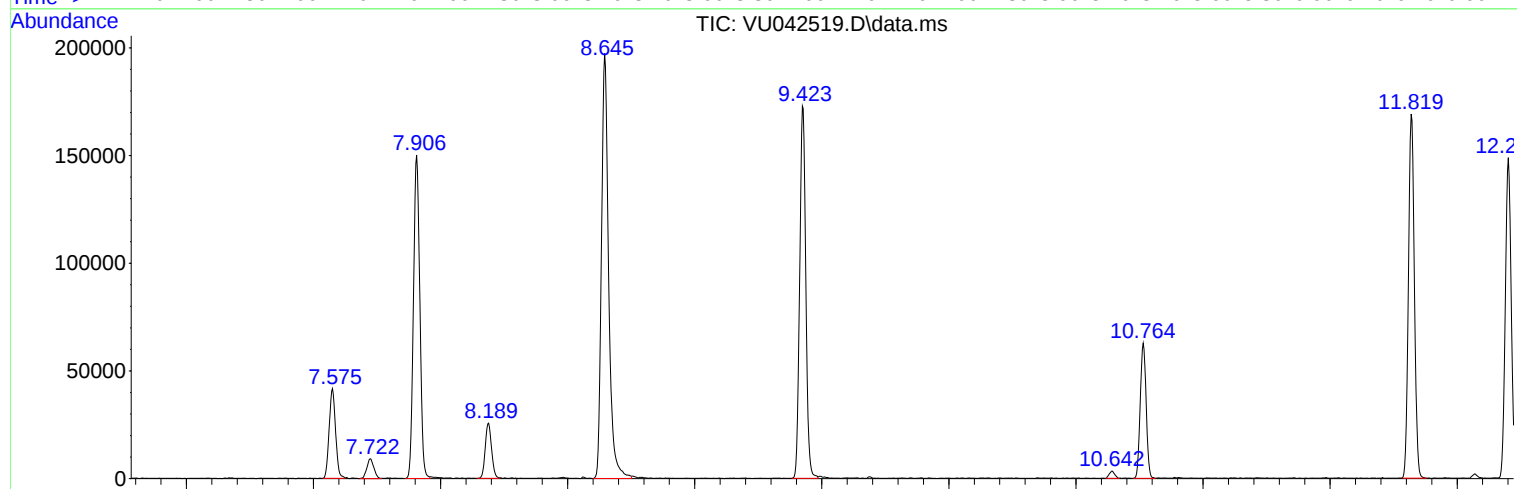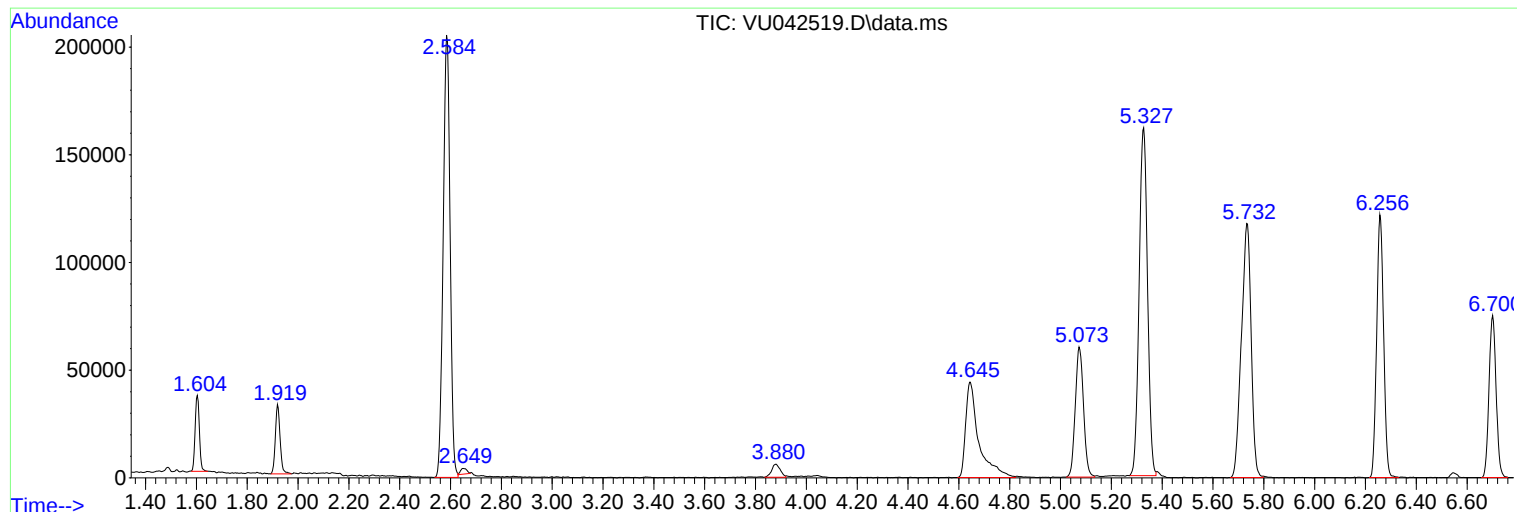

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030821\
Data File : VU042519.D
Acq On : 08 Mar 2021 11:17
Operator : SY/MD
Sample : M1588-16
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C03W3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030821\
Data File : VU042519.D
Acq On : 08 Mar 2021 11:17
Operator : SY/MD
Sample : M1588-16
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C03W3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
