


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030821\
Data File : VU042515.D
Acq On : 08 Mar 2021 09:03
Operator : SY/MD
Sample : BFB23
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB23

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Title : TRACE VOA SOM01.0
Last Update : Tue Mar 09 01:35:43 2021

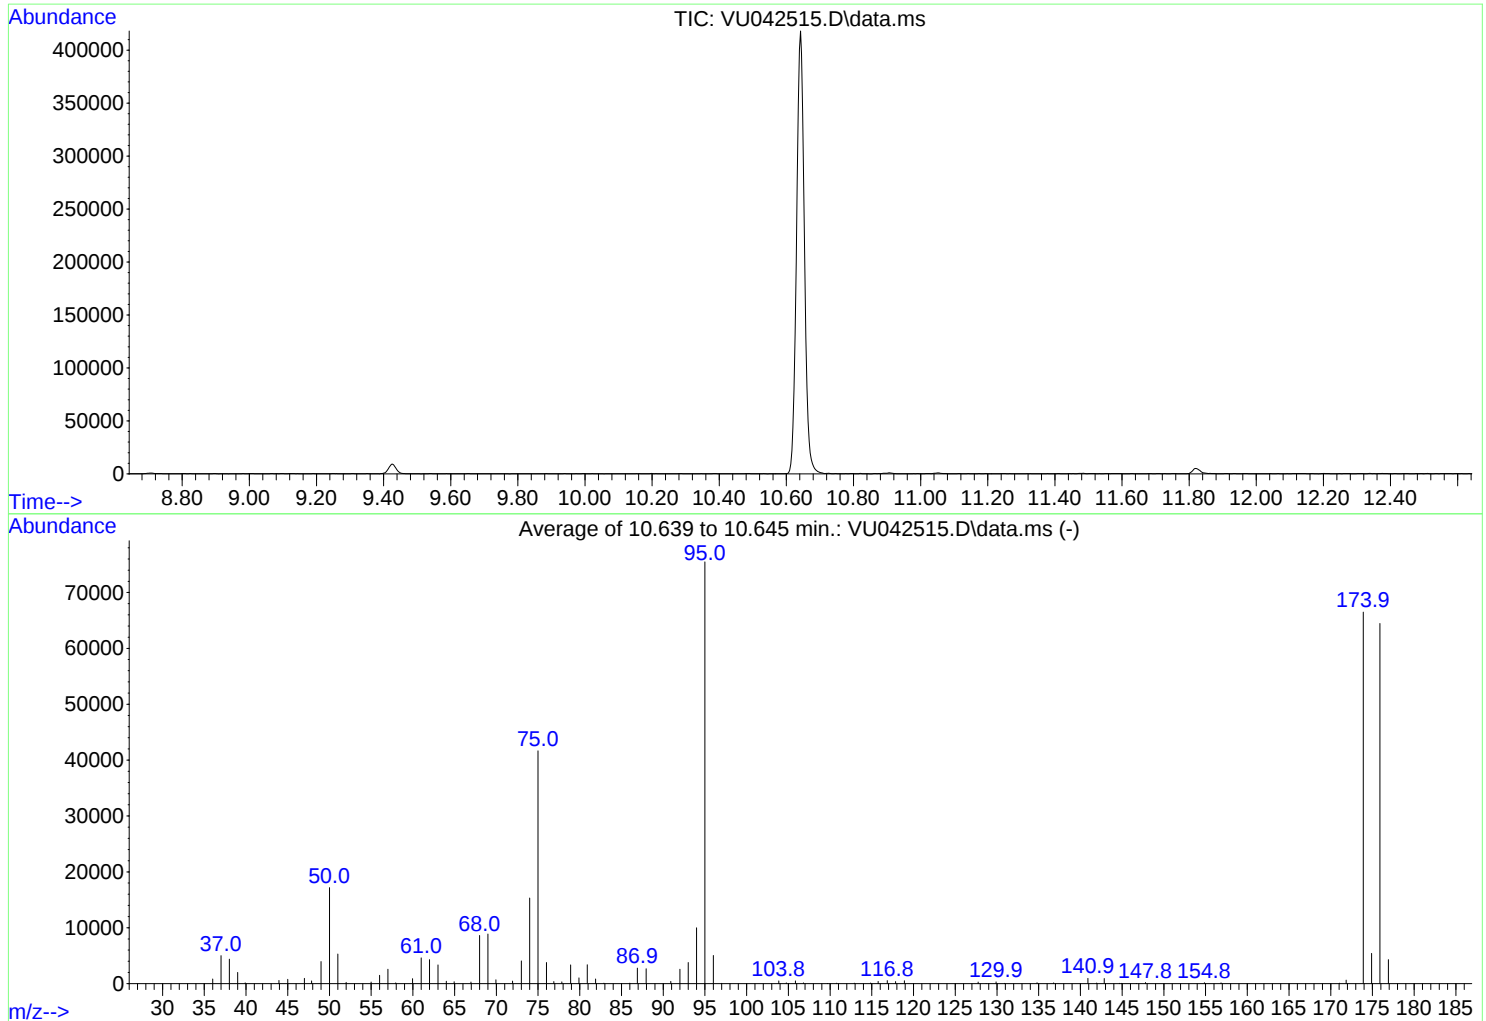

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.7	17171	PASS
75	95	30	80	55.2	41672	PASS
95	95	100	100	100.0	75488	PASS
96	95	5	9	6.7	5054	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	88.1	66496	PASS
175	174	5	9	8.1	5404	PASS
176	174	95	101	96.9	64467	PASS
177	176	5	9	6.7	4311	PASS

m/z	Abundance
36.00	871.0
37.00	5011.0
38.00	4521.0
39.00	1845.0
39.90	137.0
44.00	753.0
45.00	787.0
47.00	875.0
48.00	465.0
49.00	3876.0
50.00	17312.0
51.00	5451.0
52.00	207.0
55.00	322.0
56.00	1555.0
57.00	2649.0
58.00	147.0
60.00	820.0
61.00	4446.0
62.00	4312.0
63.00	3506.0
64.00	420.0
64.90	374.0
66.90	321.0
68.00	8791.0
69.00	9018.0
69.90	702.0
71.90	477.0
73.00	3979.0
74.00	15082.0
75.00	41744.0
76.00	3849.0
76.90	359.0
77.80	322.0
78.90	3305.0
79.90	1040.0
80.90	3412.0
81.90	873.0
82.90	122.0
86.90	2776.0
88.00	2702.0
90.90	398.0
92.00	2665.0
93.00	3684.0
94.00	10008.0
95.00	74936.0
96.00	5232.0
97.00	123.0
103.90	502.0
104.90	161.0
105.80	436.0
106.80	142.0
110.80	125.0
112.90	118.0
114.80	132.0
115.80	388.0
116.90	478.0
117.80	350.0
118.90	489.0
127.80	279.0
128.70	106.0
129.90	281.0
134.80	165.0
136.80	141.0
140.90	928.0
141.90	111.0
142.80	957.0
144.70	114.0
146.70	104.0
147.80	208.0
154.80	178.0
156.90	134.0
171.10	135.0
171.90	665.0
173.90	64088.0
174.90	5369.0
175.90	62160.0
176.90	4479.0

Instrument :
MSVOA_U
ClientSampleId :
BFB23

m/z	Abundance
36.00	856.0
37.00	5155.0
38.00	4482.0
39.00	2130.0
39.90	141.0
44.00	712.0
45.00	791.0
47.00	1015.0
47.80	483.0
49.00	4100.0
50.00	17648.0
51.00	5445.0
52.00	223.0
55.00	290.0
56.00	1571.0
57.00	2655.0
57.90	151.0
60.00	893.0
61.00	4778.0
62.00	4419.0
63.00	3449.0
64.00	452.0
64.90	362.0
66.90	306.0
68.00	8889.0
69.00	9218.0
70.00	714.0
72.00	477.0
73.00	4174.0
74.00	15873.0
75.00	43040.0
76.00	3926.0
76.90	387.0
77.80	287.0
78.90	3444.0
79.90	1064.0
80.90	3423.0
81.90	859.0
82.90	122.0
86.00	117.0
86.90	2899.0
87.90	2747.0
90.90	403.0
92.00	2651.0
93.00	3945.0
94.00	10322.0
95.00	77832.0
96.00	5254.0
97.00	103.0
103.80	501.0
104.70	151.0
105.90	511.0
106.80	142.0
109.70	102.0
110.80	105.0
112.90	119.0
114.80	125.0
115.70	425.0
116.90	549.0
117.90	406.0
118.90	519.0
127.70	288.0
129.90	312.0
130.90	114.0
134.80	177.0
136.80	139.0
140.90	995.0
141.90	124.0
142.80	930.0
144.70	111.0
145.00	107.0
147.80	193.0
154.90	186.0
156.80	142.0
171.90	643.0
173.90	68672.0
174.90	5552.0
175.90	66608.0
176.90	4410.0

Instrument :
MSVOA_U
ClientSampleId :
BFB23

m/z	Abundance
36.00	791.0
37.00	4836.0
38.00	4105.0
39.00	2050.0
39.90	153.0
44.00	696.0
45.00	770.0
47.00	928.0
47.80	497.0
49.00	3905.0
50.00	16552.0
51.00	4995.0
52.00	226.0
55.00	230.0
56.00	1354.0
57.00	2471.0
57.90	128.0
59.90	919.0
61.00	4625.0
62.00	4180.0
63.00	3098.0
64.00	432.0
65.00	321.0
67.00	277.0
68.00	8153.0
69.00	8432.0
70.00	684.0
72.00	409.0
73.00	4018.0
74.00	15002.0
75.00	40232.0
76.00	3552.0
76.90	398.0
77.90	308.0
78.90	3270.0
79.90	1032.0
80.90	3268.0
81.90	792.0
86.00	132.0
86.90	2661.0
87.90	2565.0
90.90	389.0
92.00	2425.0
93.00	3730.0
94.00	9684.0
95.00	73696.0
96.00	4676.0
103.90	478.0
104.70	129.0
105.90	494.0
106.80	140.0
114.90	122.0
115.70	418.0
116.80	574.0
117.90	375.0
118.90	582.0
127.70	279.0
129.00	104.0
129.90	330.0
130.90	104.0
134.80	153.0
136.80	141.0
140.90	948.0
142.00	134.0
142.90	875.0
144.90	115.0
147.80	173.0
154.90	185.0
156.80	158.0
171.00	103.0
171.80	603.0
173.90	66728.0
174.90	5291.0
175.90	64632.0
176.90	4045.0

Instrument :
MSVOA_U
ClientSampleId :
BFB23

m/z	Abundance
43.80	156.0

Instrument :
MSVOA_U
ClientSampleId :
BFB23