


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030824\
Data File : VU058003.D
Acq On : 08 Mar 2024 08:31
Operator : MD/SY
Sample : BFB118
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB118

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Mar 09 00:10:03 2024

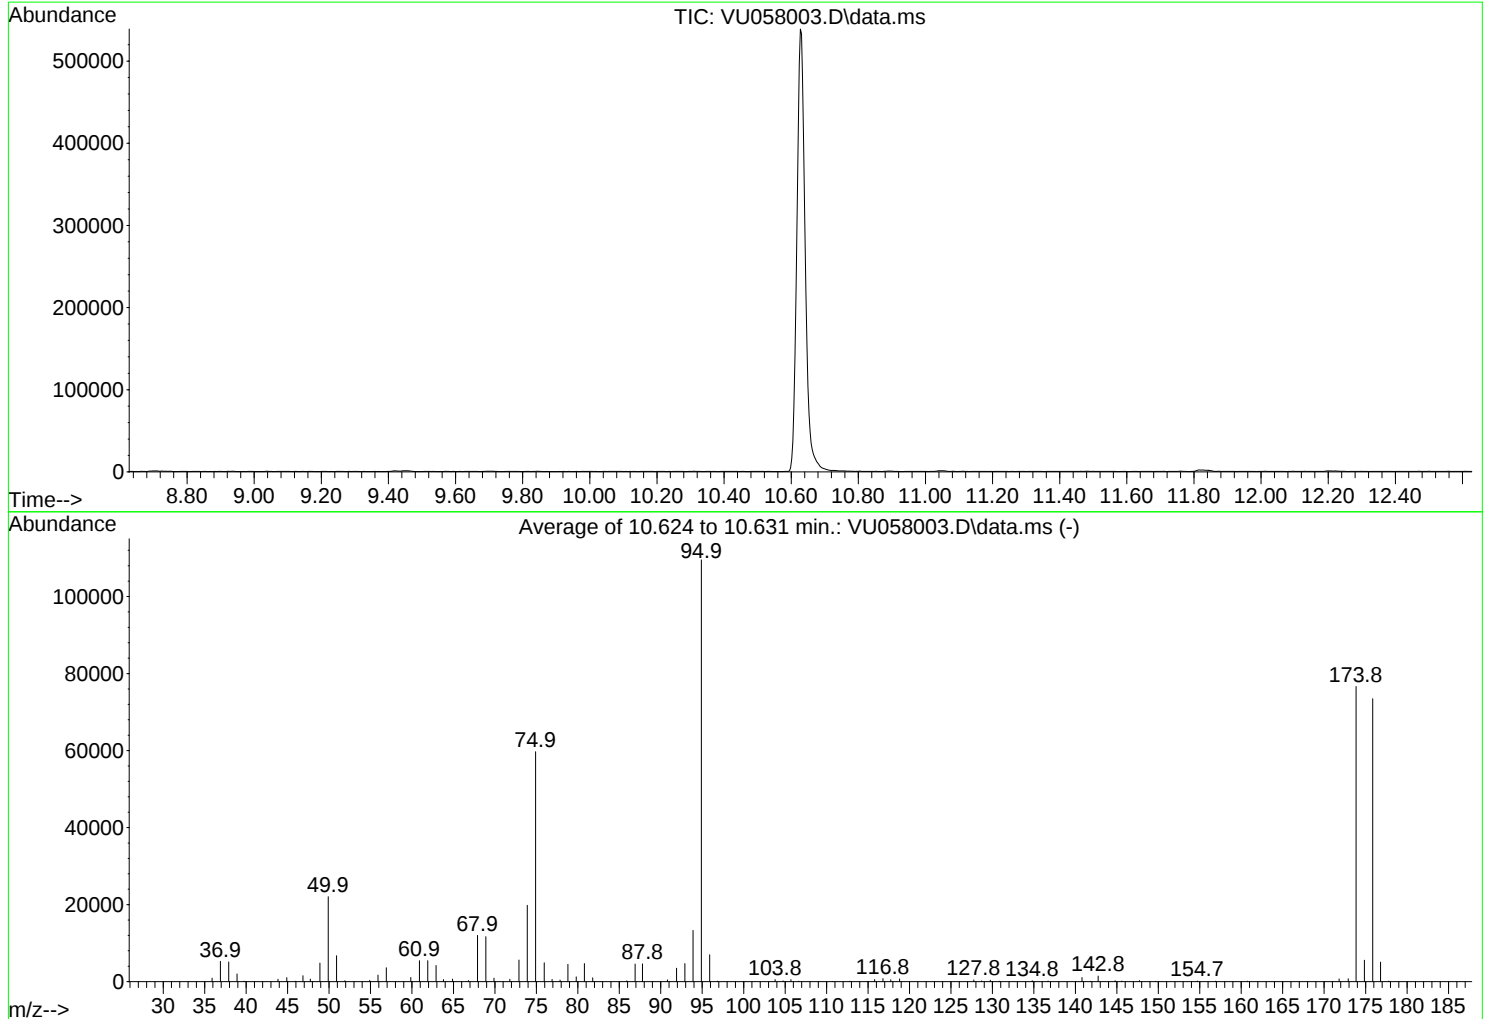

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.1	22061	PASS
75	95	30	80	54.5	59720	PASS
95	95	100	100	100.0	109528	PASS
96	95	5	9	6.4	7001	PASS
173	174	0.00	2	1.0	755	PASS
174	95	50	120	70.0	76653	PASS
175	174	5	9	7.3	5584	PASS
176	174	95	101	95.9	73477	PASS
177	176	5	9	6.9	5089	PASS

Scan 2890 (10.582 min): VU058003.D\data.ms
BFB118

m/z	Abundance
39.70	180.0
43.90	386.0

Instrument :
MSVOA_U
ClientSampleId :
BFB118

m/z	Abundance
35.90	839.0
36.90	5366.0
37.90	4963.0
38.90	1905.0
39.80	306.0
43.90	976.0
44.90	1058.0
45.90	128.0
46.90	1415.0
47.70	621.0
48.90	4576.0
49.90	21088.0
50.90	6452.0
51.90	273.0
54.90	328.0
55.90	1759.0
56.90	3320.0
59.90	948.0
60.90	5438.0
61.90	5285.0
62.90	4175.0
63.80	517.0
64.90	561.0
66.80	269.0
67.90	11522.0
68.90	11182.0
69.90	906.0
71.80	600.0
72.90	5470.0
73.90	18848.0
74.90	57664.0
76.00	4711.0
76.90	598.0
77.90	411.0
78.80	4407.0
79.80	1112.0
80.80	4423.0
81.80	964.0
85.90	157.0
86.90	4472.0
87.80	4604.0
90.80	414.0
91.90	3212.0
92.90	4427.0
93.90	12761.0
94.90	104872.0
95.90	6673.0
97.00	147.0
103.80	534.0
104.80	222.0
105.70	525.0
106.60	120.0
112.80	132.0
115.80	474.0
116.80	774.0
117.80	486.0
118.80	660.0
127.70	409.0
128.70	198.0
129.70	356.0
130.80	153.0
134.80	242.0
136.70	165.0
140.80	1046.0
141.80	149.0
142.70	1471.0
144.80	221.0
145.60	154.0
147.70	275.0
149.70	104.0
154.70	167.0
156.90	129.0
160.70	115.0
171.80	705.0
172.90	685.0
173.80	71080.0
174.90	5204.0
175.90	67728.0
176.80	4866.0
177.80	167.0

Instrument :
MSVOA_U
ClientSampleId :
BFB118

m/z	Abundance
35.90	933.0
36.90	5420.0
37.90	5357.0
38.90	2004.0
39.80	324.0
43.90	1050.0
44.90	1115.0
45.90	139.0
46.80	1608.0
47.80	681.0
48.90	4960.0
49.90	22688.0
50.90	6872.0
51.90	250.0
54.90	375.0
55.90	1749.0
56.90	3741.0
59.80	1090.0
60.90	5591.0
61.90	5628.0
62.90	4305.0
63.80	523.0
64.90	687.0
66.80	290.0
67.90	12324.0
68.90	11985.0
69.90	923.0
71.80	664.0
72.90	5812.0
73.90	20400.0
74.90	61416.0
75.90	5021.0
76.90	598.0
77.90	457.0
78.80	4611.0
79.80	1294.0
80.80	4884.0
81.80	1038.0
82.80	107.0
85.90	259.0
86.90	4681.0
87.80	4802.0
90.80	456.0
91.90	3587.0
92.90	4830.0
93.90	13647.0
94.90	112952.0
95.90	7160.0
96.80	117.0
103.80	557.0
104.70	235.0
105.70	543.0
106.60	114.0
112.80	123.0
114.90	102.0
115.80	574.0
116.80	814.0
117.80	490.0
118.80	752.0
127.70	488.0
128.70	235.0
129.70	362.0
130.80	140.0
134.80	269.0
136.70	168.0
140.80	1062.0
141.80	126.0
142.80	1504.0
144.80	257.0
145.60	170.0
147.80	292.0
149.60	100.0
154.70	190.0
156.90	133.0
160.70	128.0
171.80	759.0
172.90	784.0
173.90	79008.0
174.90	5789.0
175.80	75944.0
176.80	5235.0
177.80	183.0

Instrument :
MSVOA_U
ClientSampleId :
BFB118

m/z	Abundance
35.90	978.0
36.90	5048.0
37.90	5077.0
38.90	2032.0
39.80	310.0
43.80	1027.0
44.90	967.0
45.90	128.0
46.80	1568.0
47.80	699.0
48.90	4916.0
49.90	22408.0
50.90	6876.0
51.90	229.0
54.90	360.0
55.90	1646.0
56.90	3728.0
59.90	1164.0
60.90	5280.0
61.90	5467.0
62.90	4120.0
63.80	533.0
64.90	723.0
66.80	276.0
67.90	12151.0
68.90	11899.0
69.90	884.0
71.80	650.0
72.90	5528.0
73.90	20232.0
74.90	60080.0
75.90	4985.0
76.90	563.0
77.80	419.0
78.80	4431.0
79.80	1325.0
80.80	4804.0
81.80	993.0
85.90	268.0
86.90	4511.0
87.80	4418.0
90.80	477.0
91.90	3667.0
92.90	4894.0
93.90	13494.0
94.90	110760.0
95.90	7169.0
96.80	137.0
103.80	525.0
104.70	217.0
105.70	511.0
106.70	105.0
110.70	113.0
112.80	101.0
114.90	116.0
115.80	604.0
116.80	763.0
117.70	472.0
118.80	778.0
127.80	462.0
128.70	222.0
129.80	372.0
130.80	124.0
134.80	245.0
136.70	165.0
140.80	1098.0
142.80	1389.0
144.80	235.0
145.60	164.0
147.80	294.0
154.70	193.0
156.90	137.0
160.80	143.0
171.80	724.0
172.90	797.0
173.90	79872.0
174.80	5759.0
175.80	76760.0
176.80	5165.0
177.80	144.0

Instrument :
MSVOA_U
ClientSampleId :
BFB118