


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030919\
 Data File : VU029852.D
 Acq On : 07 Mar 2019 13:56
 Operator : JC/SP
 Sample : BFB57
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB57

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM021519WMA.M
 Title : VOC Analysis
 Last Update : Fri Mar 08 04:31:20 2019

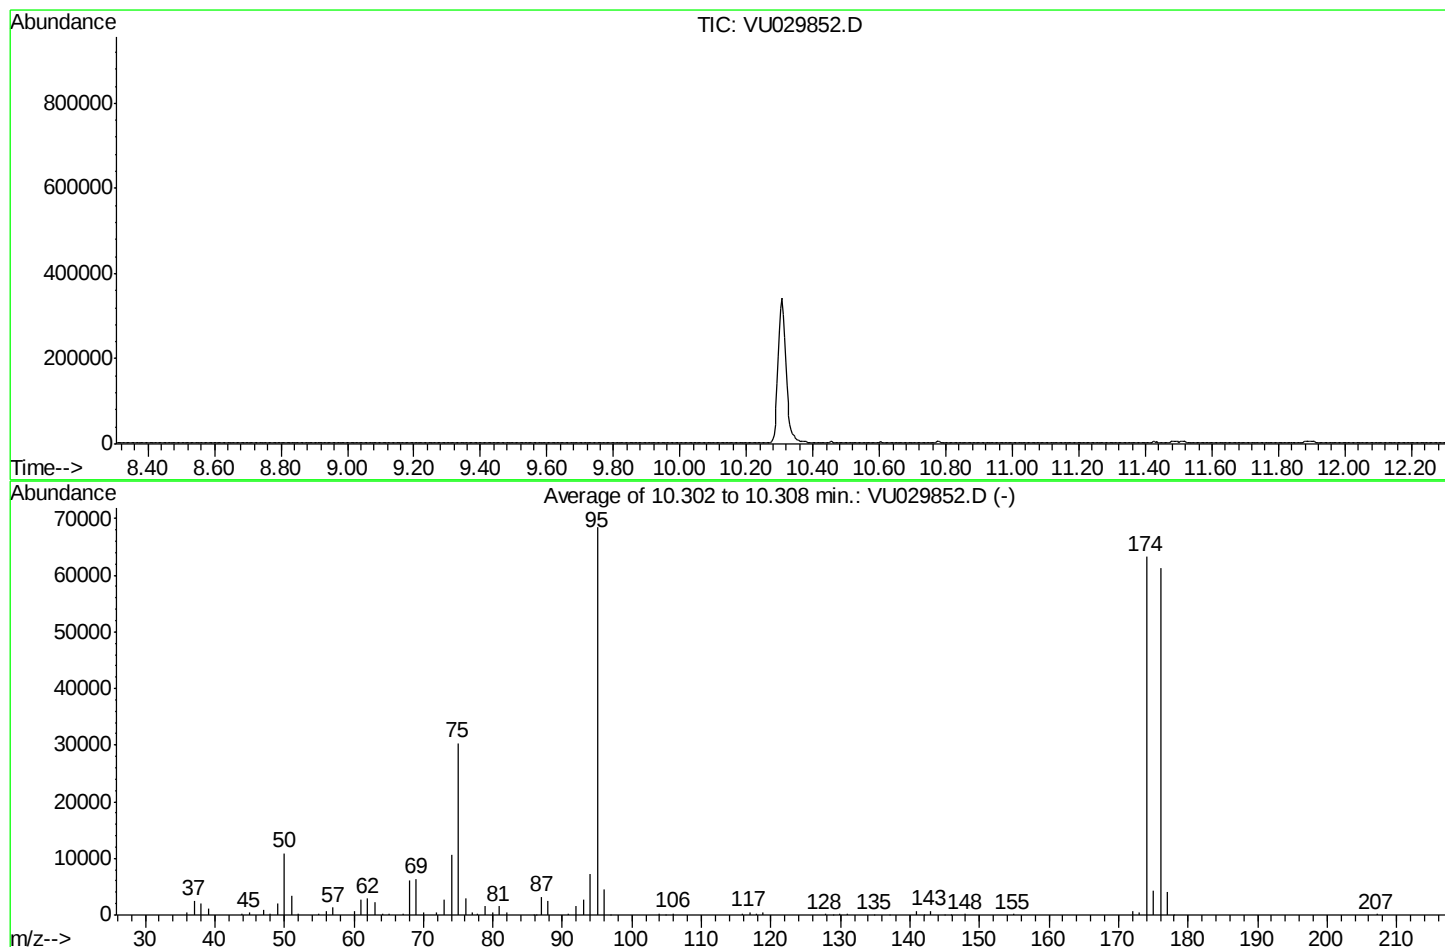

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2853

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	10869	PASS
75	95	30	80	44.4	30410	PASS
95	95	100	100	100.0	68474	PASS
96	95	5	9	6.8	4632	PASS
173	174	0.00	2	0.9	551	PASS
174	95	50	120	92.3	63234	PASS
175	174	5	9	6.8	4282	PASS
176	174	95	101	97.0	61357	PASS
177	176	5	9	6.6	4076	PASS

m/z	Abundance
39.90	1822.0
44.00	484.0

Instrument :
MSVOA_U
ClientSampleId :
BFB57

m/z	Abundance
35.90	412.0
37.00	2477.0
38.00	2233.0
39.10	1026.0
40.00	1888.0
43.90	601.0
45.00	419.0
46.90	998.0
47.90	218.0
49.00	2087.0
50.00	10591.0
51.00	3167.0
52.00	238.0
55.00	195.0
56.00	757.0
57.00	1209.0
60.10	580.0
61.00	2398.0
62.00	2515.0
63.00	2285.0
64.10	262.0
65.00	341.0
67.00	150.0
68.00	6201.0
69.00	6193.0
70.00	392.0
72.00	371.0
73.00	2564.0
74.00	10400.0
75.00	29448.0
76.10	2692.0
77.00	434.0
77.80	235.0
78.90	1548.0
79.90	482.0
80.90	1455.0
82.00	369.0
86.20	154.0
87.00	3194.0
88.00	2525.0
90.80	203.0
92.00	1691.0
93.00	2475.0
94.10	7329.0
95.00	66112.0
96.00	4371.0
103.90	274.0
104.90	106.0
106.00	285.0
115.90	234.0
116.90	466.0
117.90	139.0
118.90	351.0
127.90	213.0
129.00	114.0
129.90	192.0
130.90	148.0
134.90	111.0
137.00	108.0
141.00	612.0
142.90	730.0
144.90	113.0
145.80	106.0
148.00	131.0
154.90	122.0
172.00	663.0
172.90	493.0
174.00	58712.0
175.00	4015.0
176.00	57840.0
177.00	4096.0
177.90	101.0
207.10	155.0

Instrument :
MSVOA_U
ClientSampleId :
BFB57

m/z	Abundance
35.90	469.0
37.00	2532.0
38.00	2159.0
39.00	1054.0
40.00	1764.0
43.90	659.0
44.90	464.0
46.90	962.0
48.00	293.0
49.00	2152.0
50.00	11107.0
51.00	3403.0
52.00	252.0
55.00	211.0
56.00	779.0
57.00	1368.0
60.10	638.0
61.00	2739.0
62.00	2903.0
63.00	2400.0
64.10	304.0
65.00	314.0
67.10	158.0
68.00	6312.0
69.00	6574.0
70.00	400.0
71.90	386.0
73.00	2822.0
74.00	11011.0
75.00	31320.0
76.10	3095.0
77.00	439.0
77.80	278.0
78.90	1581.0
79.90	511.0
80.90	1582.0
82.00	367.0
86.20	147.0
87.00	3337.0
87.90	2564.0
90.90	224.0
92.00	1767.0
93.00	2663.0
94.10	7386.0
95.00	70616.0
96.10	4810.0
97.00	140.0
103.80	236.0
104.90	118.0
106.00	288.0
115.90	215.0
116.90	570.0
117.90	220.0
118.90	390.0
127.80	230.0
128.90	127.0
129.90	186.0
131.00	145.0
134.90	112.0
137.00	100.0
141.00	605.0
142.00	100.0
142.90	753.0
144.90	122.0
145.80	116.0
147.90	183.0
154.80	148.0
172.00	764.0
172.90	576.0
174.00	65320.0
175.00	4472.0
176.00	63272.0
177.00	4239.0
207.10	140.0

Instrument :
MSVOA_U
ClientSampleId :
BFB57

m/z	Abundance
35.90	531.0
37.00	2472.0
38.00	1993.0
39.00	1038.0
40.00	1714.0
43.90	738.0
44.90	483.0
47.00	811.0
48.00	381.0
49.00	2138.0
50.00	10909.0
51.00	3371.0
52.00	215.0
54.90	217.0
56.00	752.0
57.00	1441.0
60.00	595.0
61.00	2759.0
62.00	3102.0
63.00	2347.0
64.20	299.0
65.00	340.0
67.10	163.0
68.10	5962.0
69.00	6423.0
70.00	401.0
71.90	329.0
73.00	2795.0
74.00	10485.0
75.00	30464.0
76.10	3045.0
77.00	381.0
77.80	307.0
78.90	1568.0
79.90	511.0
80.90	1657.0
82.00	324.0
85.80	107.0
87.00	3129.0
87.90	2413.0
90.90	221.0
92.00	1638.0
93.00	2784.0
94.00	6950.0
95.00	68696.0
96.10	4717.0
97.00	158.0
103.80	194.0
105.90	254.0
115.90	177.0
116.90	595.0
117.90	298.0
118.90	355.0
127.80	216.0
128.80	127.0
129.90	188.0
131.00	135.0
134.80	109.0
141.00	517.0
142.00	107.0
142.90	723.0
144.90	100.0
147.90	214.0
154.90	168.0
172.00	773.0
172.90	586.0
174.00	65672.0
175.00	4361.0
176.00	62960.0
177.00	3893.0
207.20	142.0

Instrument :
MSVOA_U
ClientSampleId :
BFB57