


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU030920\
 Data File : VU037128.D
 Acq On : 09 Mar 2020 11:23
 Operator : JC/MD
 Sample : BFB
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U030920DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER
 Last Update : Mon Mar 09 15:46:40 2020

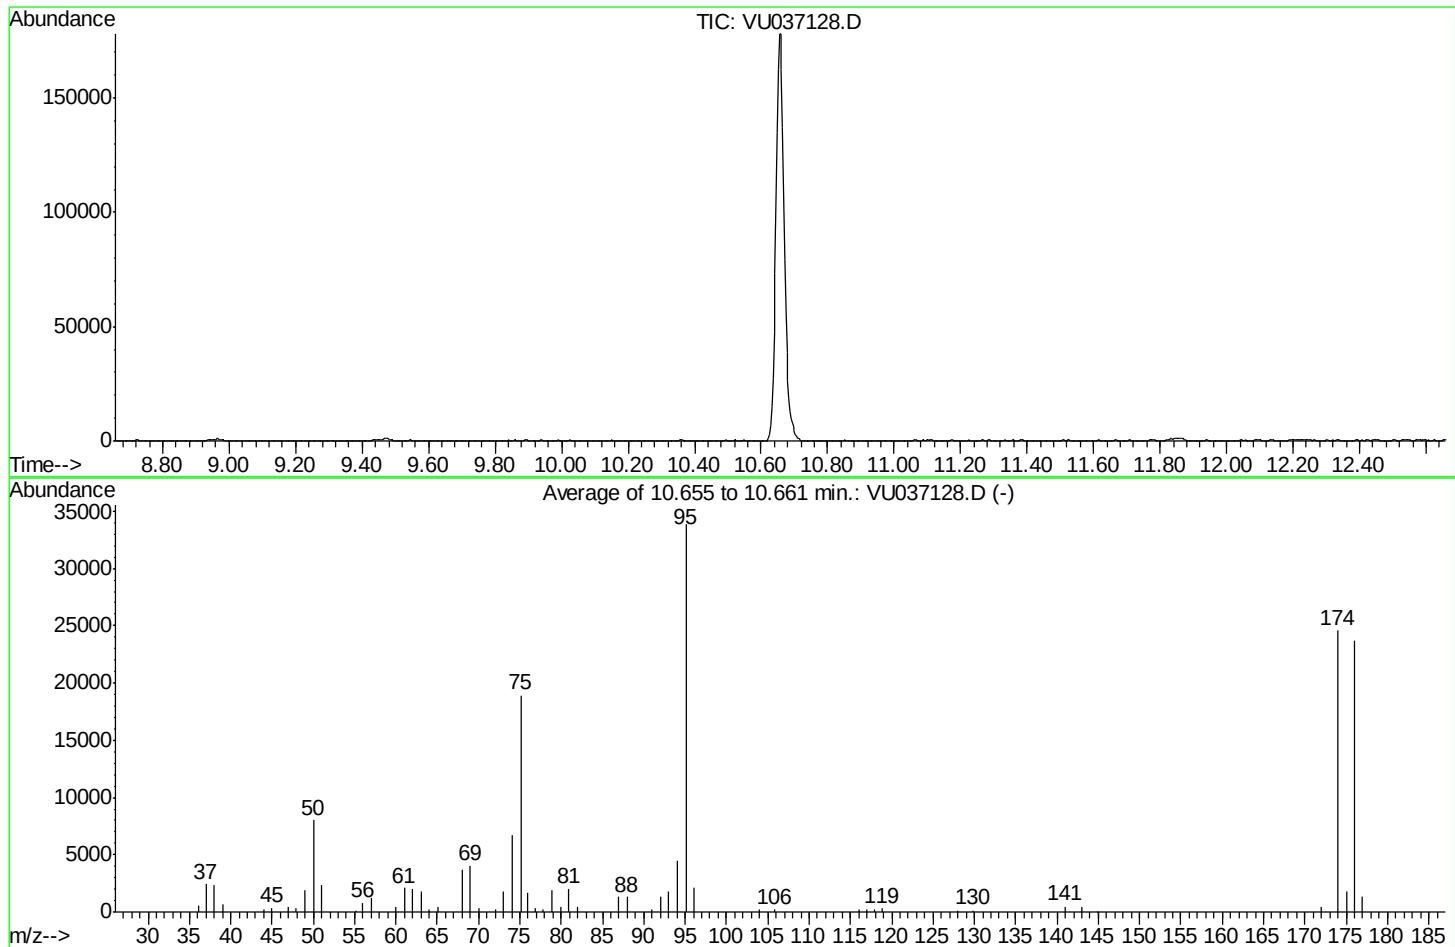

AutoFind: Scans 2897, 2898, 2899; Background Corrected with Scan 2884

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.7	8014	PASS
75	95	30	60	56.0	18944	PASS
95	95	100	100	100.0	33850	PASS
96	95	5	9	6.4	2180	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	72.5	24549	PASS
175	174	5	9	7.5	1834	PASS
176	174	95	101	96.7	23730	PASS
177	176	5	9	5.9	1390	PASS