


t-1,4-Dichloro-2-butene

Response Ratio

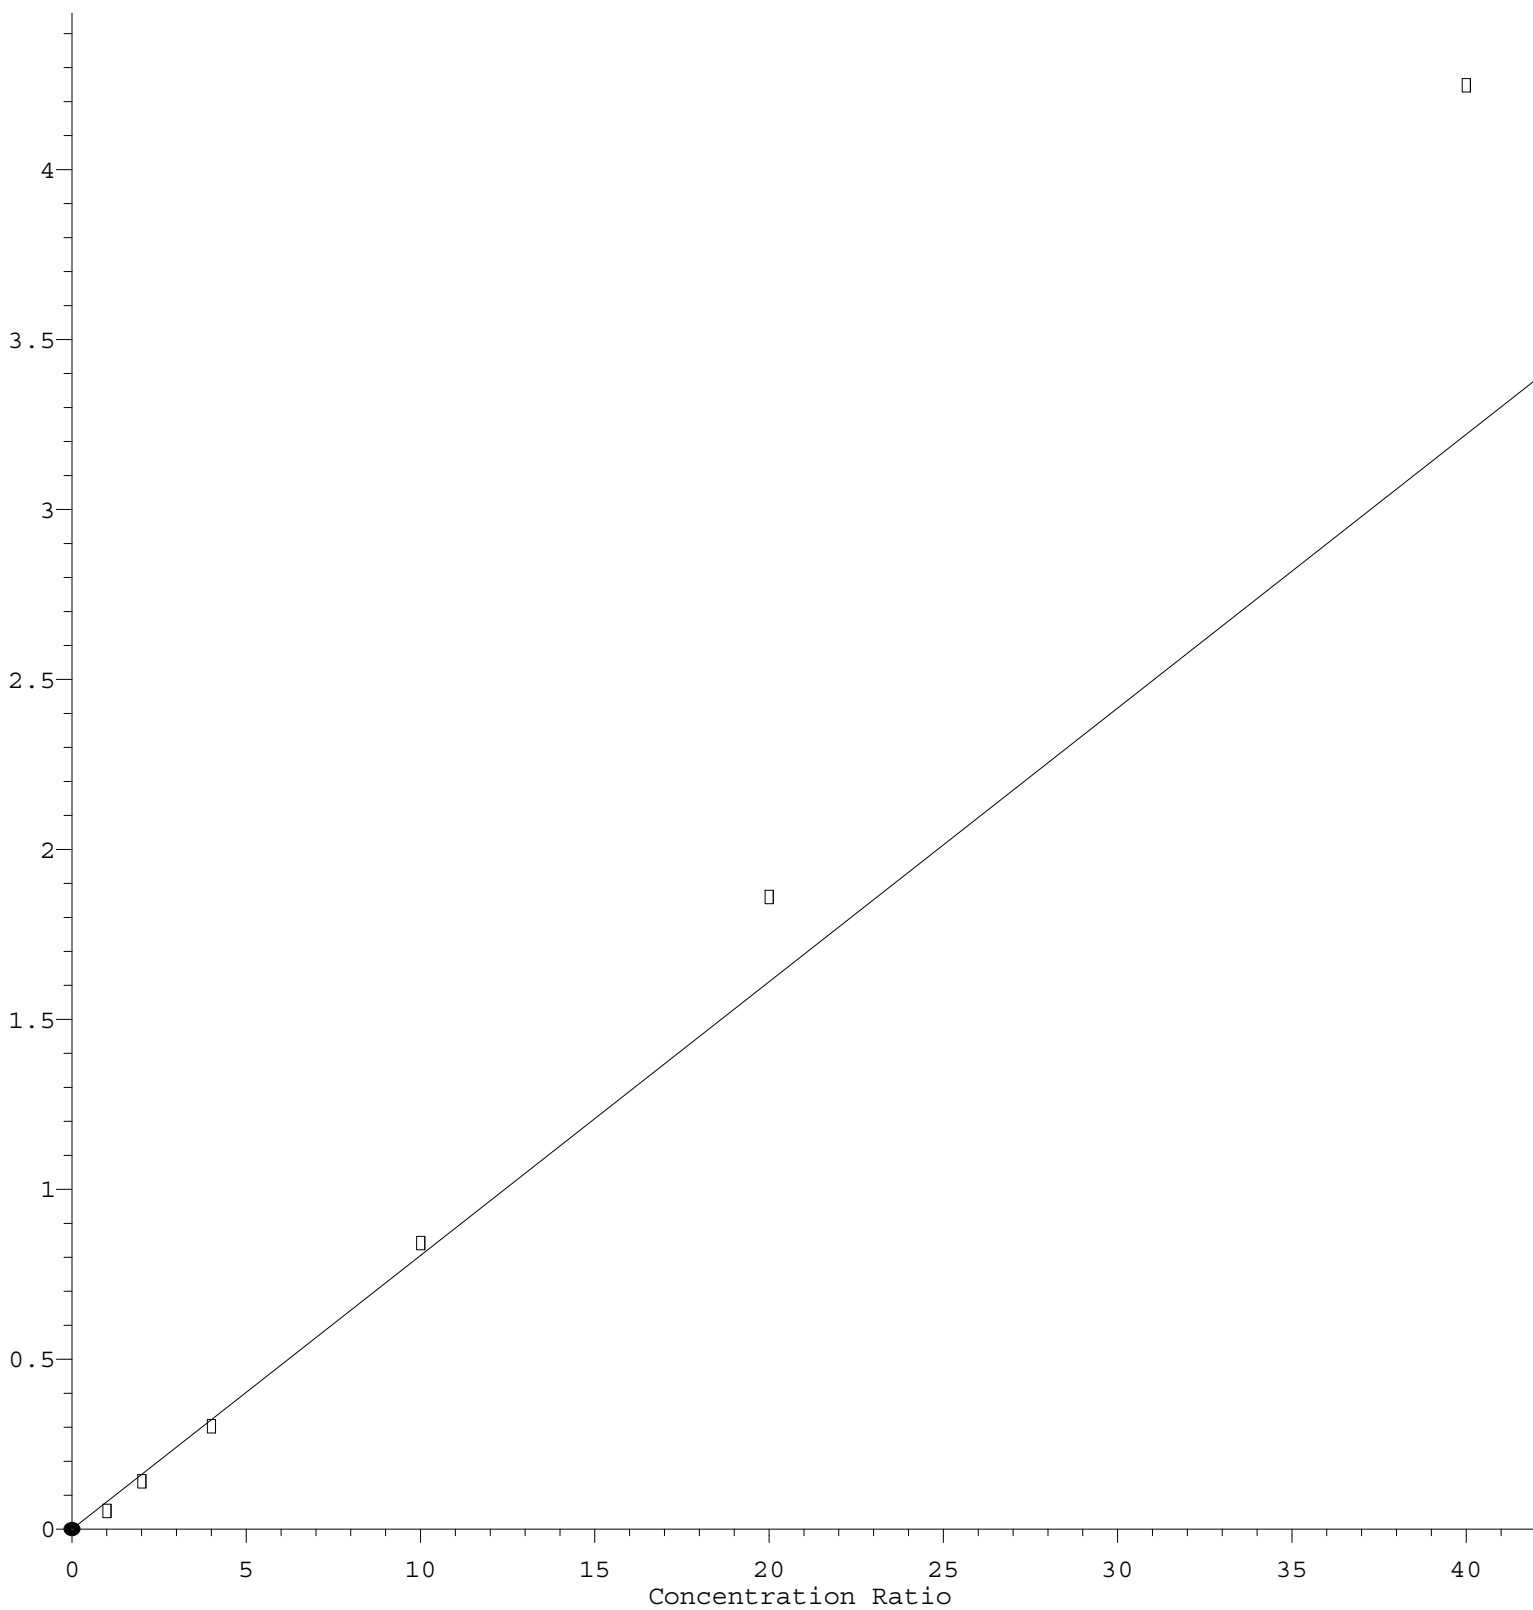

$$\text{Response} = 8.053\text{e-}002 * \text{Amt}$$


RF Rel Std Dev = 22.700% Curve Fit: Avg RF

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\524U030921DW.M

Calibration Table Last Updated: Thu Mar 11 12:50:28 2021

Hexachloroethane

Response Ratio

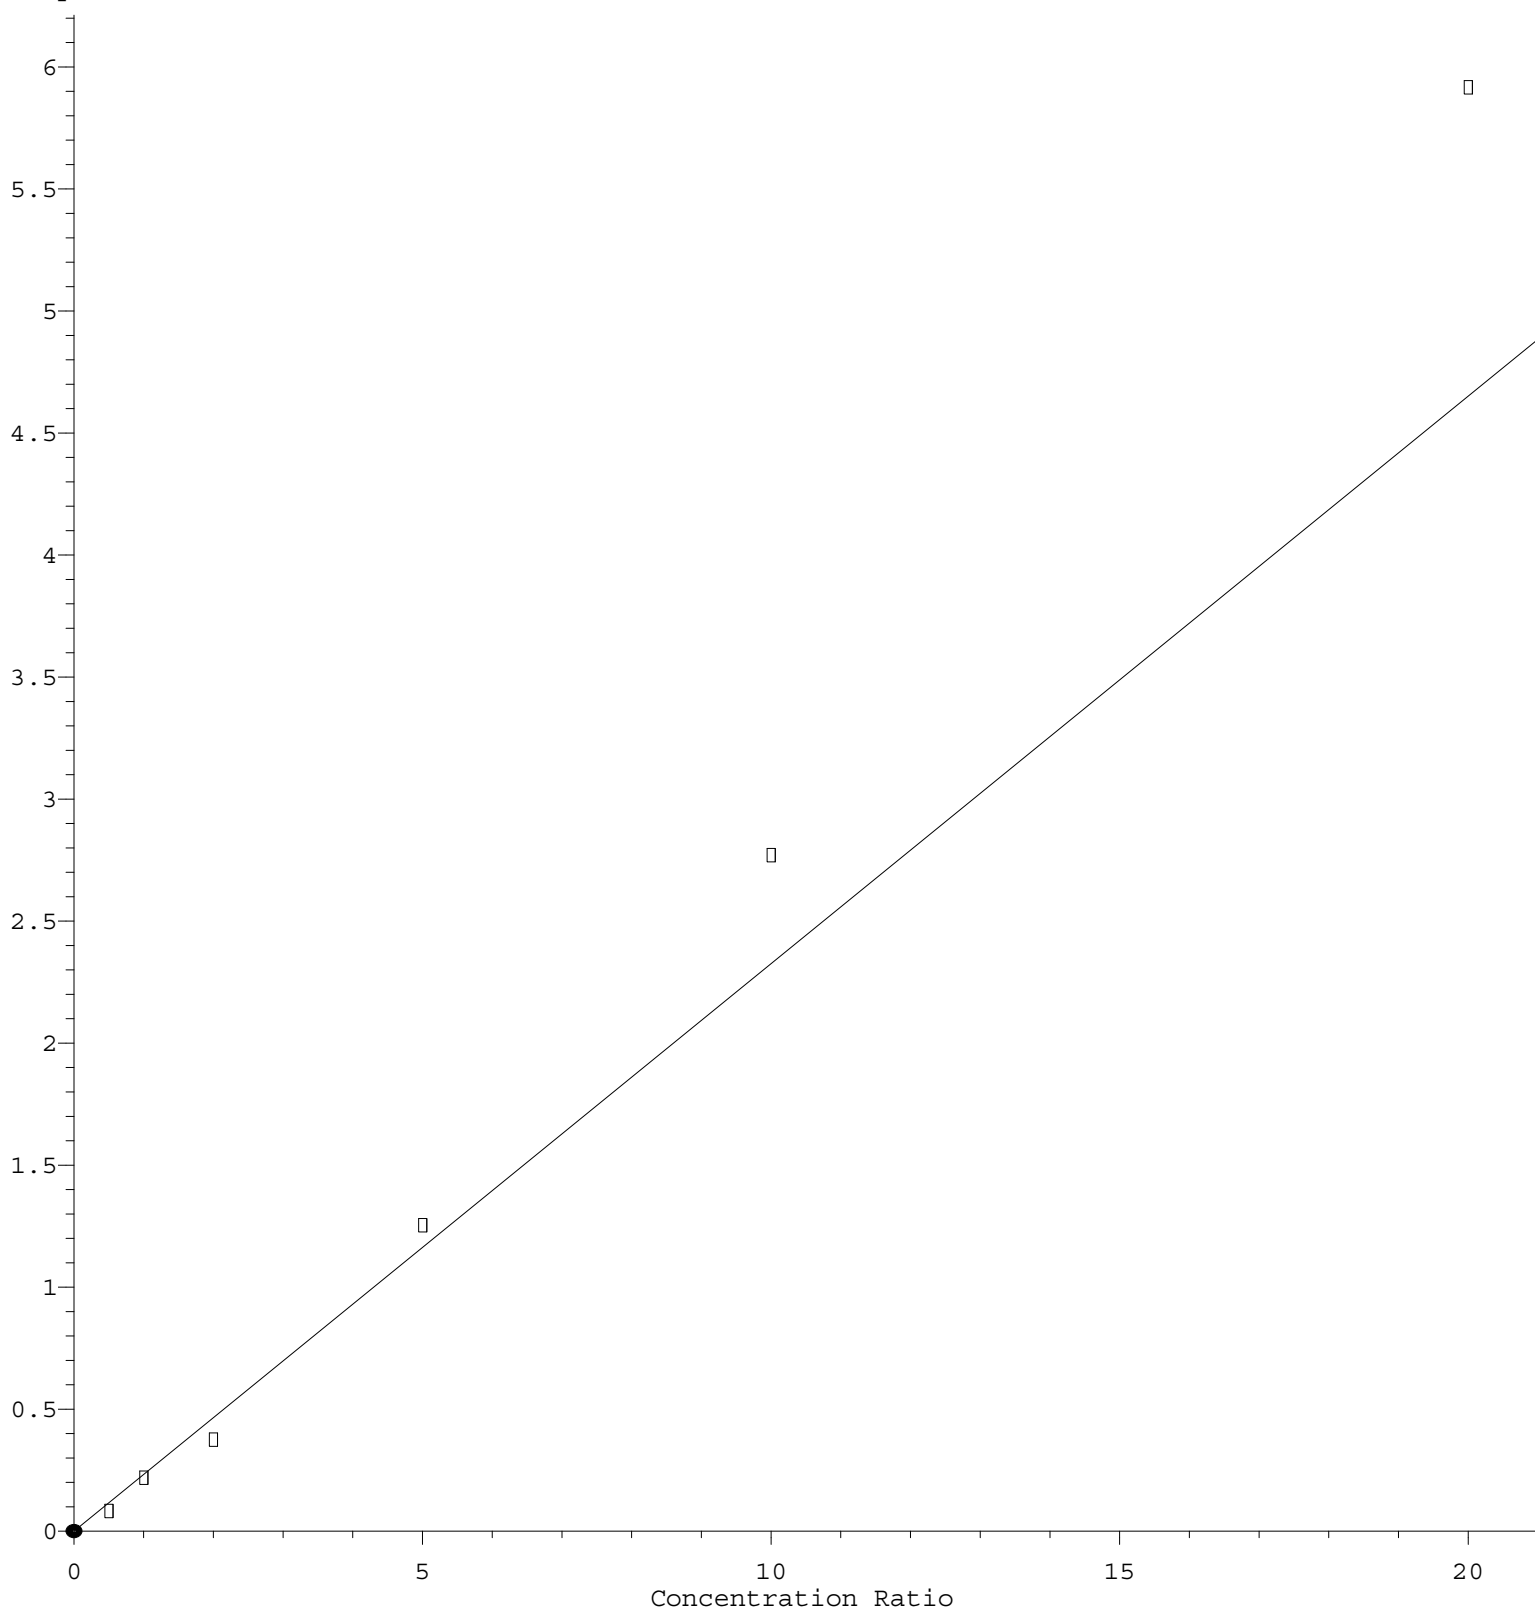

$$\text{Response} = 2.326\text{e-}001 * \text{Amt}$$


RF Rel Std Dev = 21.954% Curve Fit: Avg RF

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\524U030921DW.M

Calibration Table Last Updated: Thu Mar 11 12:50:28 2021

1,2,4-Trimethylbenzene

Response Ratio

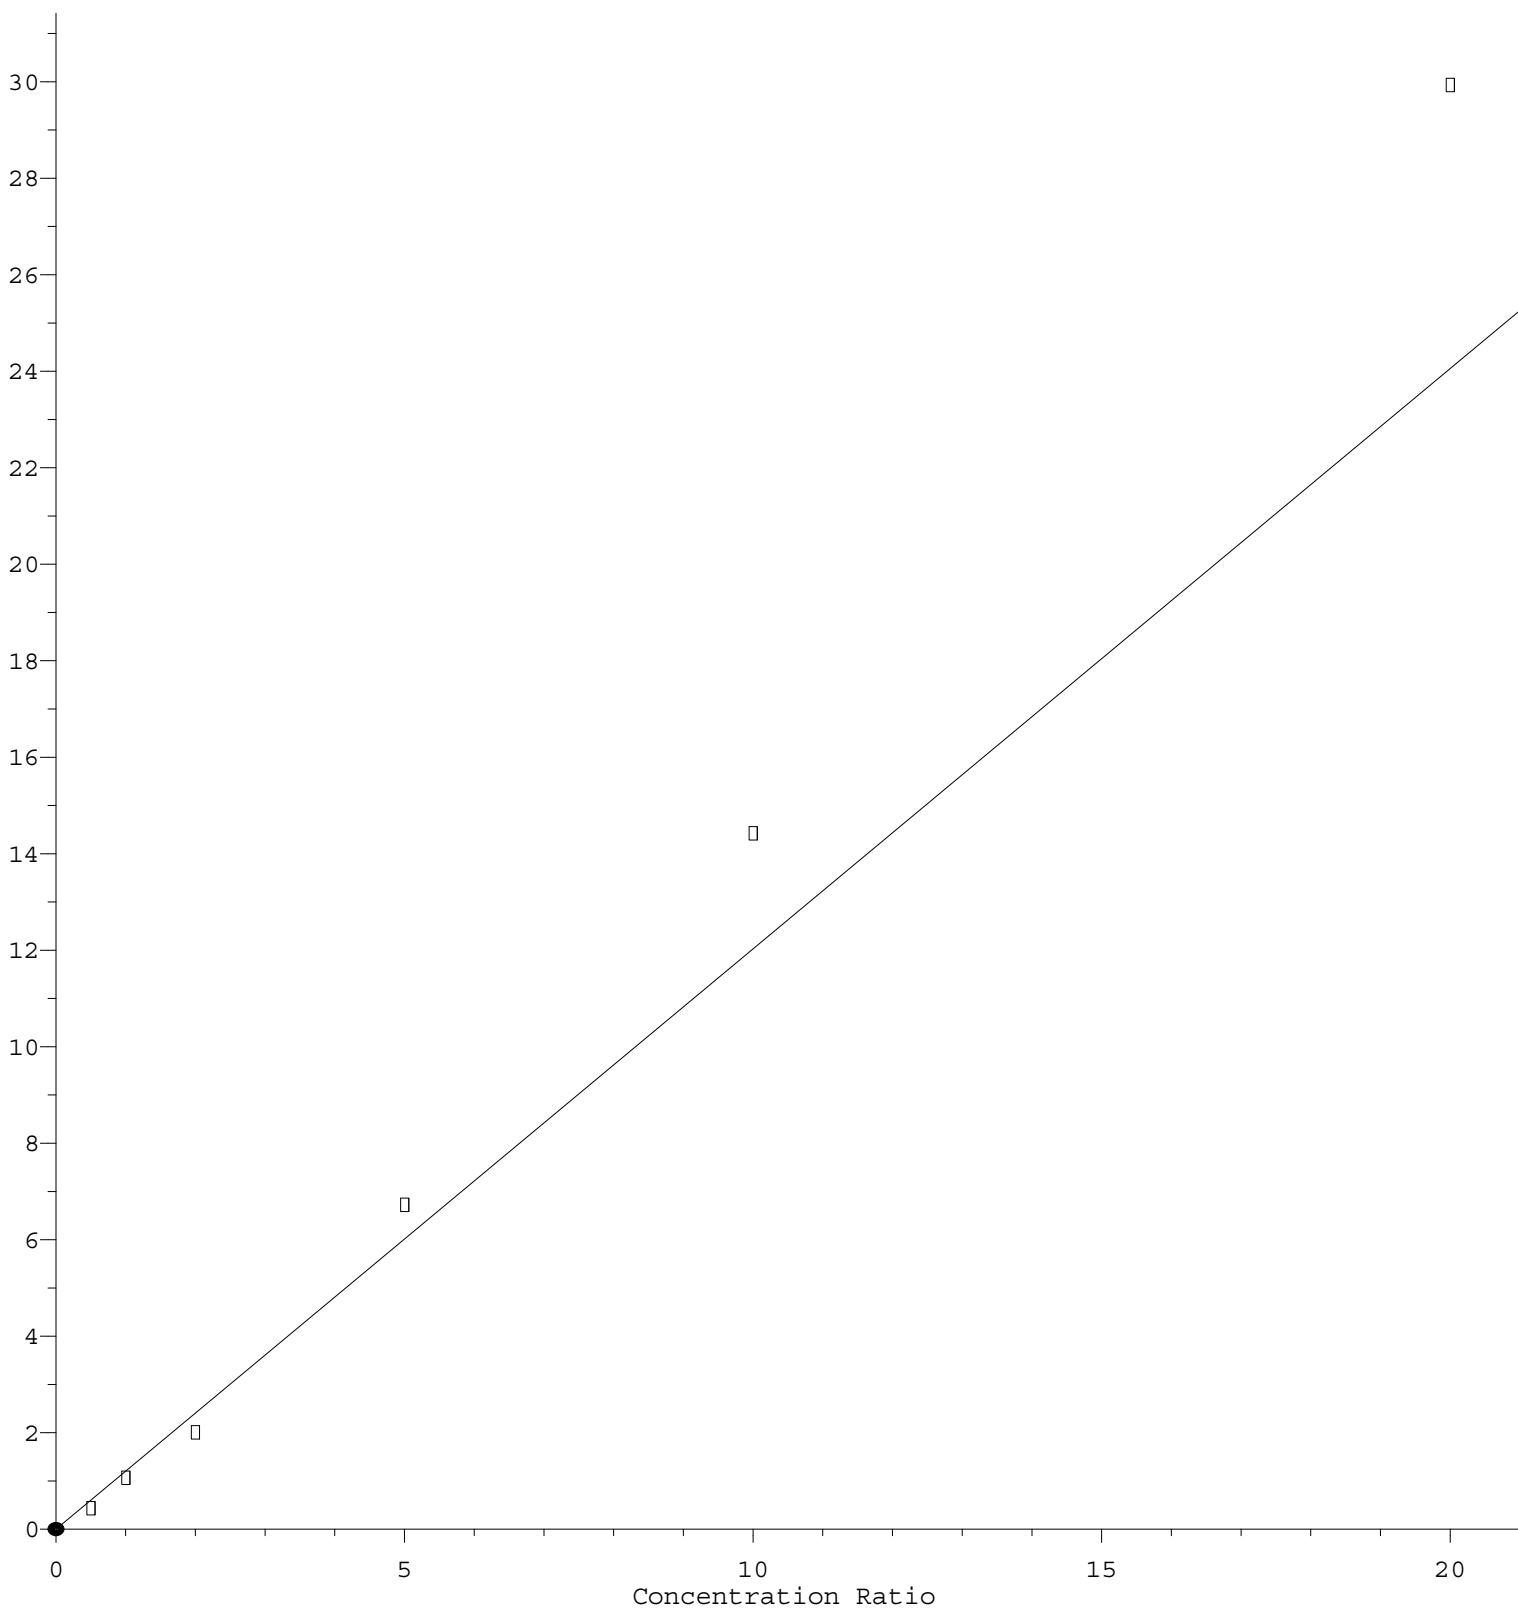

$$\text{Response} = 1.203\text{e}+000 * \text{Amt}$$


RF Rel Std Dev = 21.533% Curve Fit: Avg RF

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\524U030921DW.M

Calibration Table Last Updated: Thu Mar 11 12:50:28 2021

sec-Butylbenzene

Response Ratio

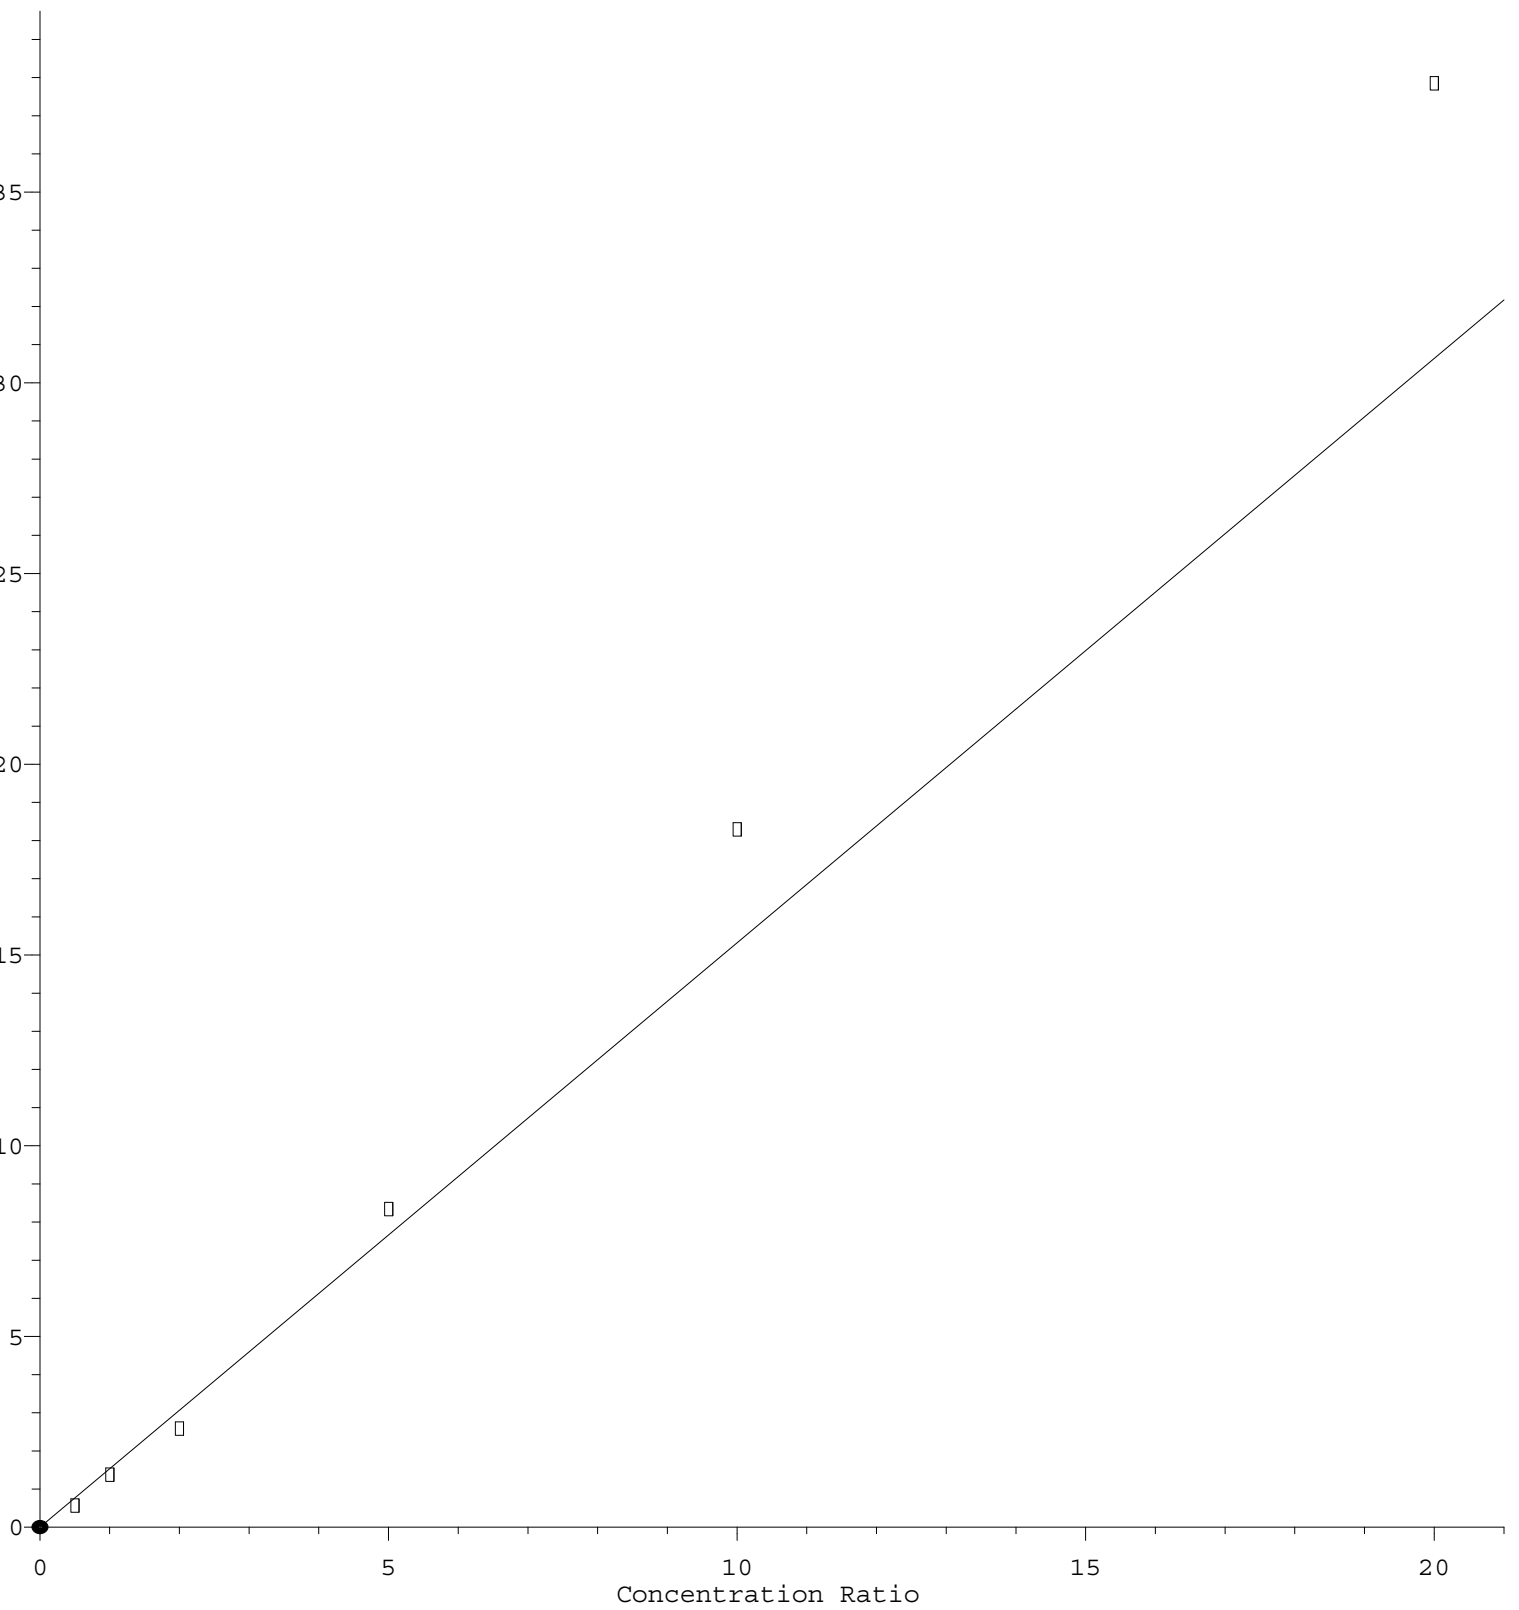


$$\text{Response} = 1.532\text{e}+000 * \text{Amt}$$

RF Rel Std Dev = 20.141% Curve Fit: Avg RF
 Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\524U030921DW.M
 Calibration Table Last Updated: Thu Mar 11 12:50:28 2021

Nitrobenzene

Response Ratio

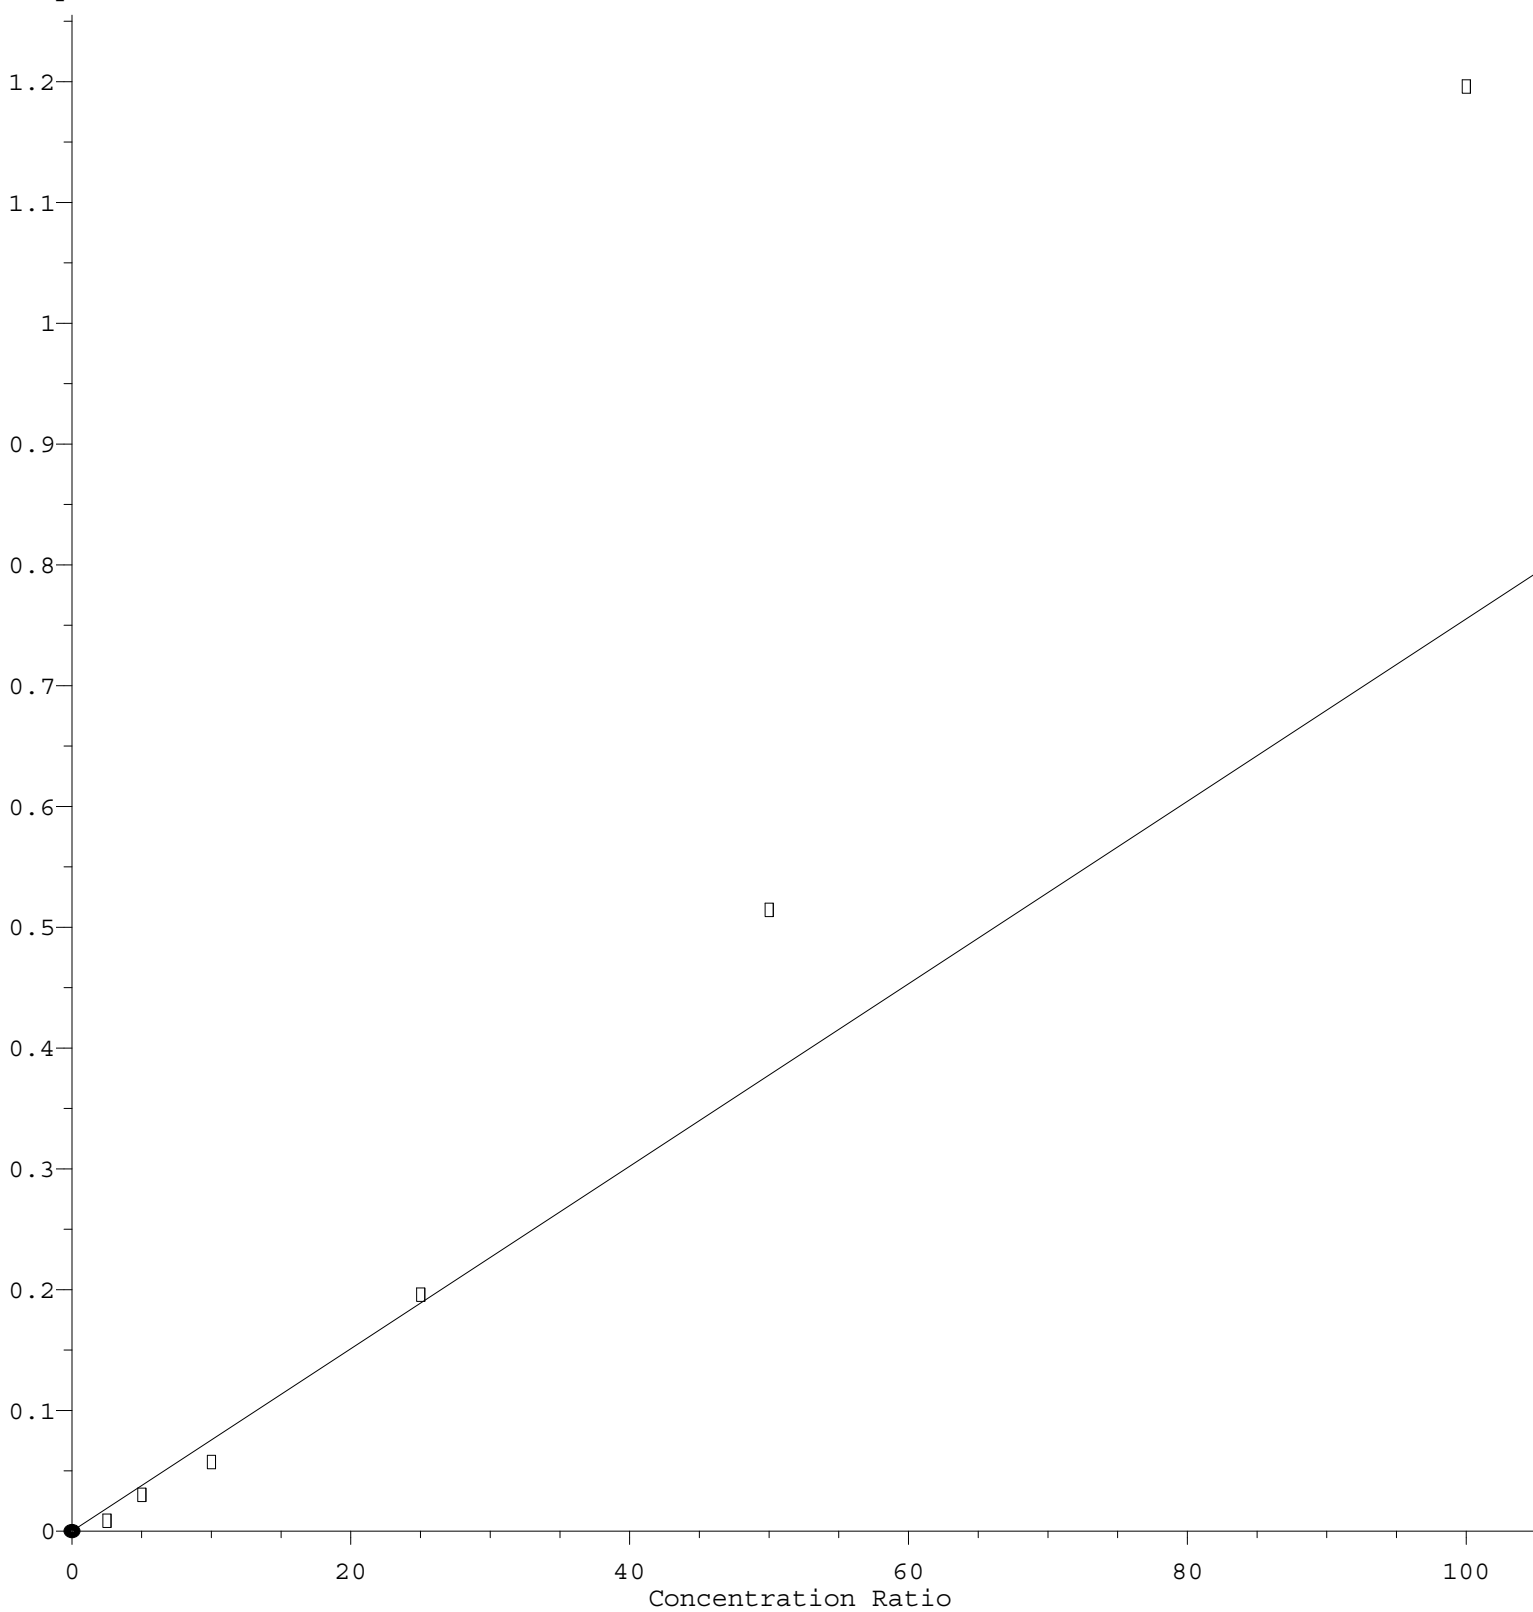

$$\text{Response} = 7.548\text{e-}003 * \text{Amt}$$


RF Rel Std Dev = 41.639% Curve Fit: Avg RF

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\524U030921DW.M

Calibration Table Last Updated: Thu Mar 11 12:50:28 2021

p-Isopropyltoluene

Response Ratio

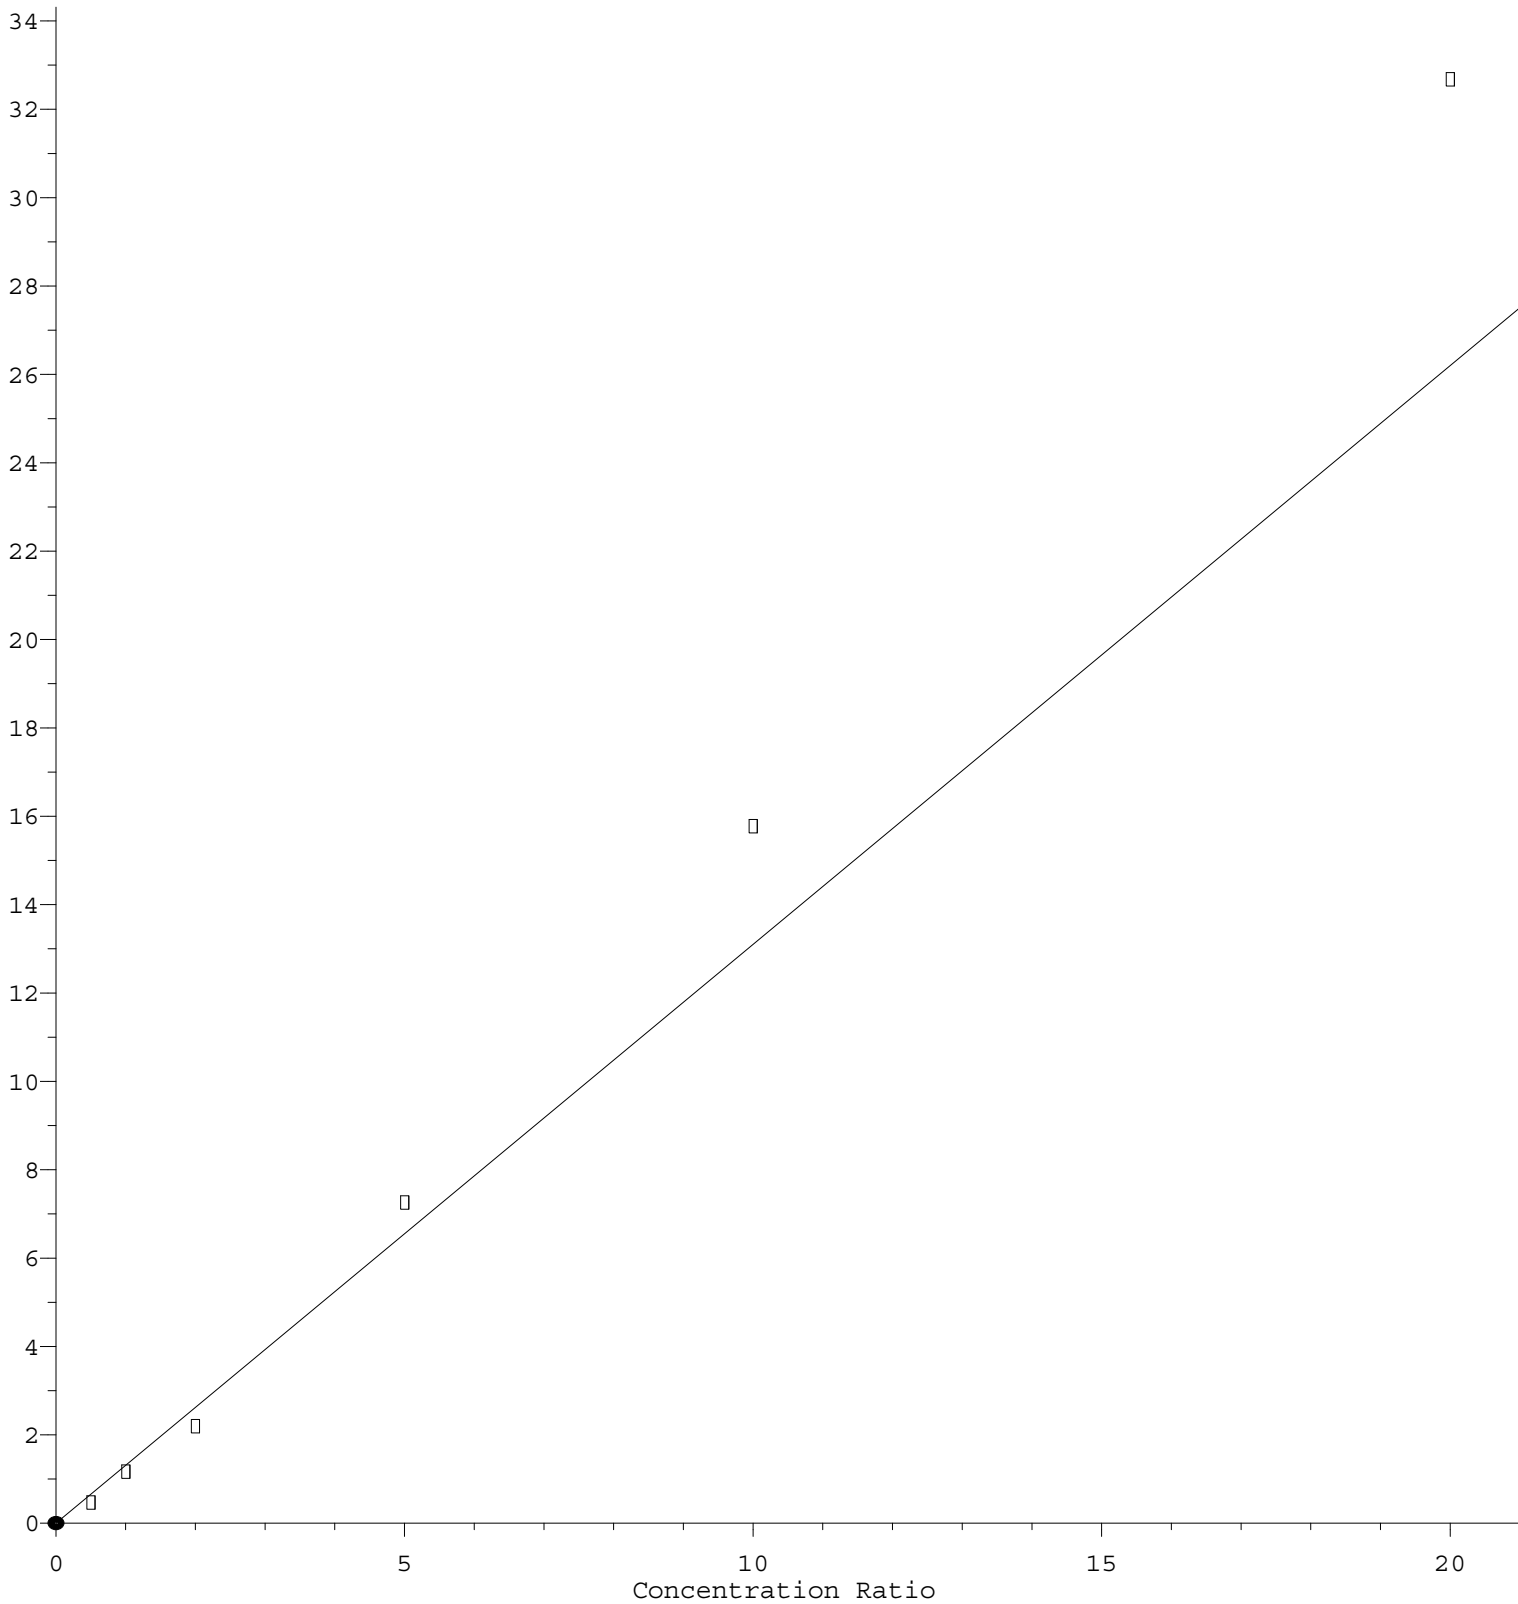

$$\text{Response} = 1.310\text{e}+000 * \text{Amt}$$


RF Rel Std Dev = 21.714% Curve Fit: Avg RF

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\524U030921DW.M

Calibration Table Last Updated: Thu Mar 11 12:50:28 2021

n-Butylbenzene

Response Ratio

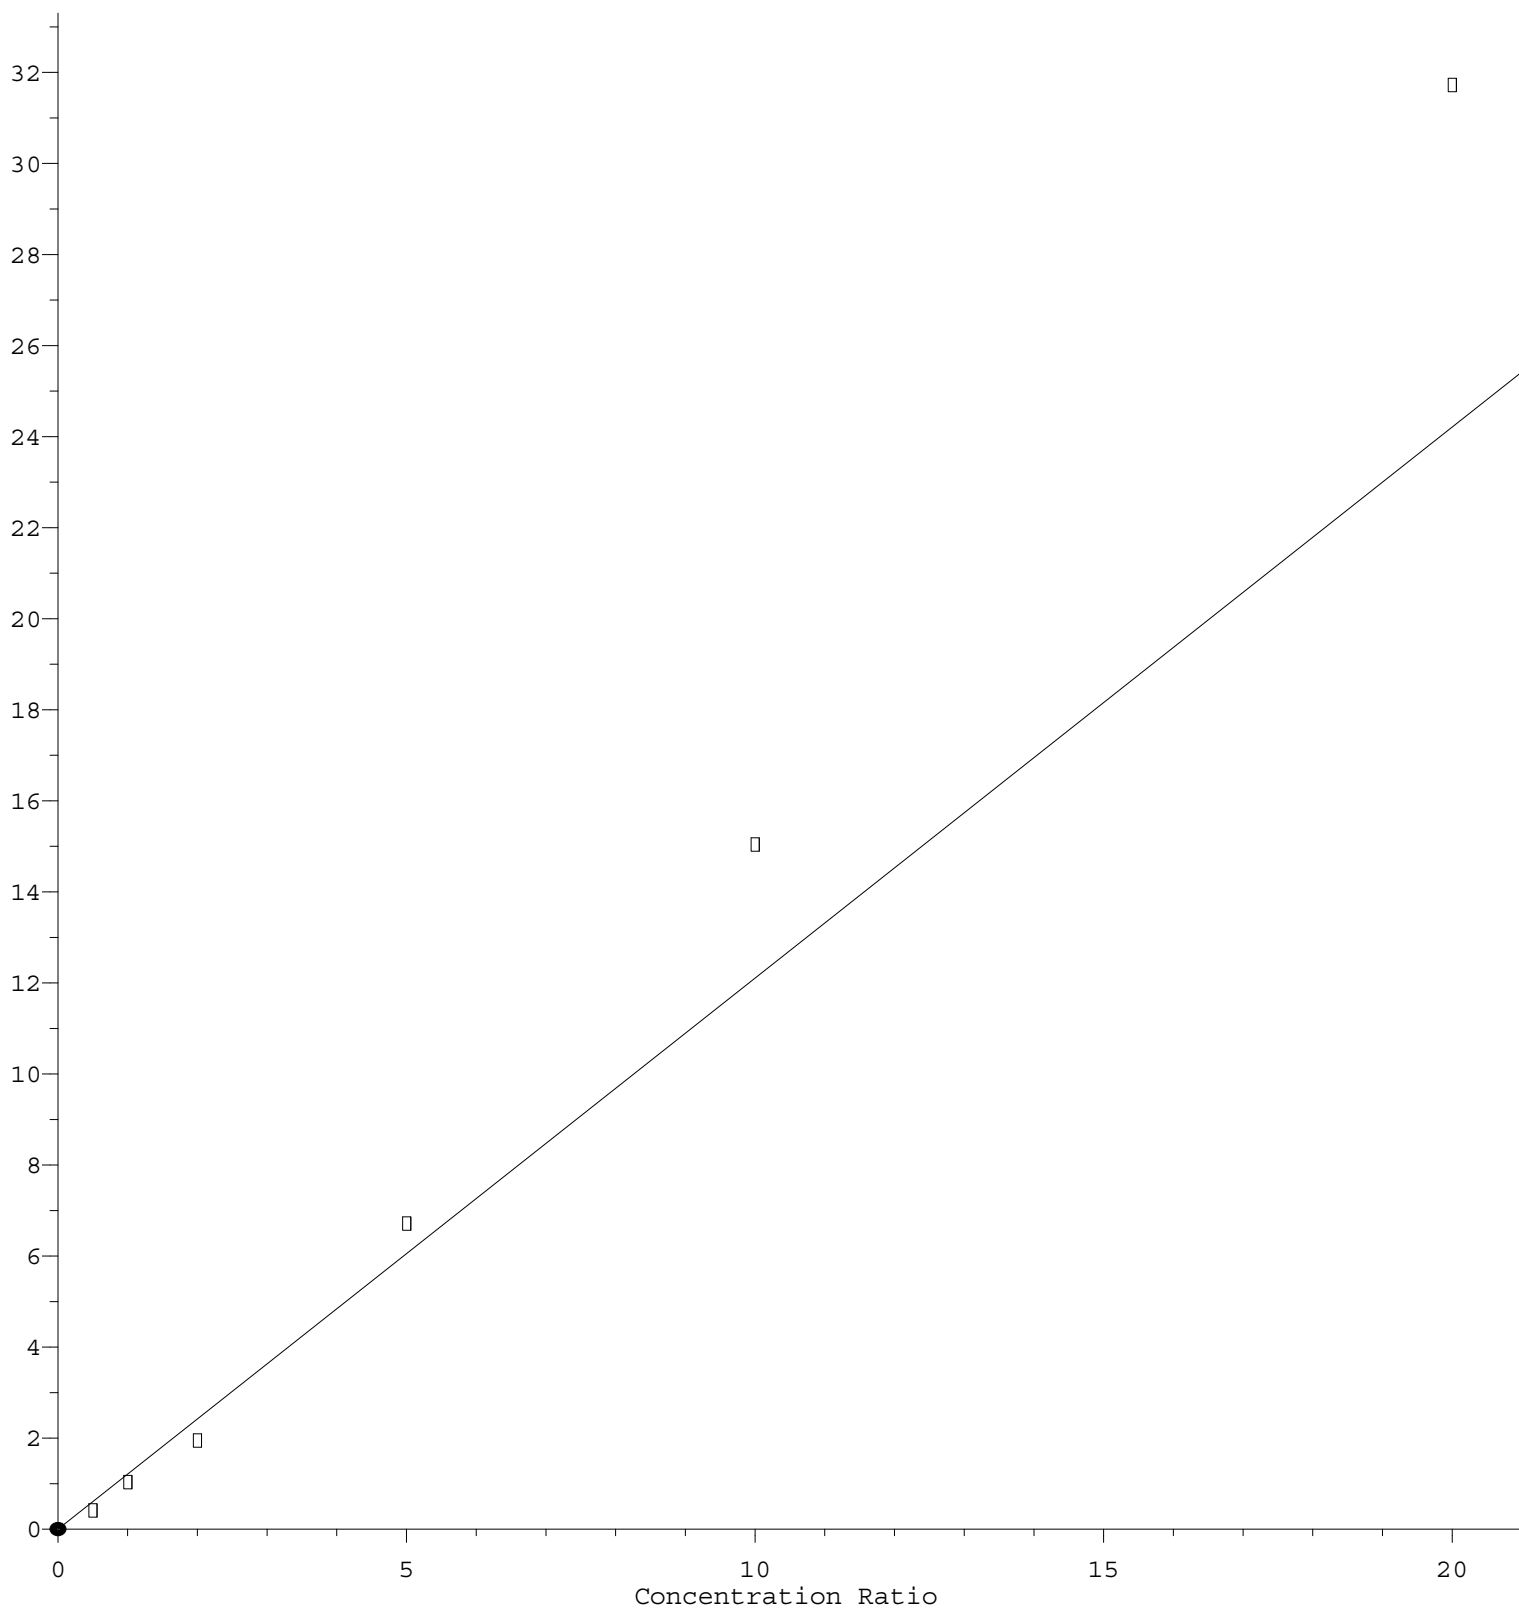

$$\text{Response} = 1.210\text{e}+000 * \text{Amt}$$


RF Rel Std Dev = 25.633% Curve Fit: Avg RF

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\524U030921DW.M

Calibration Table Last Updated: Thu Mar 11 12:50:28 2021

1,2-Dibromo-3-Chloropropane

Response Ratio

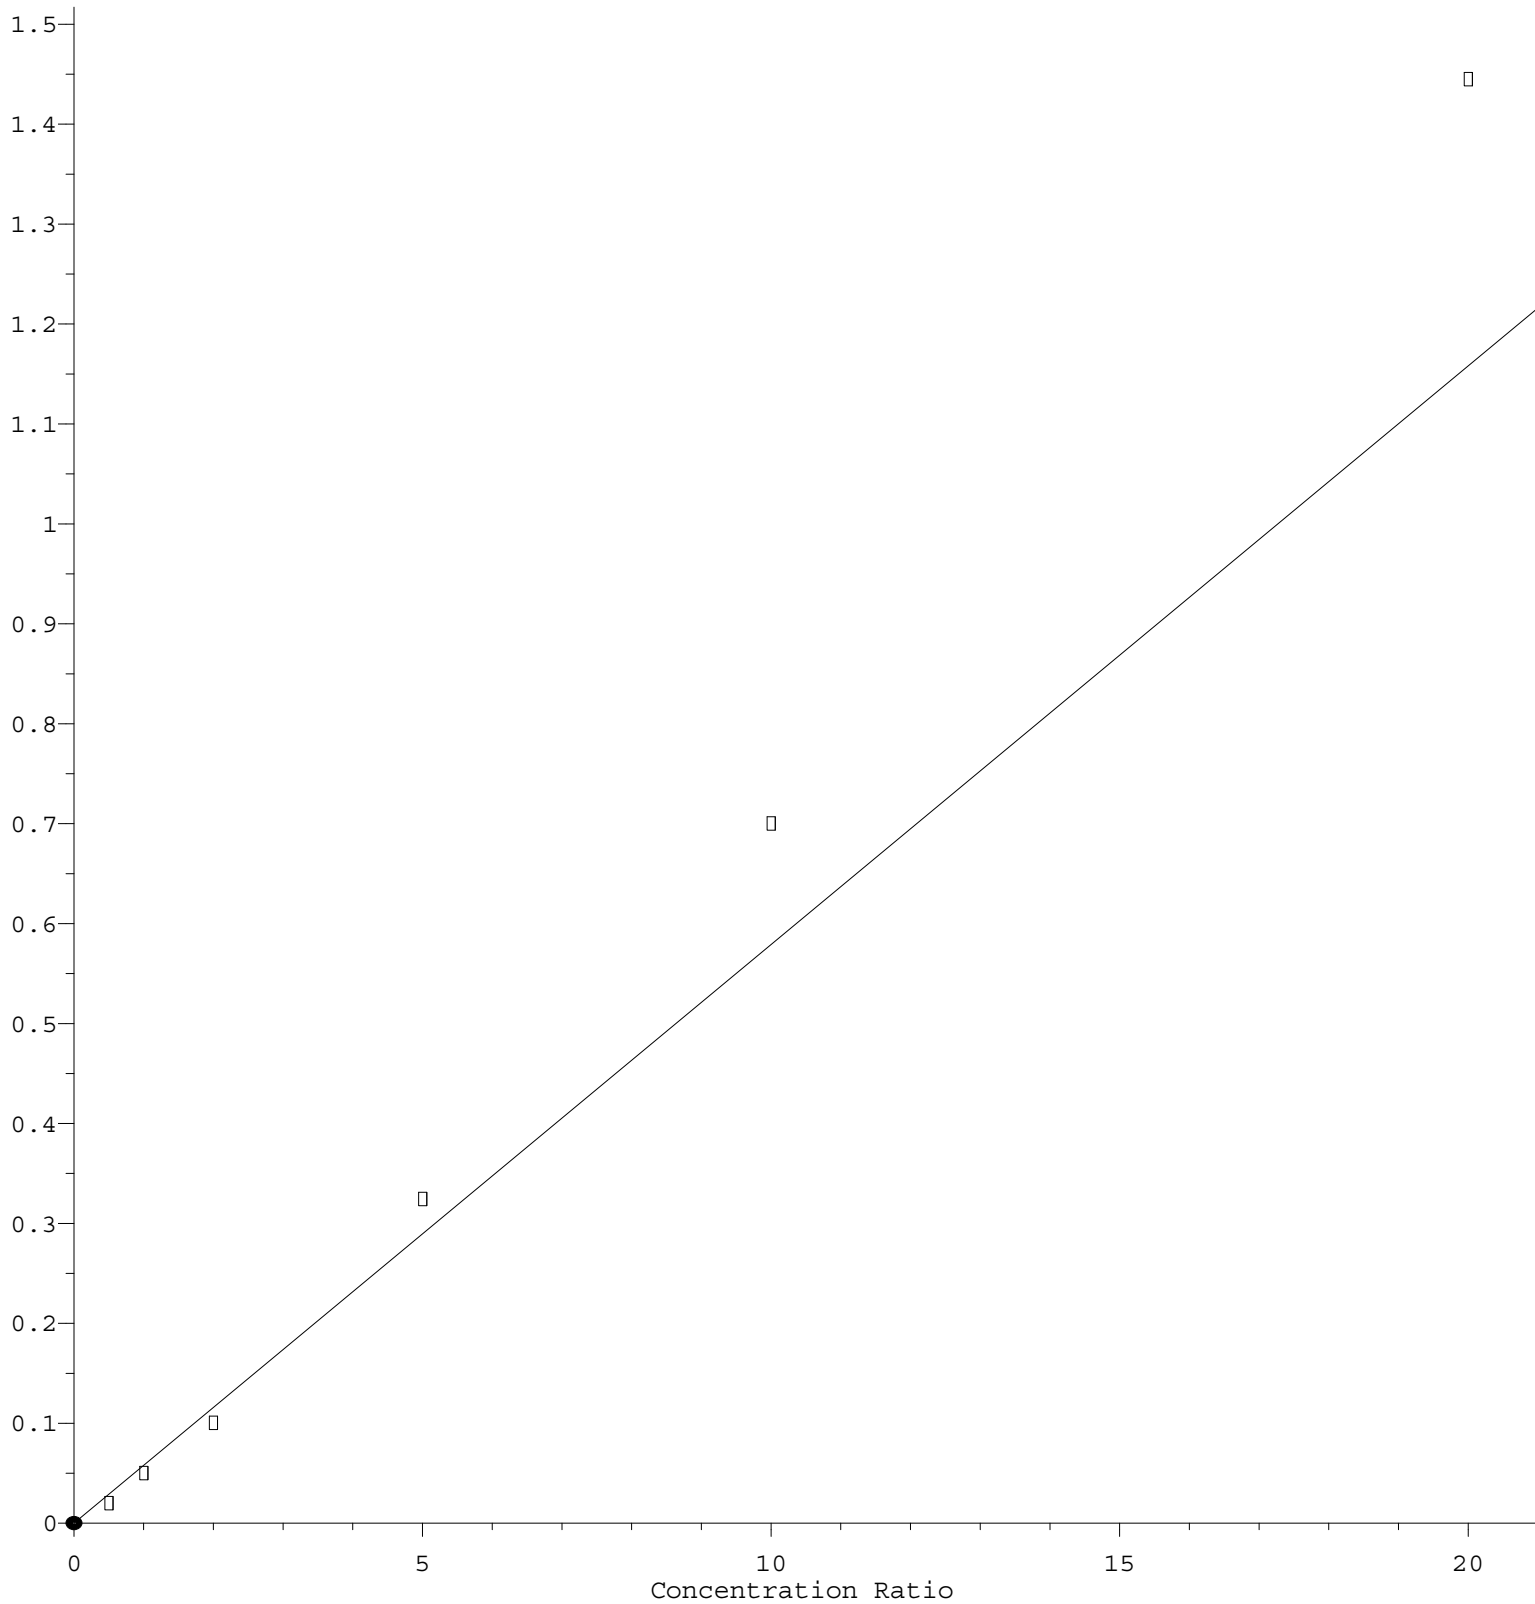

$$\text{Response} = 5.792\text{e-}002 * \text{Amt}$$


RF Rel Std Dev = 22.351% Curve Fit: Avg RF

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\524U030921DW.M

Calibration Table Last Updated: Thu Mar 11 12:50:28 2021

1,2,4-Trichlorobenzene

Response Ratio

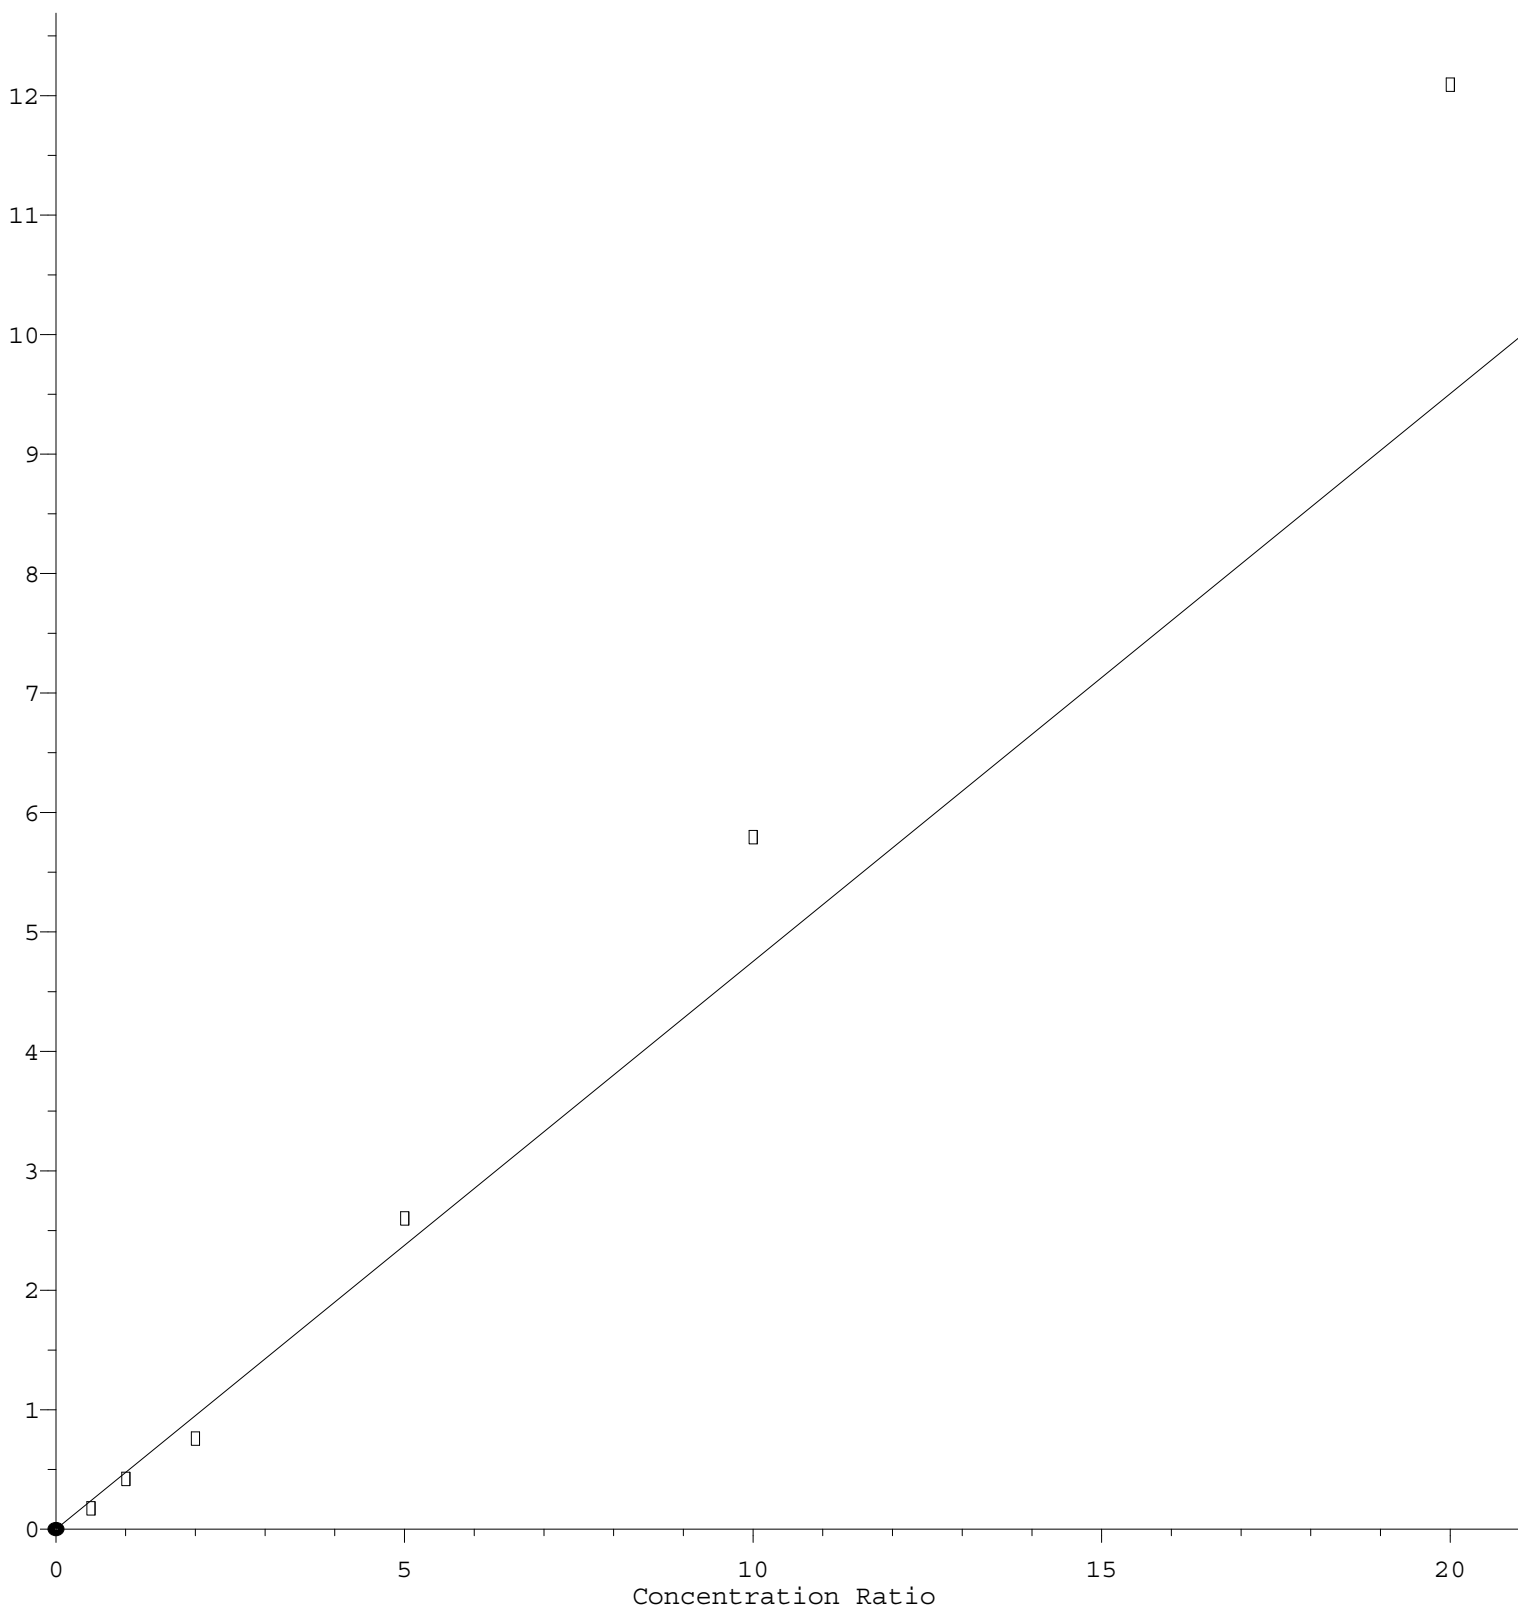

$$\text{Response} = 4.754\text{e-}001 * \text{Amt}$$


RF Rel Std Dev = 22.631% Curve Fit: Avg RF

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\524U030921DW.M

Calibration Table Last Updated: Thu Mar 11 12:50:28 2021

Naphthalene

Response Ratio

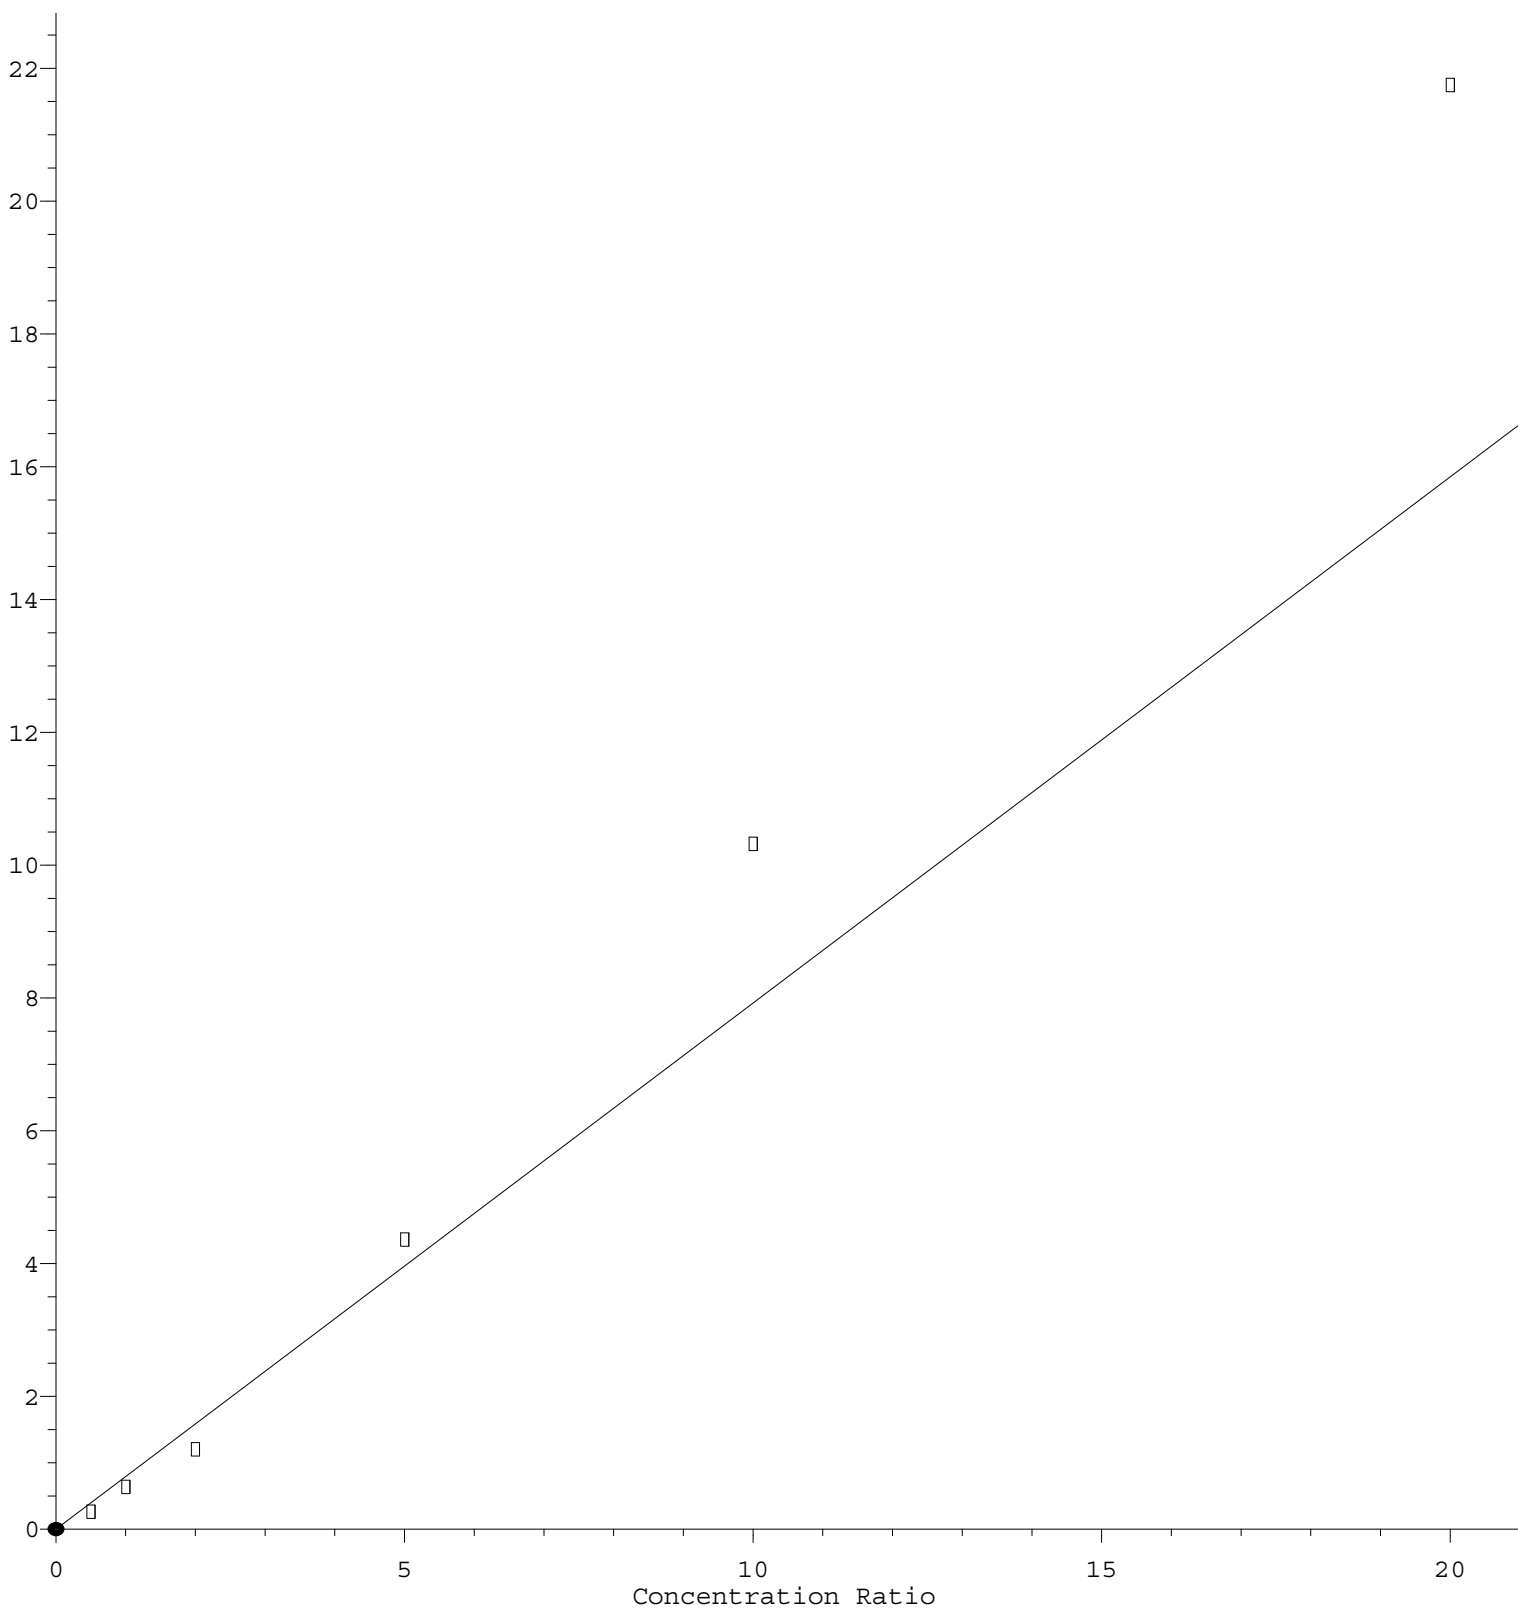

$$\text{Response} = 7.925\text{e-}001 * \text{Amt}$$


RF Rel Std Dev = 29.999% Curve Fit: Avg RF

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\524U030921DW.M

Calibration Table Last Updated: Thu Mar 11 12:50:28 2021

1,2,3-Trichlorobenzene

Response Ratio

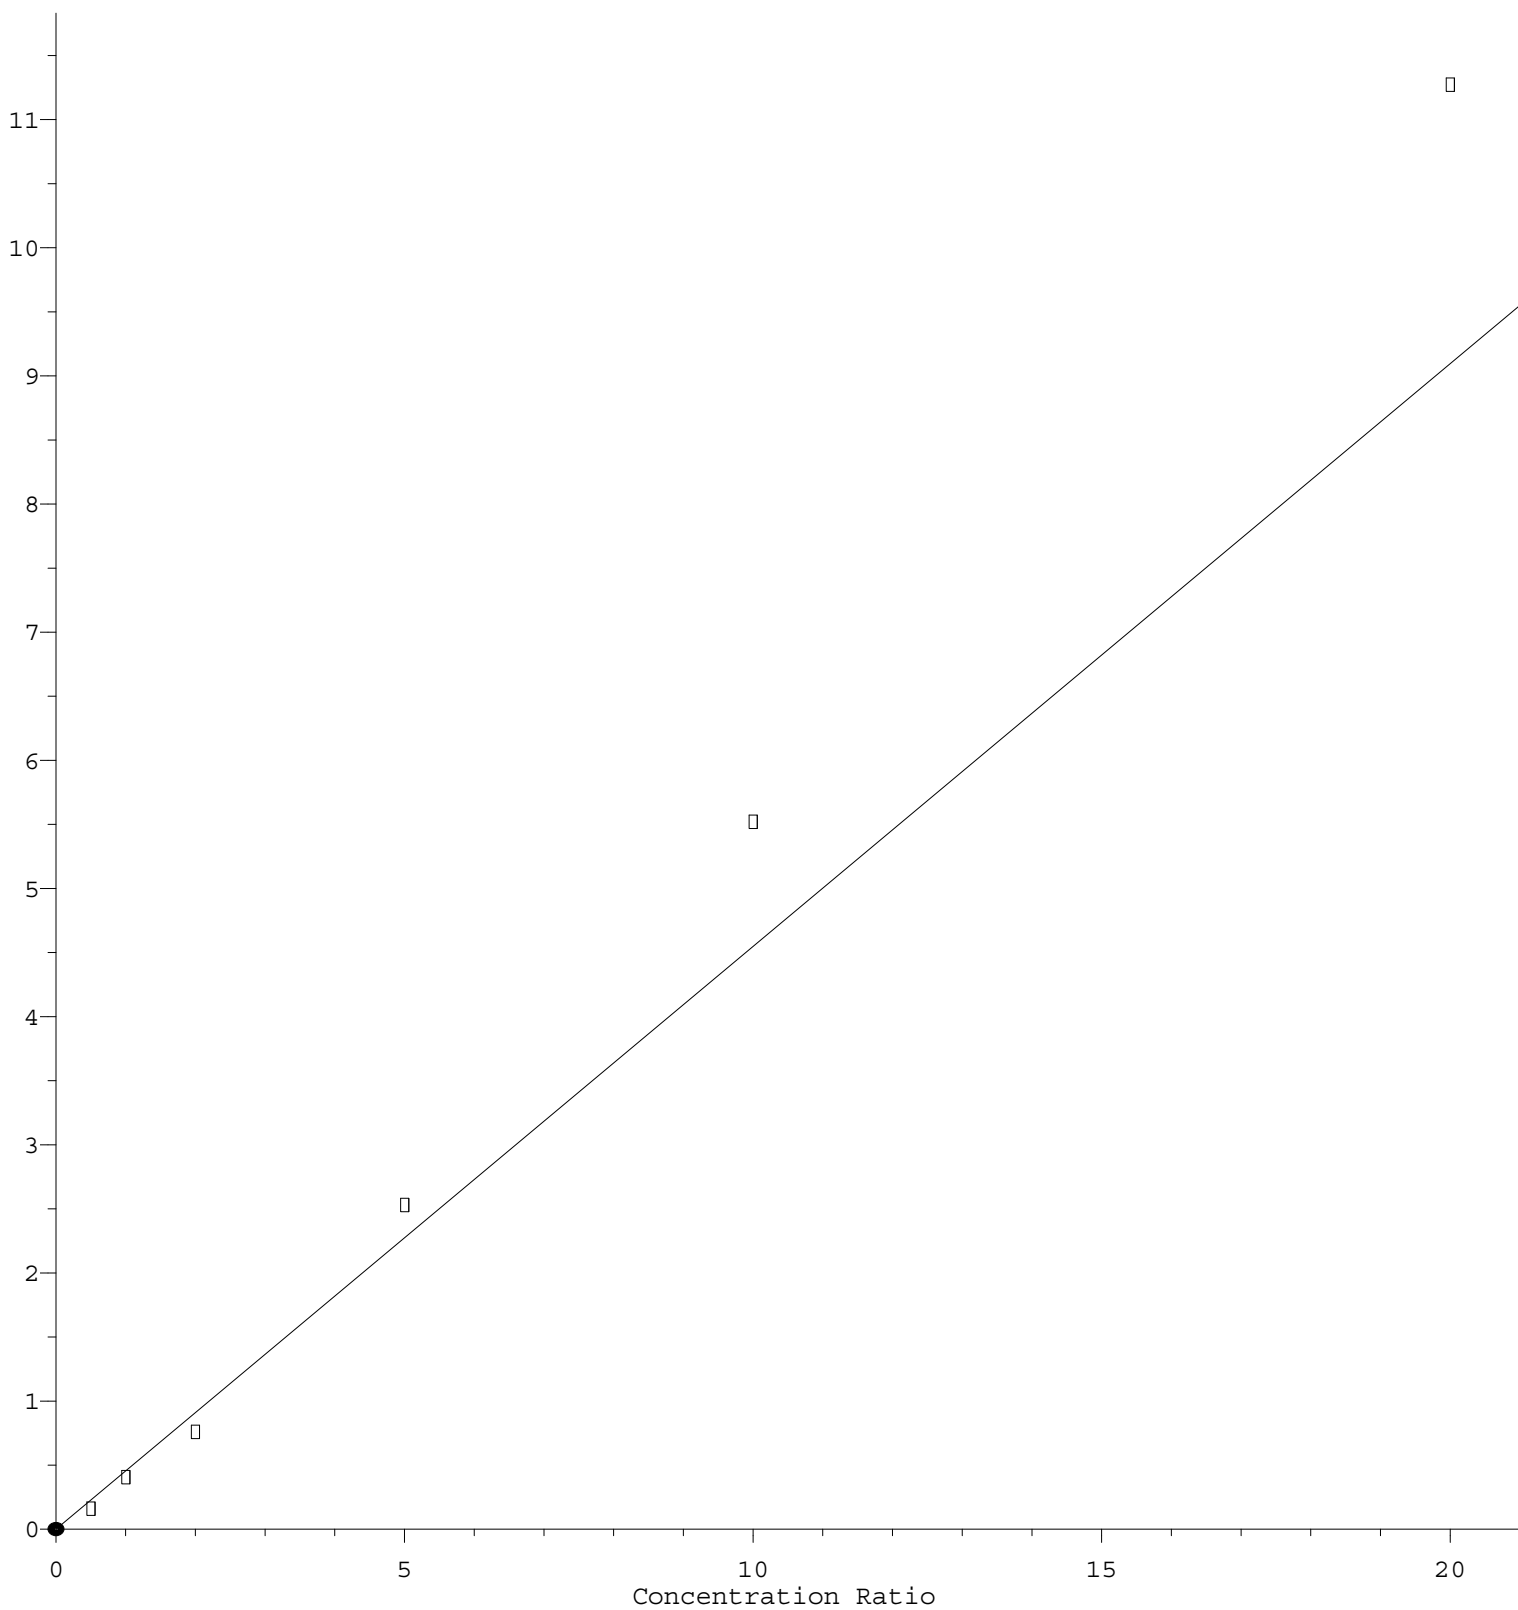

$$\text{Response} = 4.546\text{e-}001 * \text{Amt}$$

RF Rel Std Dev = 21.989% Curve Fit: Avg RF

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\524U030921DW.M

Calibration Table Last Updated: Thu Mar 11 12:50:28 2021