

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030921\
 Data File : VU042539.D
 Acq On : 09 Mar 2021 14:34
 Operator : SY/MD
 Sample : VU0309WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK23

Quant Time: Mar 11 12:51:20 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U030921DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Mar 11 12:50:28 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Fluorobenzene	6.125	96	20683	1.00	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.645	95	7491	0.82	ug/l	0.00
Spiked Amount 1.000			Recovery	=	82.00%	
68) 1,2-Dichlorobenzene-d4	12.201	152	7624	0.81	ug/l	0.00
Spiked Amount 1.000			Recovery	=	81.00%	
Target Compounds						
15) Methylene Chloride	3.054	84	1031	0.17	ug/l	# 83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030921\
Data File : VU042539.D
Acq On : 09 Mar 2021 14:34
Operator : SY/MD
Sample : VU0309WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK23

Quant Time: Mar 11 12:51:20 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U030921DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu Mar 11 12:50:28 2021
Response via : Initial Calibration




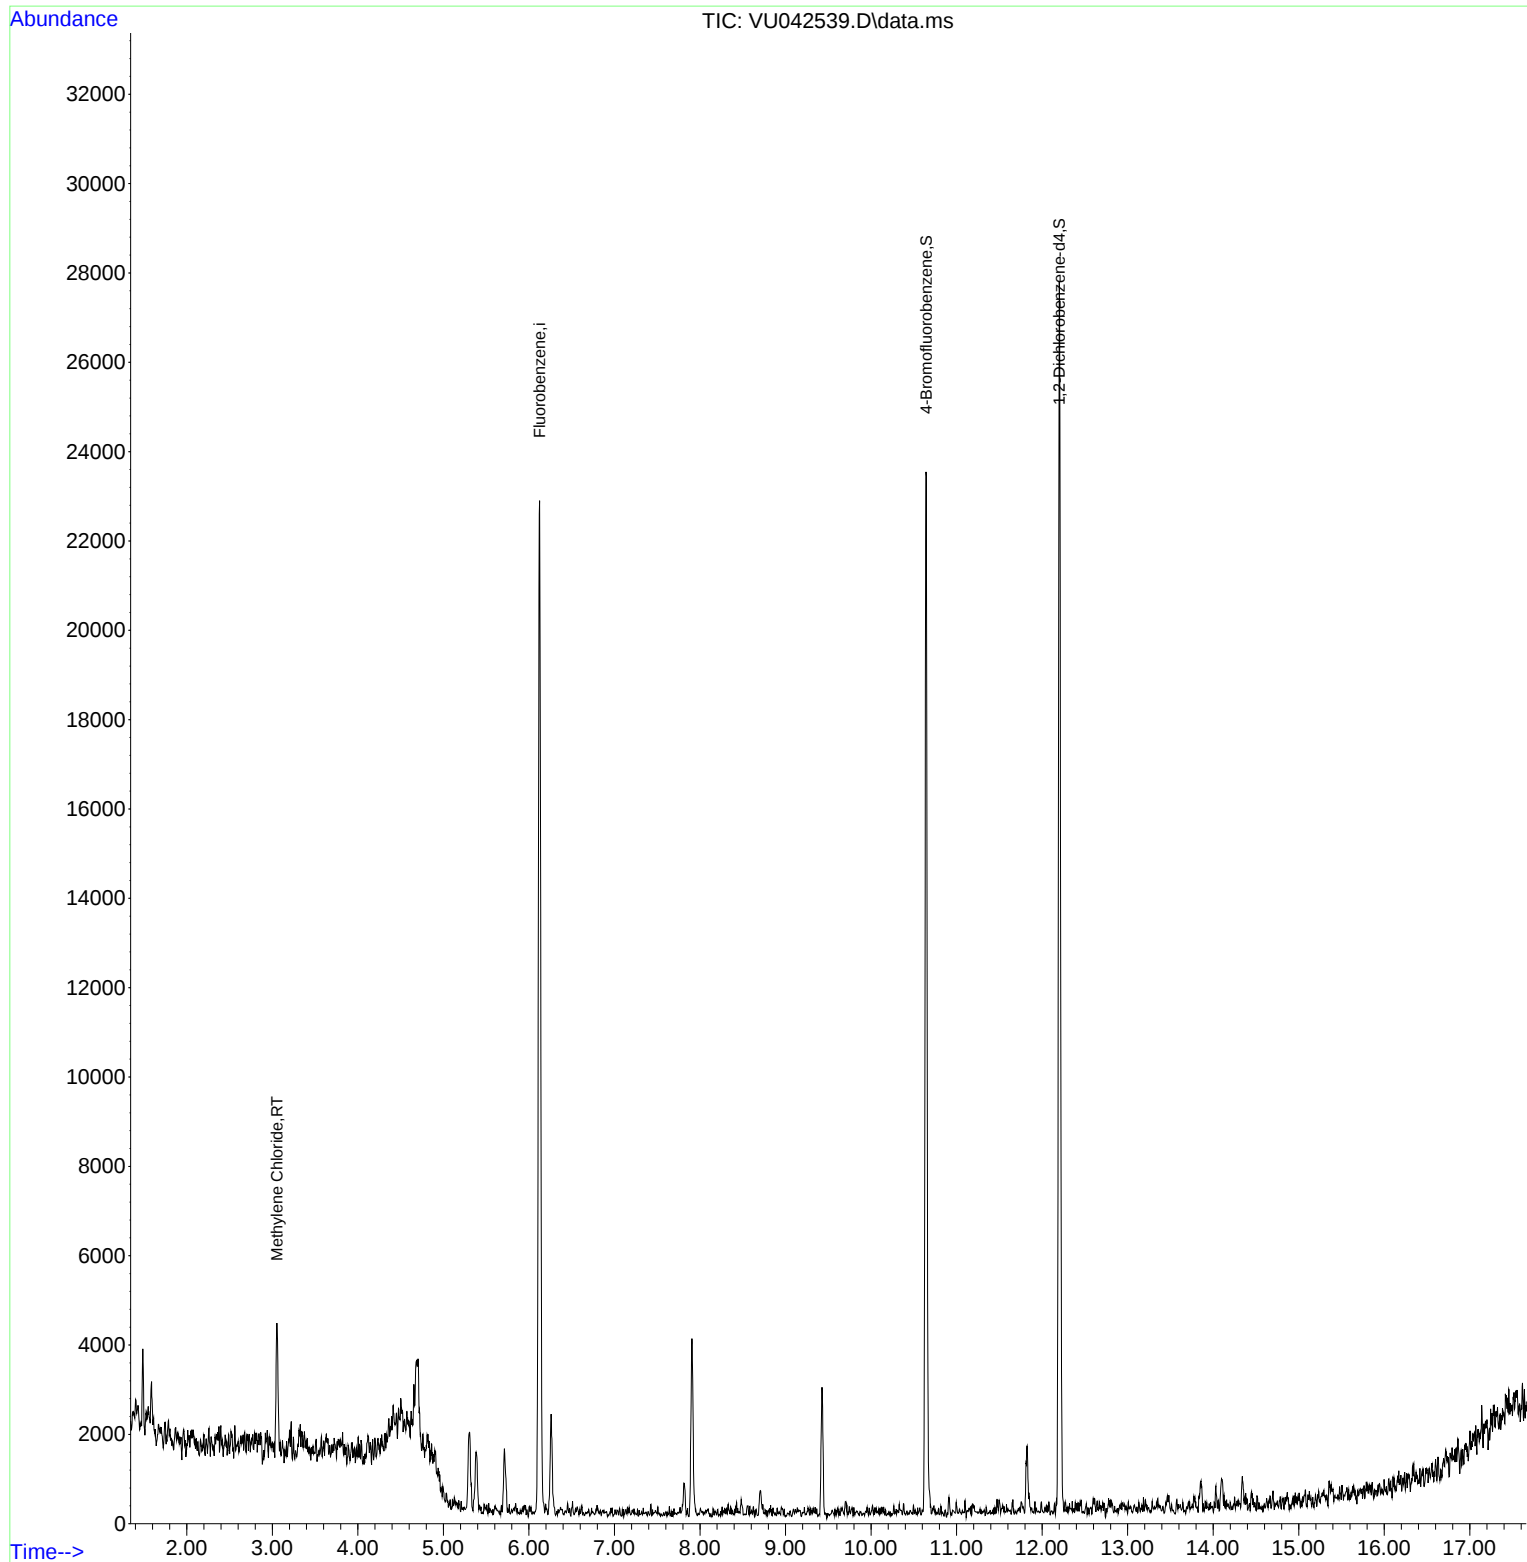


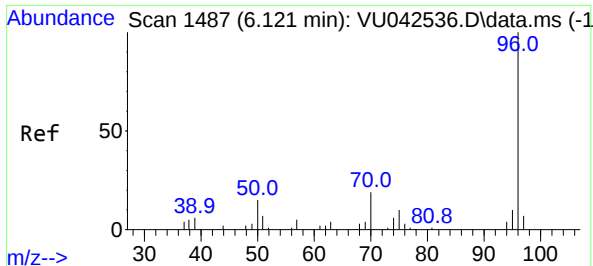

#1
Fluorobenzene
Concen: 1.00 ug/l
RT: 6.125 min Scan# 1488
Delta R.T. 0.004 min
Lab File: VU042539.D
Acq: 09 Mar 2021 14:34




Instrument :
MSVOA_U
ClientSampled :
VBLK23


Tgt Ion: 96	Resp: 20683
Ion Ratio	Lower Upper
96 100	
70 18.6	16.3 24.5
95 8.9	7.0 10.4
97 5.5	0.0 0.0#

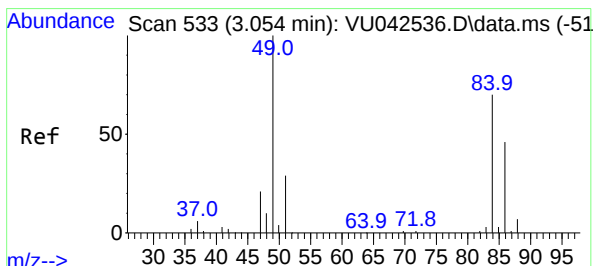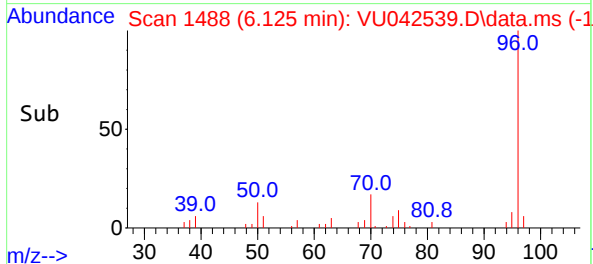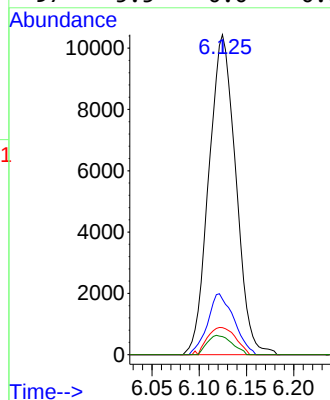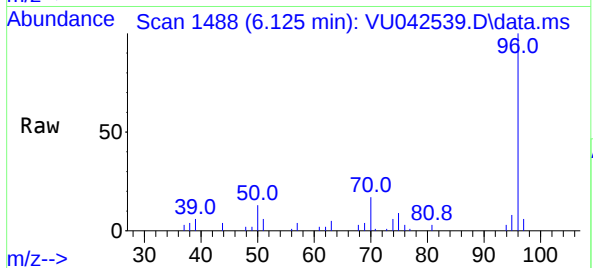

#15
Methylene Chloride
Concen: 0.17 ug/l
RT: 3.054 min Scan# 533
Delta R.T. -0.000 min
Lab File: VU042539.D
Acq: 09 Mar 2021 14:34

Tgt Ion: 84	Resp: 1031
Ion Ratio	Lower Upper
84 100	
49 121.4	114.6 172.0
51 44.0	0.0 83.0
86 48.0	52.3 78.5#


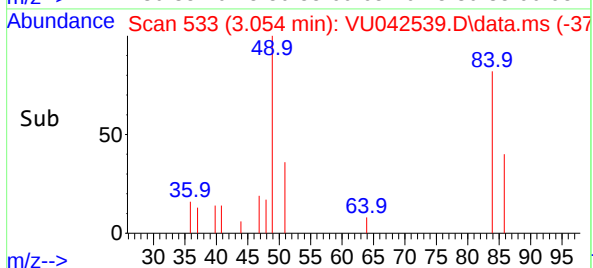
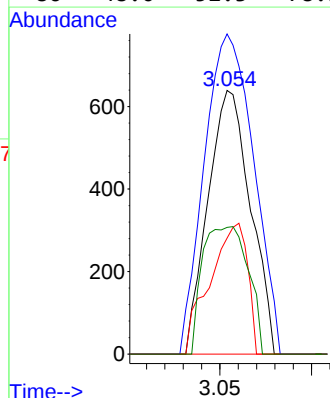
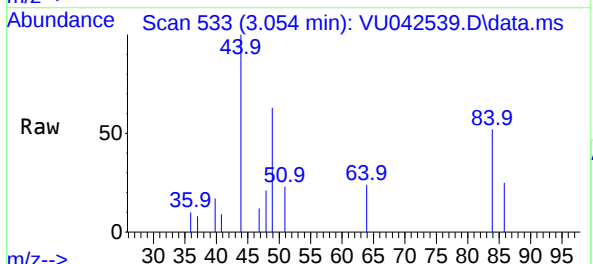


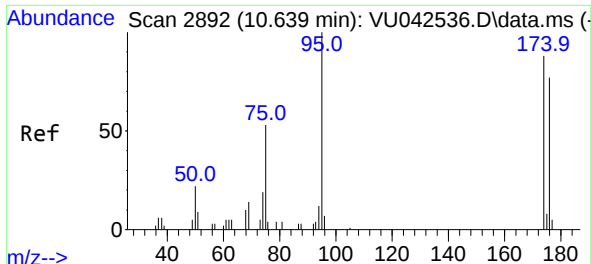

#57
4-Bromofluorobenzene
Concen: 0.82 ug/l
RT: 10.645 min Scan# 2894
Delta R.T. 0.006 min
Lab File: VU042539.D
Acq: 09 Mar 2021 14:34

Instrument :
MSVOA_U
ClientSampleId :
VBLK23

Tgt Ion: 95 Resp: 7491
Ion Ratio Lower Upper
95 100
174 90.7 73.1 109.7
176 86.7 63.4 95.2

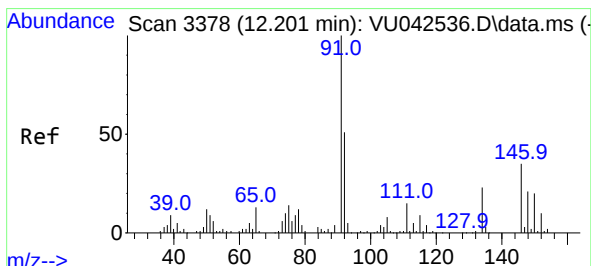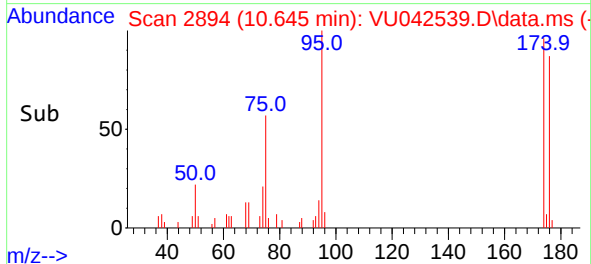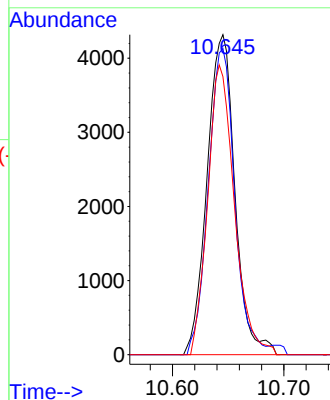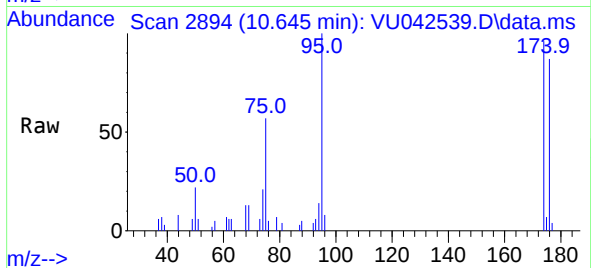

#68
1,2-Dichlorobenzene-d4
Concen: 0.81 ug/l
RT: 12.201 min Scan# 3378
Delta R.T. -0.000 min
Lab File: VU042539.D
Acq: 09 Mar 2021 14:34

Tgt Ion: 152 Resp: 7624
Ion Ratio Lower Upper
152 100
115 63.6 0.0 266.0
150 156.1 0.0 657.2

