

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030921\
 Data File : VU042540.D
 Acq On : 09 Mar 2021 15:03
 Operator : SY/MD
 Sample : VU0309WBL02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK24

Quant Time: Mar 11 13:00:00 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U030921DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Mar 11 12:50:28 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Fluorobenzene	6.121	96	20017	1.00	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.642	95	7005	0.79	ug/l	0.00
Spiked Amount 1.000			Recovery	=	79.00%	
68) 1,2-Dichlorobenzene-d4	12.205	152	7764	0.85	ug/l	0.00
Spiked Amount 1.000			Recovery	=	85.00%	
Target Compounds						
15) Methylene Chloride	3.051	84	2007	0.34	ug/l	Qvalue 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030921\
Data File : VU042540.D
Acq On : 09 Mar 2021 15:03
Operator : SY/MD
Sample : VU0309WBL02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK24

Quant Time: Mar 11 13:00:00 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U030921DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu Mar 11 12:50:28 2021
Response via : Initial Calibration




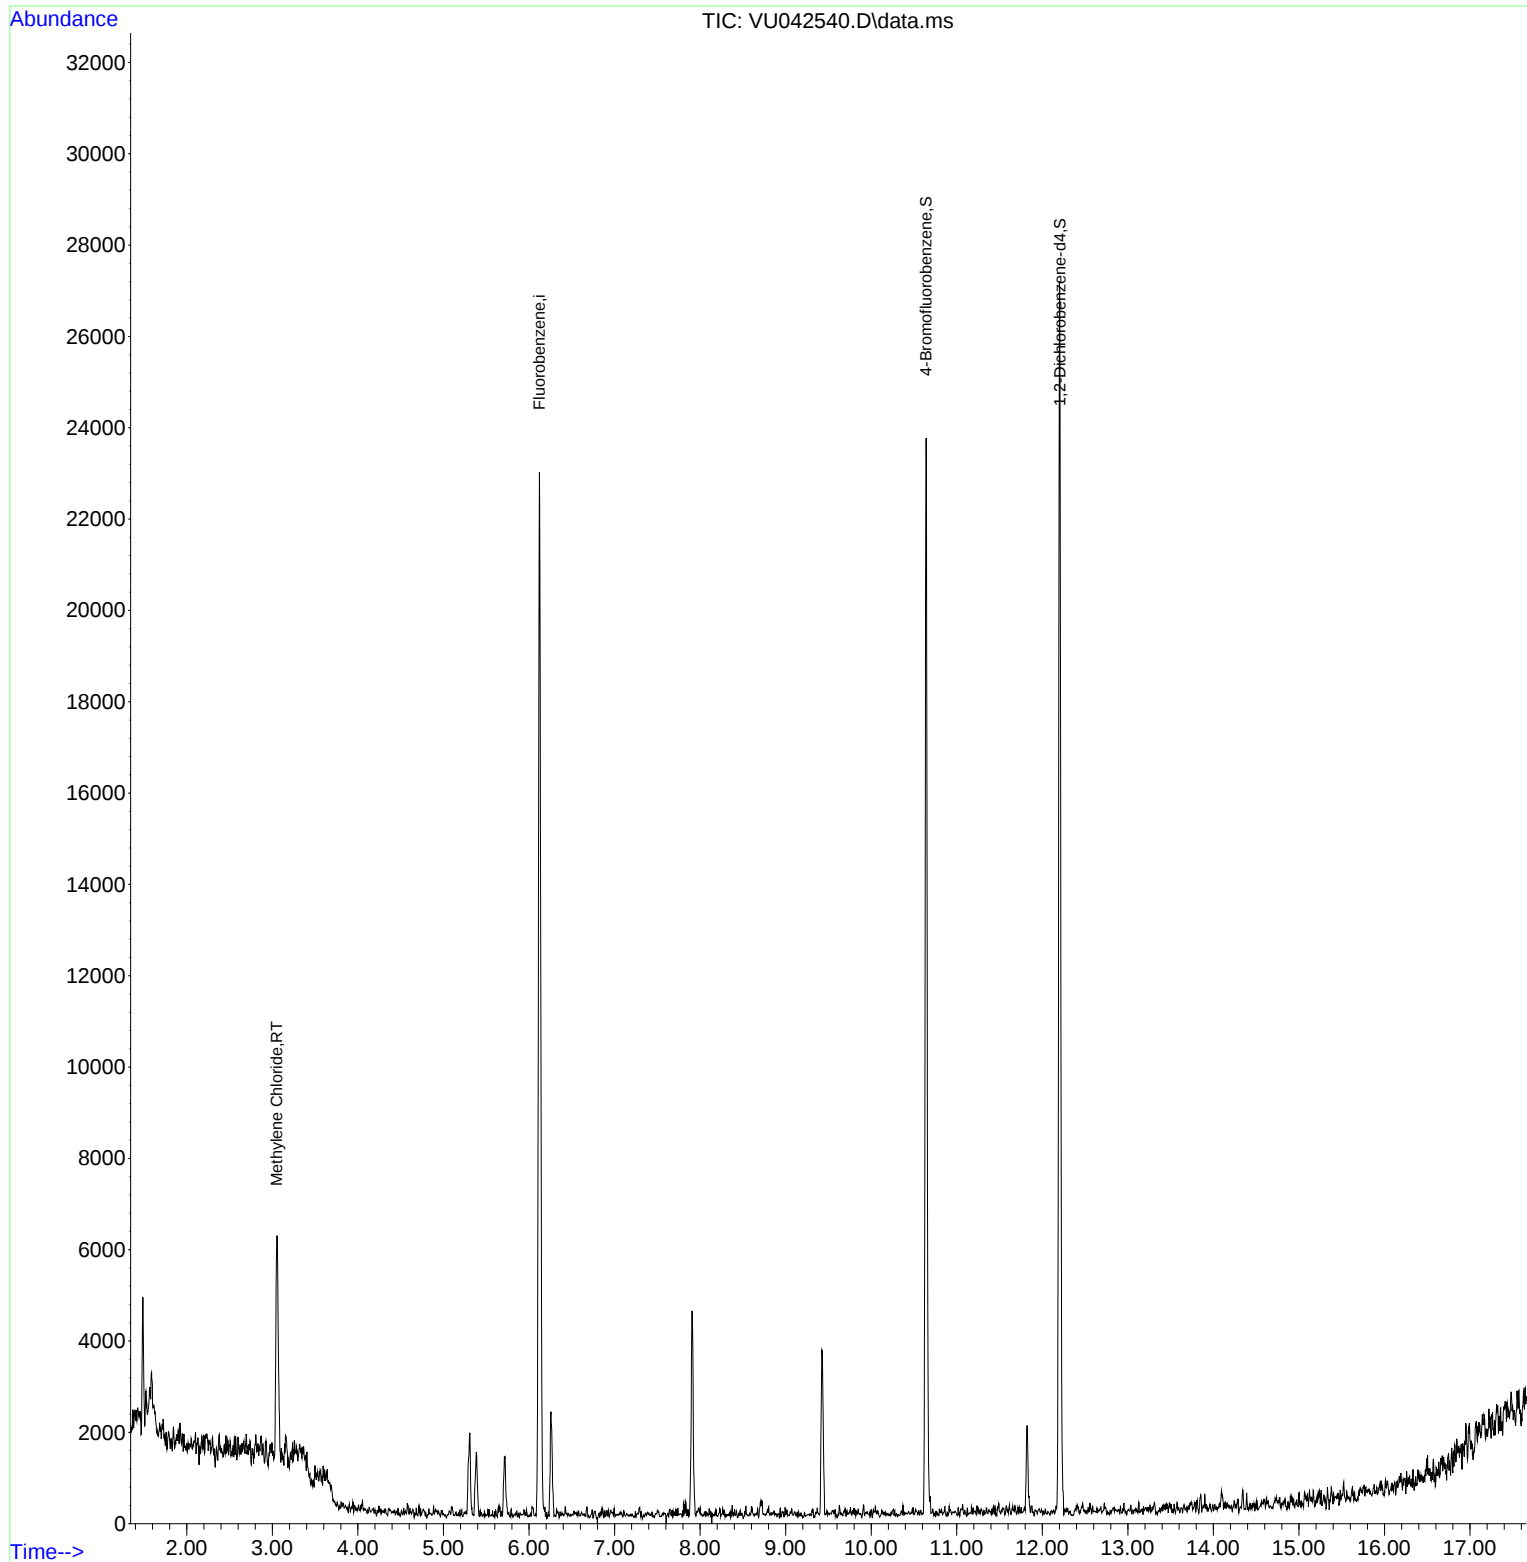


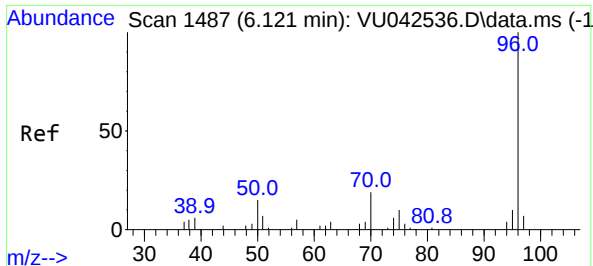

#1
Fluorobenzene
Concen: 1.00 ug/l
RT: 6.121 min Scan# 1487
Delta R.T. 0.000 min
Lab File: VU042540.D
Acq: 09 Mar 2021 15:03




Instrument :
MSVOA_U
ClientSampled :
VBLK24


Tgt Ion:	96	Resp:	20017
Ion	Ratio	Lower	Upper
96	100		
70	19.5	16.3	24.5
95	9.3	7.0	10.4
97	5.6	0.0	0.0

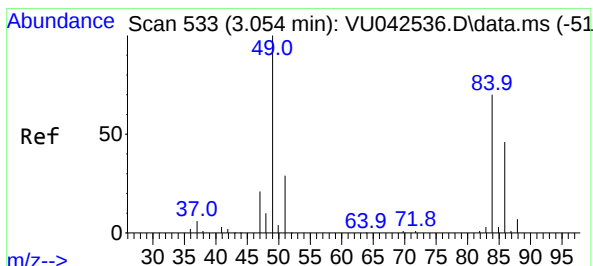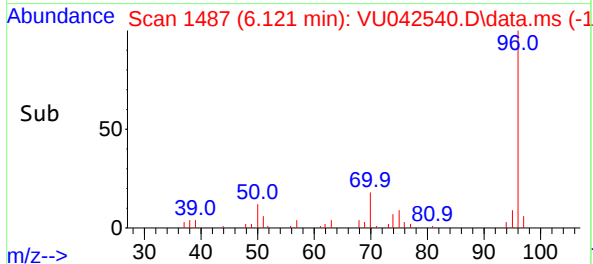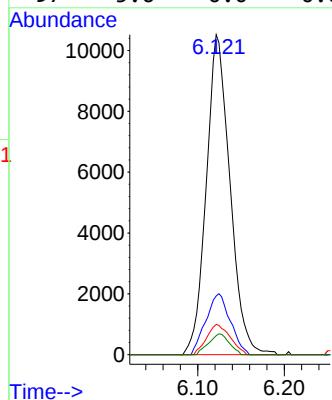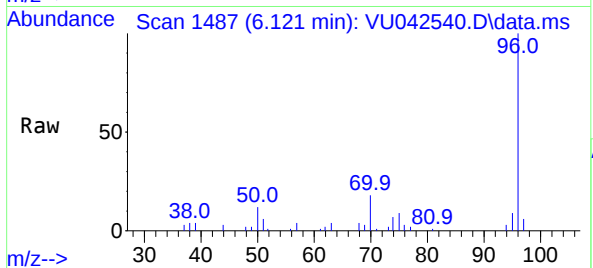

#15
Methylene Chloride
Concen: 0.34 ug/l
RT: 3.051 min Scan# 532
Delta R.T. -0.003 min
Lab File: VU042540.D
Acq: 09 Mar 2021 15:03

Tgt Ion:	84	Resp:	2007
Ion	Ratio	Lower	Upper
84	100		
49	132.5	114.6	172.0
51	46.3	0.0	83.0
86	58.3	52.3	78.5

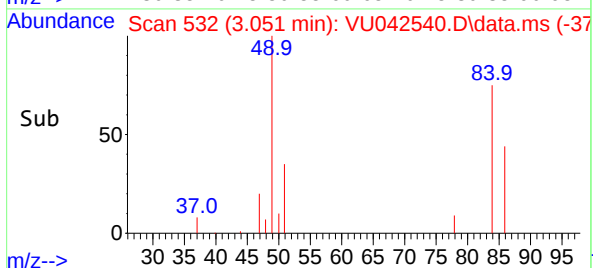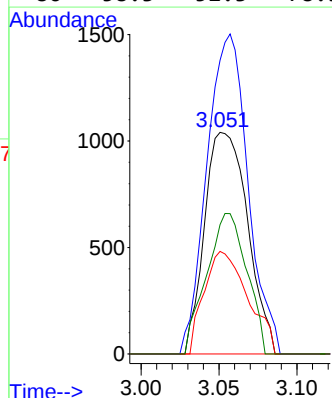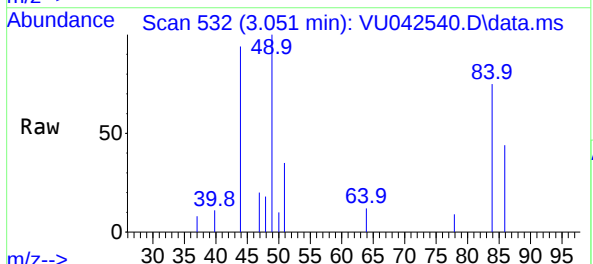




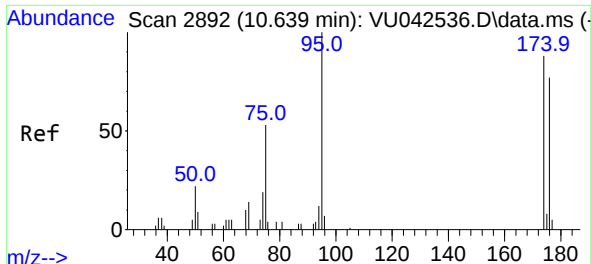


#57
4-Bromofluorobenzene
Concen: 0.79 ug/l
RT: 10.642 min Scan# 2893
Delta R.T. 0.003 min
Lab File: VU042540.D
Acq: 09 Mar 2021 15:03

Instrument :
MSVOA_U
ClientSampleId :
VBLK24

Tgt Ion: 95 Resp: 7005

Ion	Ratio	Lower	Upper
95	100		
174	101.6	73.1	109.7
176	94.5	63.4	95.2

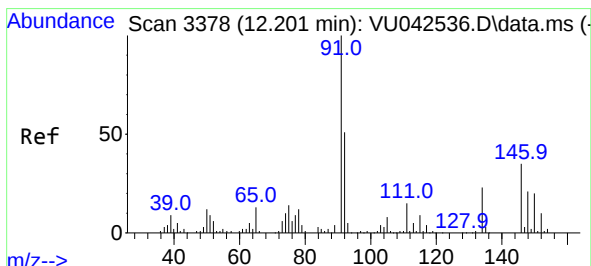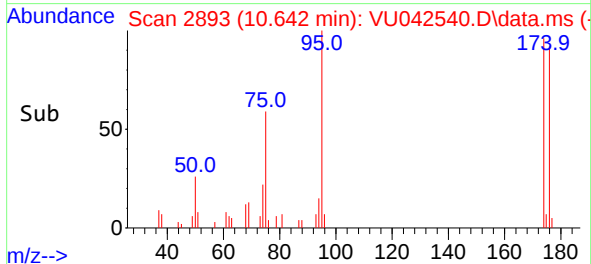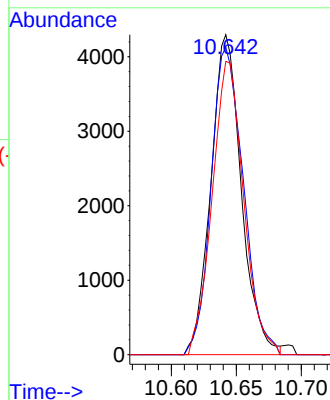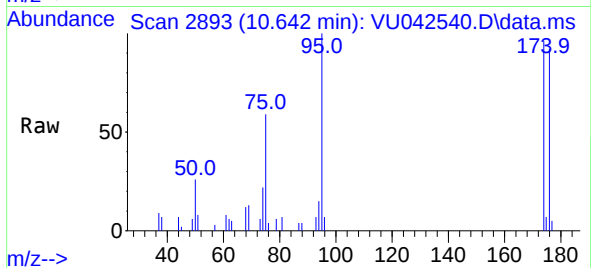

#68
1,2-Dichlorobenzene-d4
Concen: 0.85 ug/l
RT: 12.205 min Scan# 3379
Delta R.T. 0.003 min
Lab File: VU042540.D
Acq: 09 Mar 2021 15:03

Tgt Ion: 152 Resp: 7764

Ion	Ratio	Lower	Upper
152	100		
115	60.6	0.0	266.0
150	151.6	0.0	657.2

