


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030921\
 Data File : VU042531.D
 Acq On : 09 Mar 2021 08:58
 Operator : SY/MD
 Sample : BFB
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U030921DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER
 Last Update : Thu Mar 11 12:50:28 2021

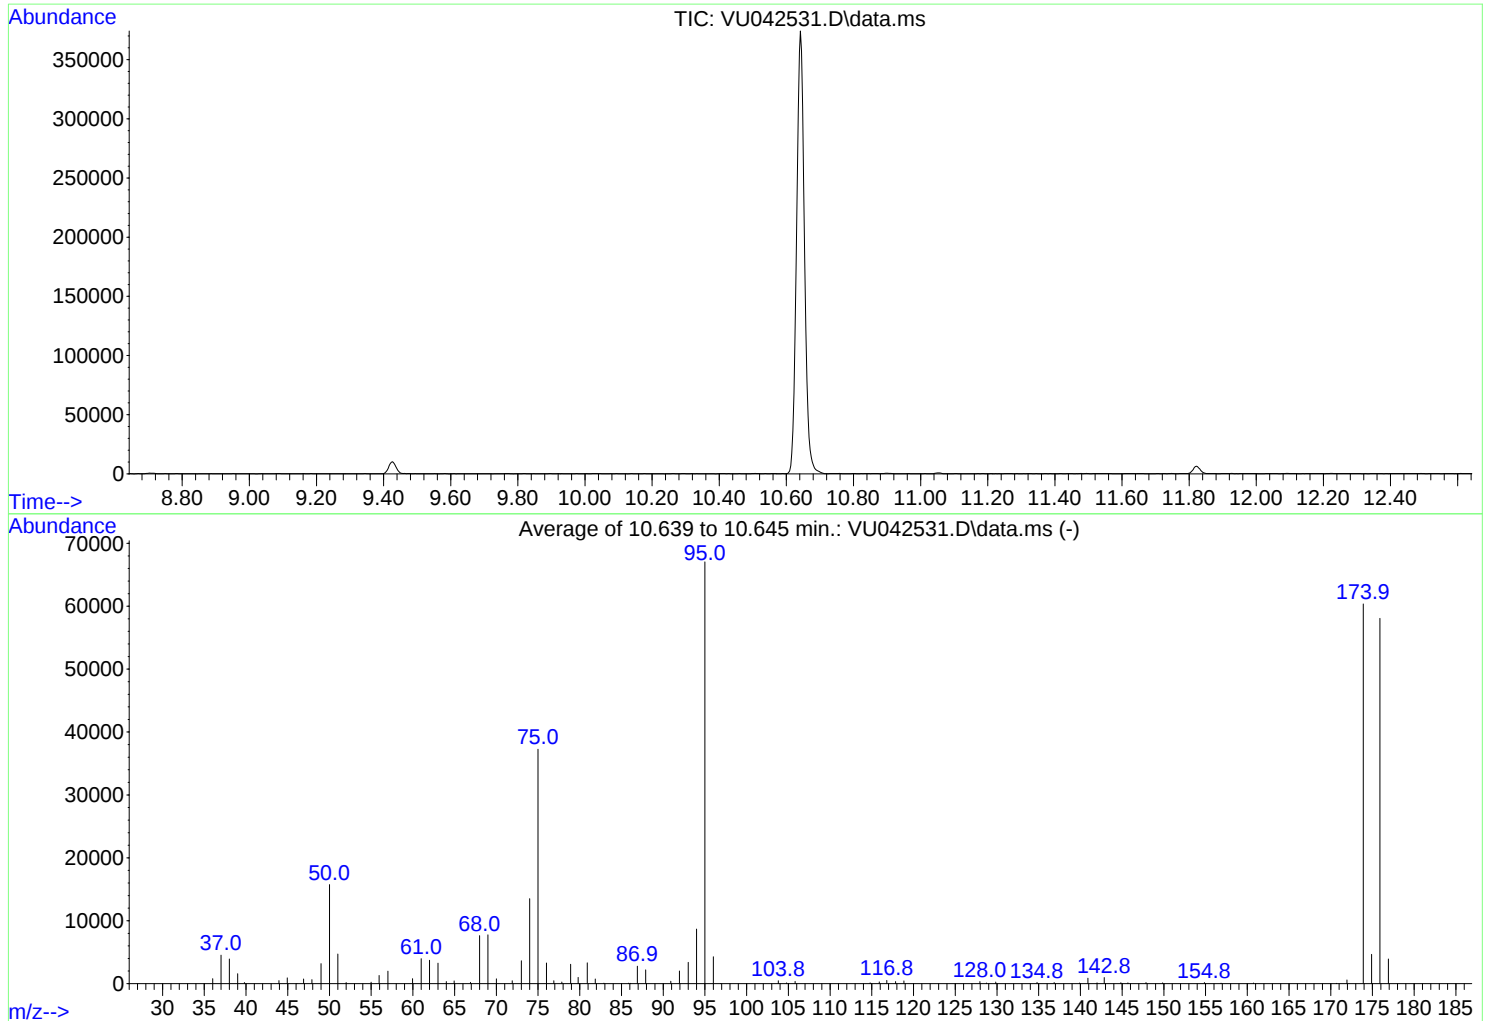

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.5	15753	PASS
75	95	30	60	55.6	37267	PASS
95	95	100	100	100.0	67056	PASS
96	95	5	9	6.4	4272	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	90.0	60357	PASS
175	174	5	9	7.7	4659	PASS
176	174	95	101	96.2	58085	PASS
177	176	5	9	6.7	3916	PASS