

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031019\
Data File : VU029876.D
Acq On : 08 Mar 2019 09:39
Operator : JC/SP
Sample : VU0310WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0310WBL01

Quant Time: Mar 08 22:48:58 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA U\METHOD\524U030719DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Fri Mar 08 00:30:10 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----	-----	-----	-----	-----	-----	-----
1) Fluorobenzene	5.74	96	62527	1.00	ug/l	0.00

System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.31	95	19048	0.85	ug/l	0.00
Spiked Amount 1.000			Recovery	=	85.00%	
68) 1,2-Dichlorobenzene-d4	11.86	152	21409	0.82	ug/l	0.00
Spiked Amount 1.000			Recovery	=	82.00%	


Target Compounds	Ovalue
-----	-----


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU031019\
Data File : VU029876.D
Acq On : 08 Mar 2019 09:39
Operator : JC/SP
Sample : VU0310WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0310WBL01

Quant Time: Mar 08 22:48:58 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA U\METHOD\524U030719DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Fri Mar 08 00:30:10 2019
Response via : Initial Calibration

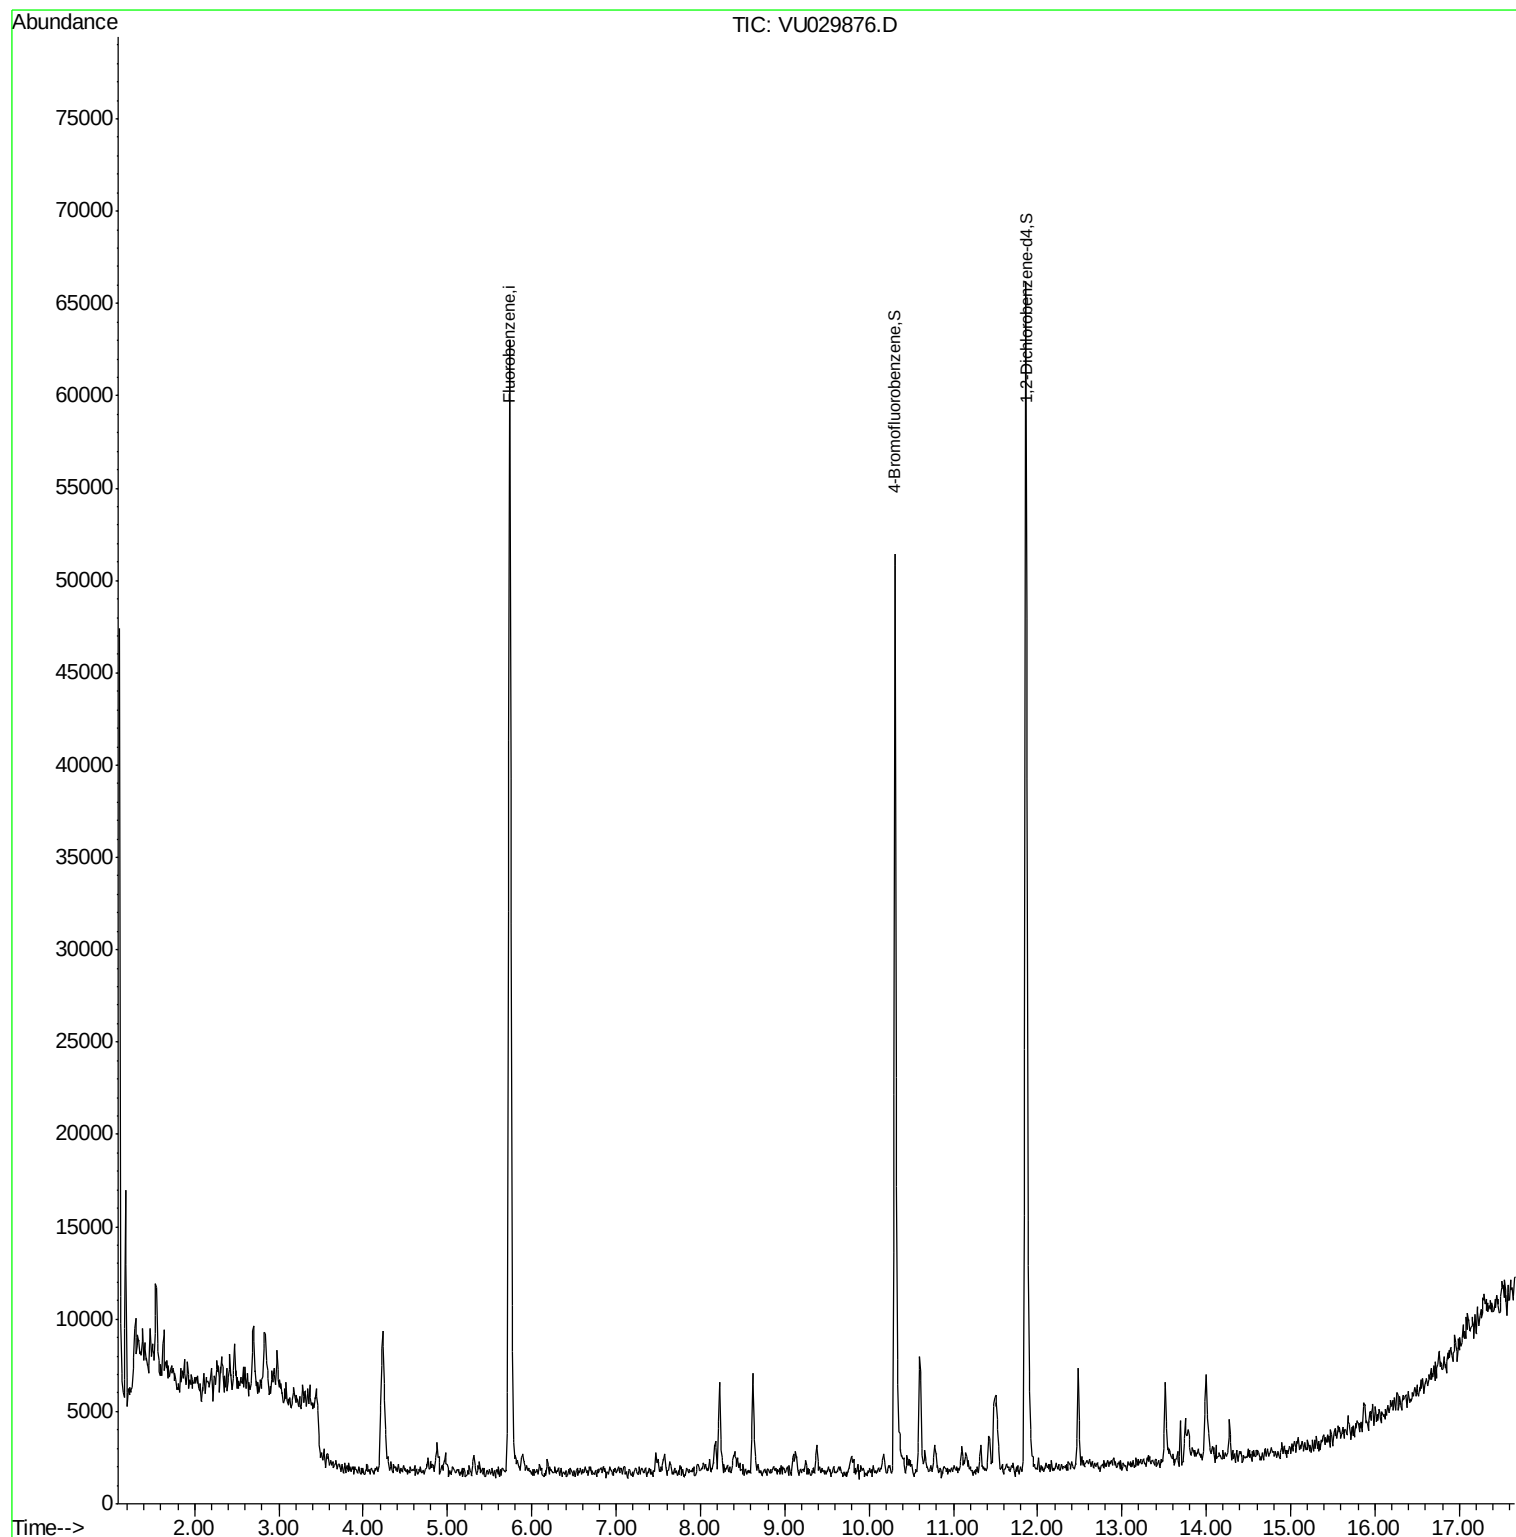

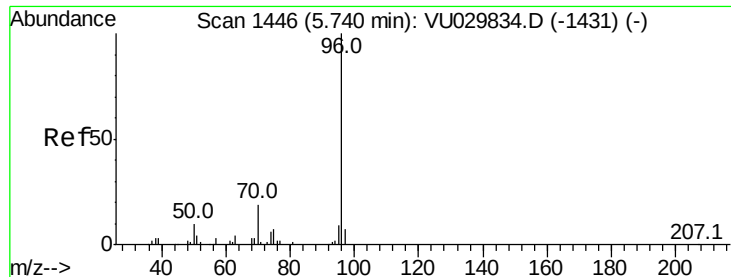

#1

Fluorobenzene

Concen: 1.000 ug/l

RT: 5.74 min Scan# 1446

Delta R.T. -0.00 min

Lab File: VU029876.D

Acq: 08 Mar 2019 09:39

Instrument :

MSVOA_U

ClientSampleId :

VU0310WBL01

Tot Ion: 96 Resp: 62527


Ion Ratio Lower Upper

96 100

70 19.3 14.4 21.6

95 8.9 7.0 10.6

97 6.5 0.0 0.0#



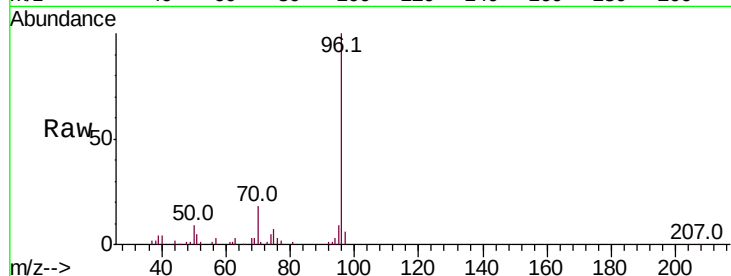


Abundance Ion 96.00 (95.70 to 96.70): VU0

Ion 70.00 (69.70 to 70.70): VU0

Ion 95.00 (94.70 to 95.70): VU0

Ion 97.00 (96.70 to 97.70): VU0

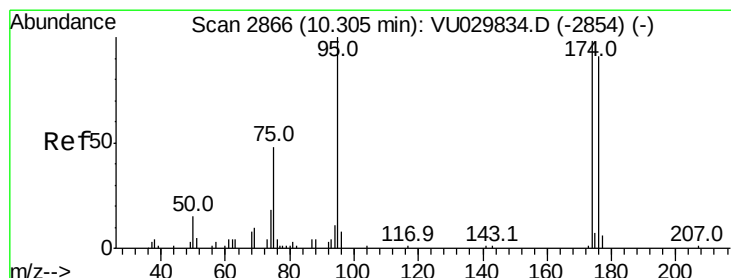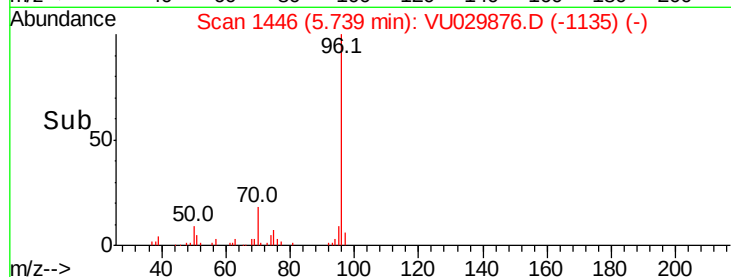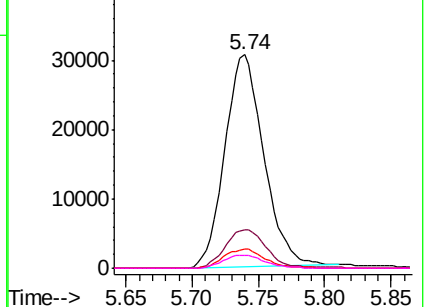

#57

4-Bromofluorobenzene

Concen: N.D. ug/l

RT: 10.31 min Scan# 2868

Delta R.T. 0.01 min

Lab File: VU029876.D

Acq: 08 Mar 2019 09:39


Tgt Ion: 95 Resp: 19048

Ion Ratio Lower Upper

95 100

174 93.9 76.5 114.7



176 89.6 74.2 111.2

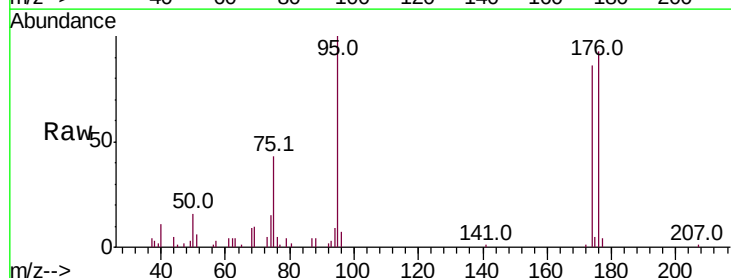


Abundance Ion 95.00 (94.70 to 95.70): VU0

Ion 174.00 (173.70 to 174.70): V

Ion 176.00 (175.70 to 176.70): V

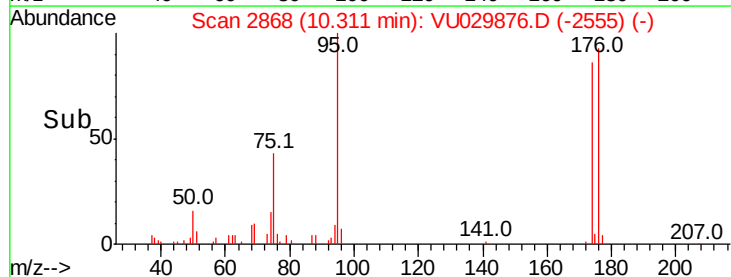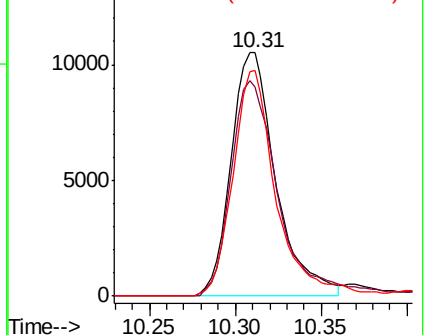

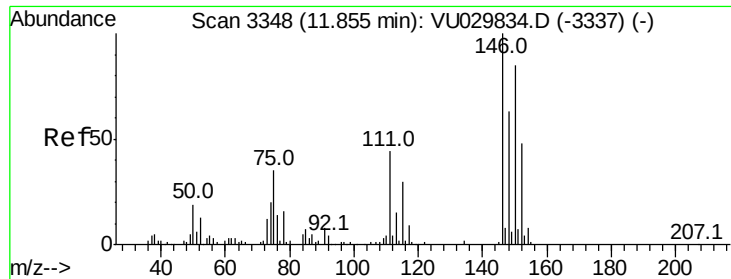

#68

1,2-Dichlorobenzene-d4

Concen: N.D. ug/l

RT: 11.86 min Scan# 3350

Delta R.T. 0.01 min

Lab File: VU029876.D

Acq: 08 Mar 2019 09:39

Instrument :

MSVOA_U

ClientSampleId :

VU0310WBL01


Tot Ion:152 Resp: 21409

Ion Ratio Lower Upper

152 100

115 59.3 0.0 124.0

150 163.3 0.0 631.2

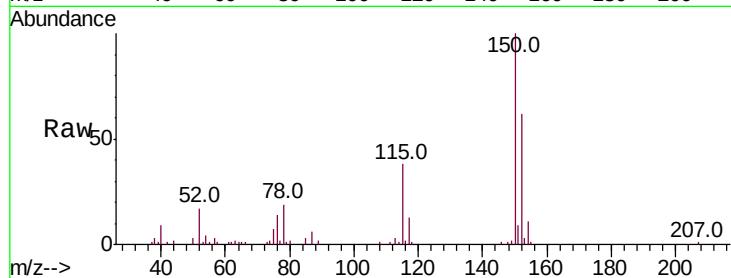

Abundance Ion 152.00 (151.70 to 152.70): V

Ion 115.00 (114.70 to 115.70): V

Ion 150.00 (149.70 to 150.70): V

