


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031019\
Data File : VU029874.D
Acq On : 08 Mar 2019 08:36
Operator : JC/SP
Sample : BFB
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U030719DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Fri Mar 08 00:30:10 2019

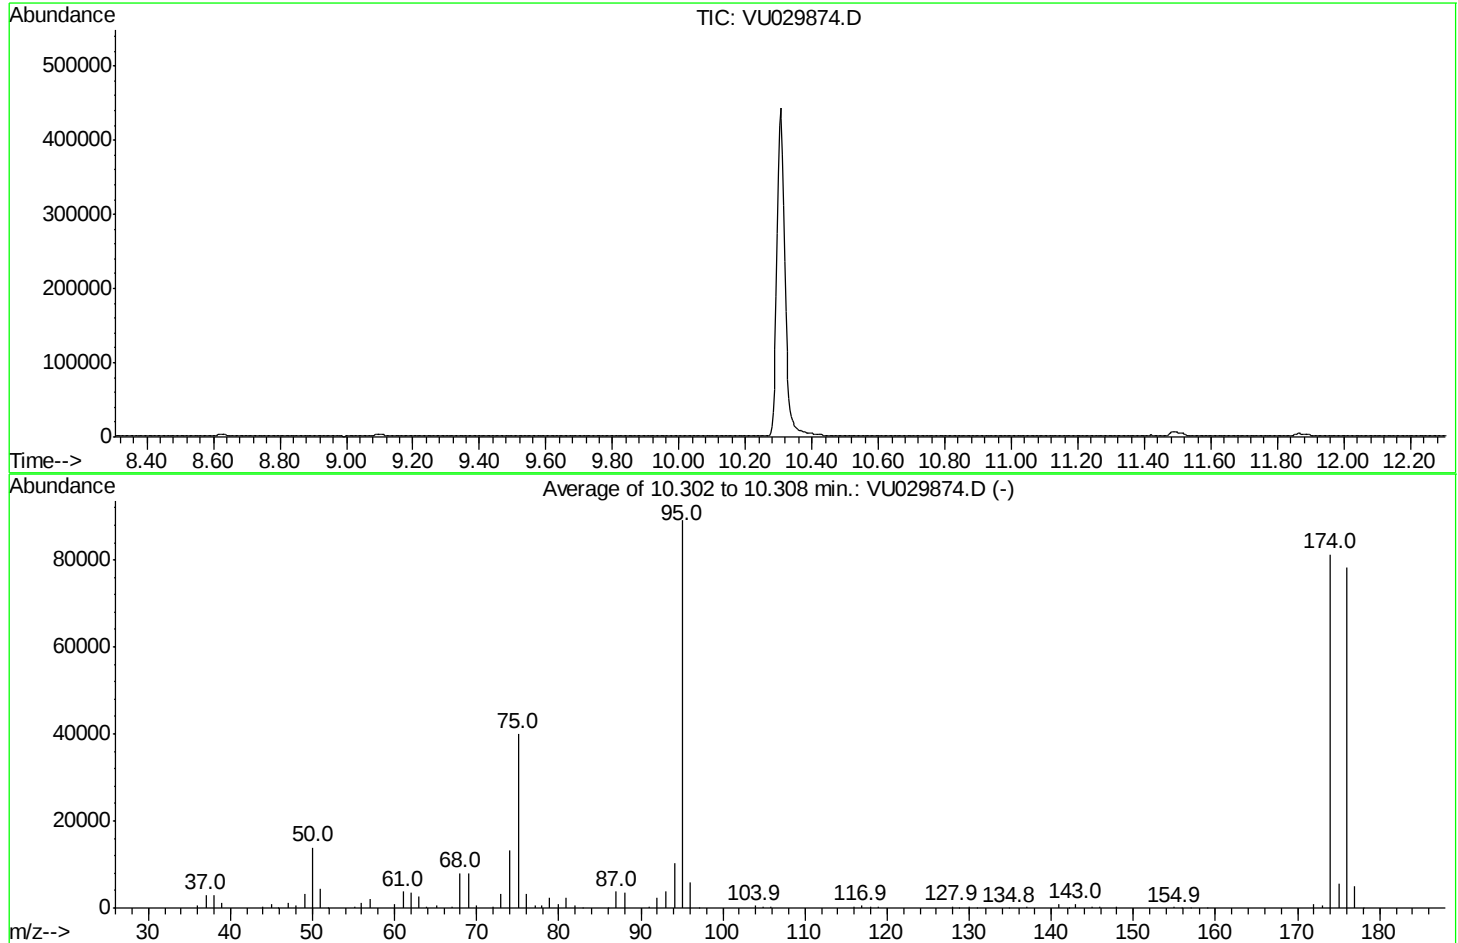

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2852

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	13890	PASS
75	95	30	60	44.9	40029	PASS
95	95	100	100	100.0	89101	PASS
96	95	5	9	6.7	5980	PASS
173	174	0.00	2	0.7	606	PASS
174	95	50	100	91.3	81341	PASS
175	174	5	9	7.0	5699	PASS
176	174	95	101	96.3	78341	PASS
177	176	5	9	6.3	4969	PASS