


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU031020\
 Data File : VU037142.D
 Acq On : 10 Mar 2020 09:06
 Operator : JC/MD
 Sample : BFB
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U030920DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER
 Last Update : Mon Mar 09 15:46:40 2020

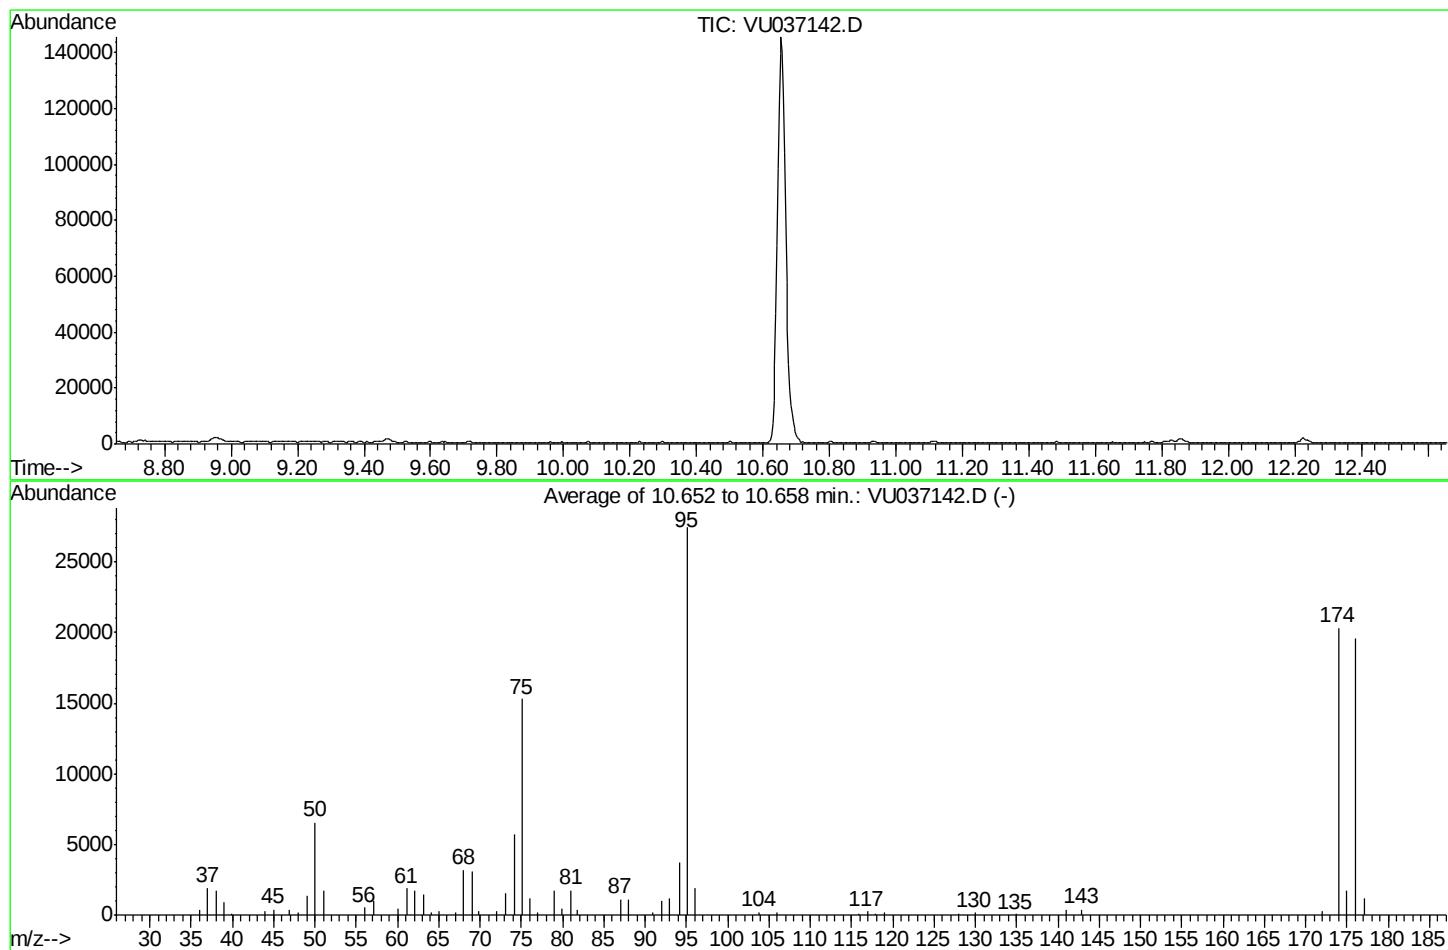

AutoFind: Scans 2896, 2897, 2898; Background Corrected with Scan 2883

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.9	6564	PASS
75	95	30	60	55.7	15279	PASS
95	95	100	100	100.0	27445	PASS
96	95	5	9	6.9	1885	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	74.0	20301	PASS
175	174	5	9	8.7	1768	PASS
176	174	95	101	96.5	19594	PASS
177	176	5	9	6.1	1187	PASS