

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031021\
 Data File : VU042548.D
 Acq On : 10 Mar 2021 10:31
 Operator : SY/MD
 Sample : VU0310WBL03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK25

Quant Time: Mar 11 13:43:35 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U030921DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Mar 11 12:50:28 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Fluorobenzene	6.125	96	18396	1.00	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.642	95	7637	0.94	ug/l	0.00
Spiked Amount 1.000			Recovery	=	94.00%	
68) 1,2-Dichlorobenzene-d4	12.205	152	7999	0.95	ug/l	0.00
Spiked Amount 1.000			Recovery	=	95.00%	
Target Compounds						
15) Methylene Chloride	3.057	84	896	0.16	ug/l	# 74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031021\
Data File : VU042548.D
Acq On : 10 Mar 2021 10:31
Operator : SY/MD
Sample : VU0310WBL03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK25

Quant Time: Mar 11 13:43:35 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U030921DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu Mar 11 12:50:28 2021
Response via : Initial Calibration

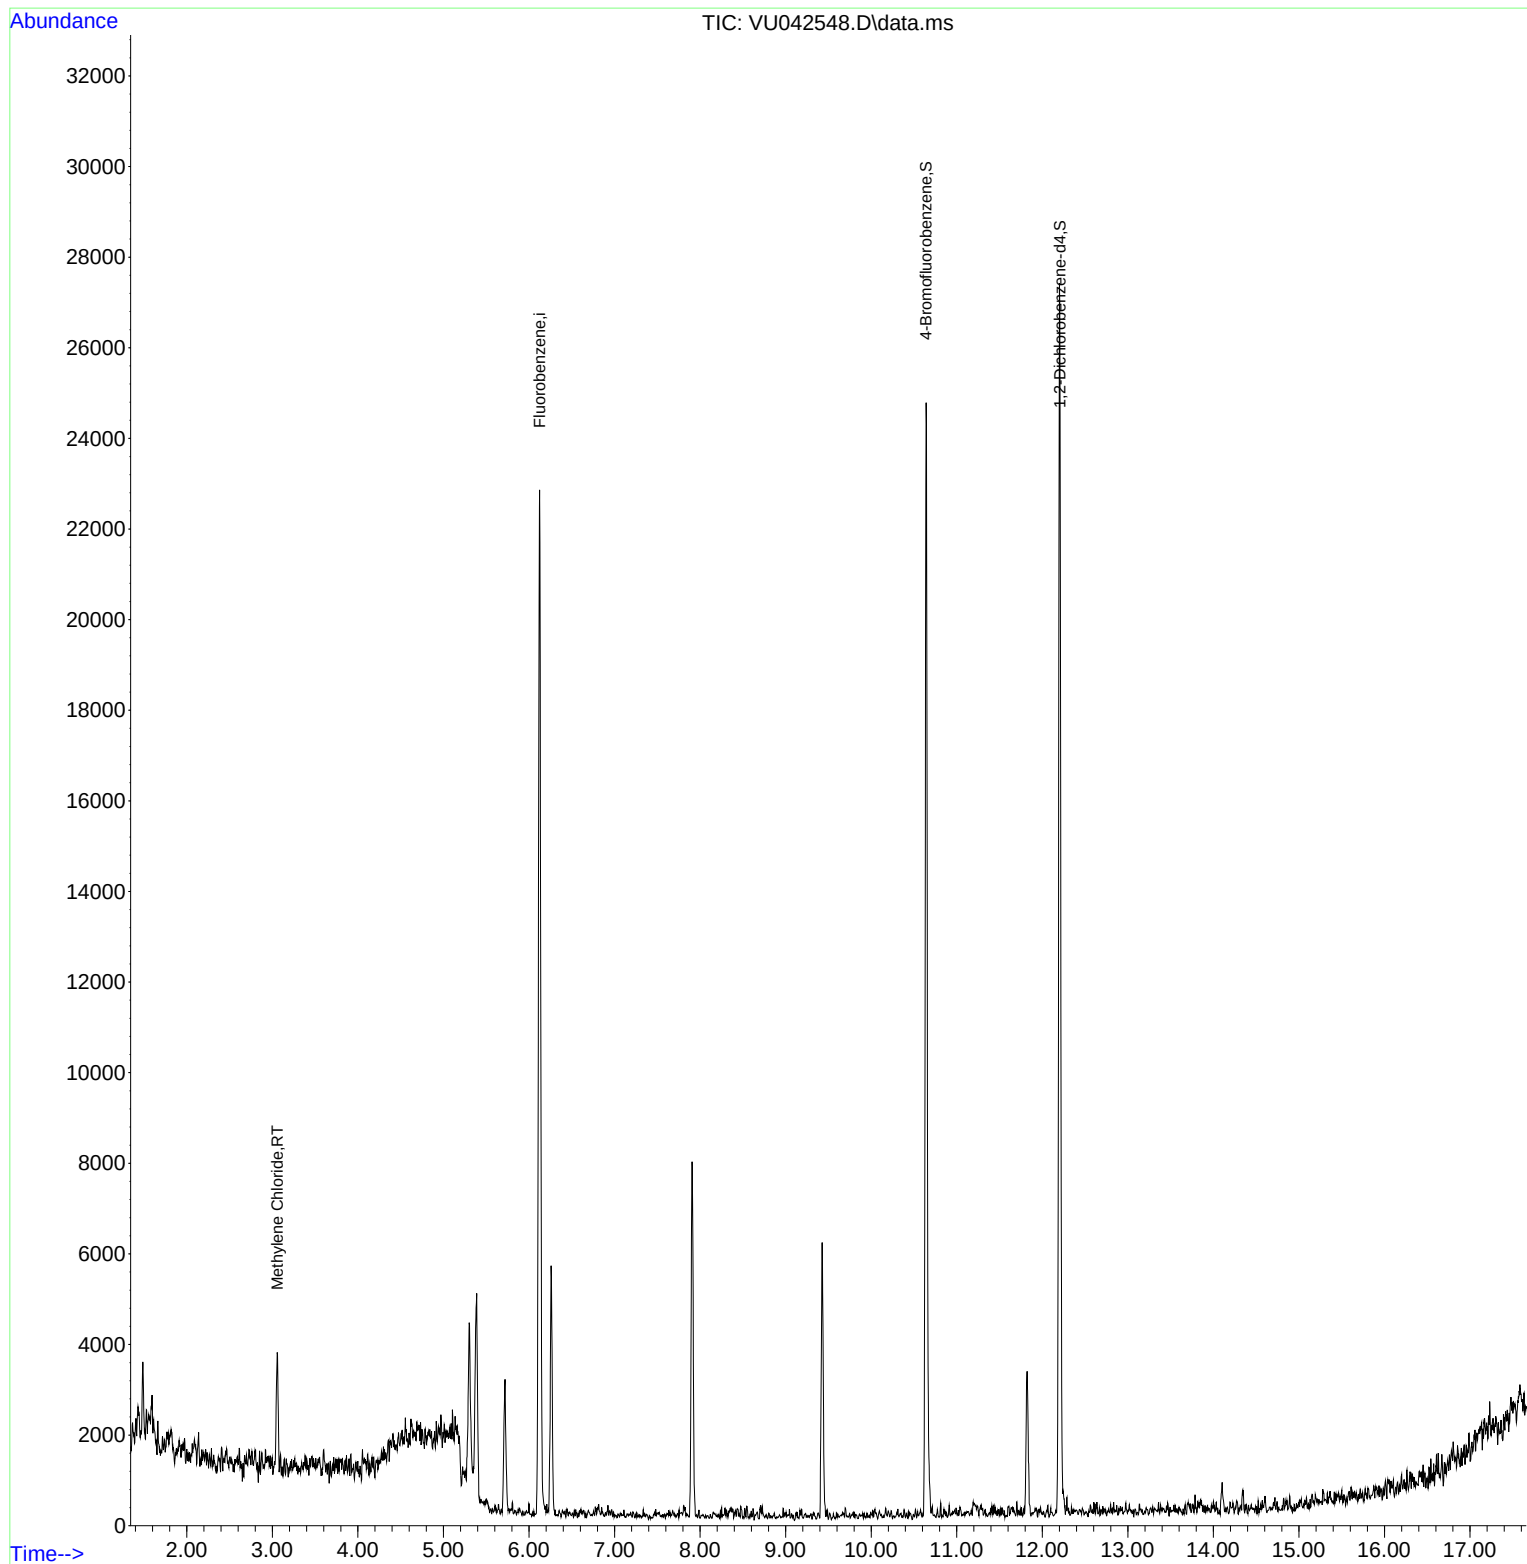




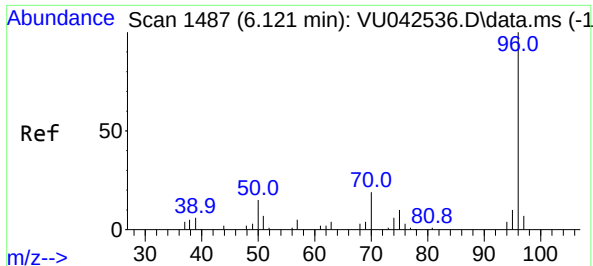


#1
Fluorobenzene
Concen: 1.00 ug/l
RT: 6.125 min Scan# 1488
Delta R.T. 0.004 min
Lab File: VU042548.D
Acq: 10 Mar 2021 10:31

Instrument :
MSVOA_U
ClientSampleId :
VBLK25

Tgt Ion: 96 Resp: 18396




Ion	Ratio	Lower	Upper
96	100		
70	20.6	16.3	24.5
95	10.4	7.0	10.4
97	6.4	0.0	0.0

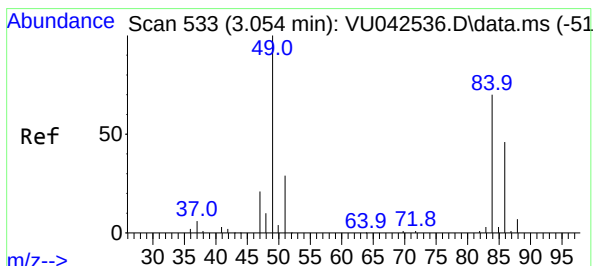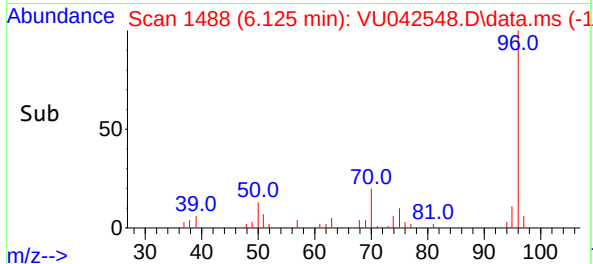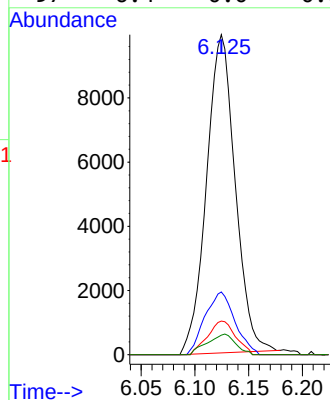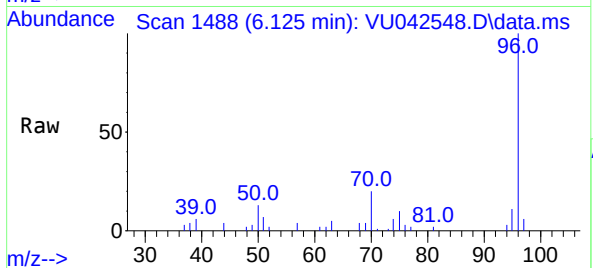


#15
Methylene Chloride
Concen: 0.16 ug/l
RT: 3.057 min Scan# 534
Delta R.T. 0.003 min
Lab File: VU042548.D
Acq: 10 Mar 2021 10:31

Tgt Ion: 84 Resp: 896

Ion	Ratio	Lower	Upper
84	100		
49	102.5	114.6	172.0
51	57.5	0.0	83.0
86	57.3	52.3	78.5


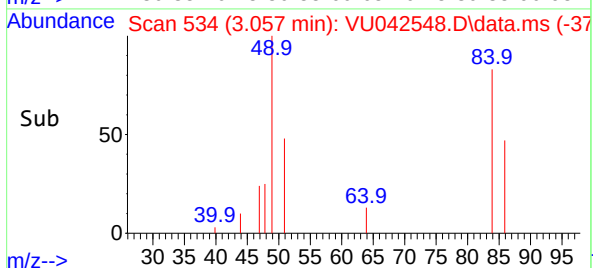
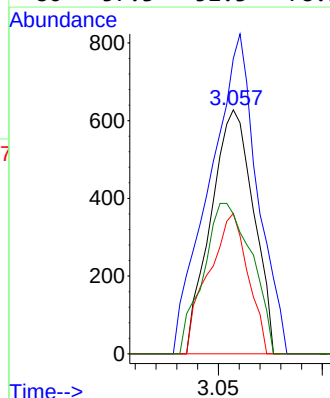
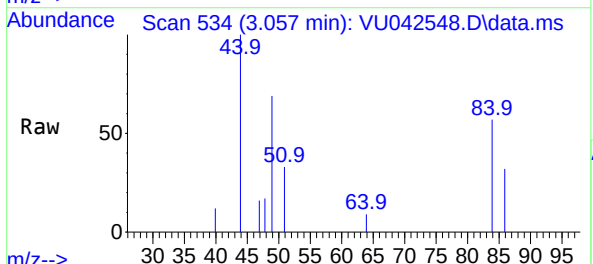


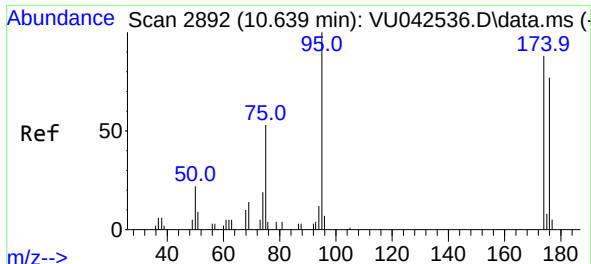

#57
4-Bromofluorobenzene
Concen: 0.94 ug/l
RT: 10.642 min Scan# 2893
Delta R.T. 0.003 min
Lab File: VU042548.D
Acq: 10 Mar 2021 10:31

Instrument :
MSVOA_U
ClientSampled :
VBLK25

Tgt Ion: 95 Resp: 7637
Ion Ratio Lower Upper
95 100
174 98.3 73.1 109.7
176 91.7 63.4 95.2

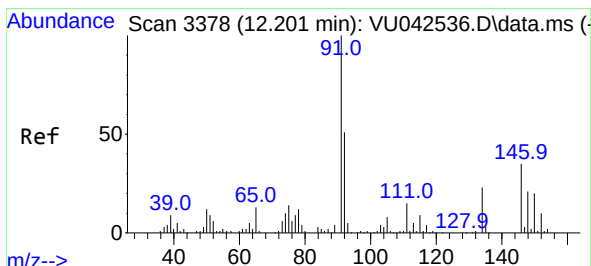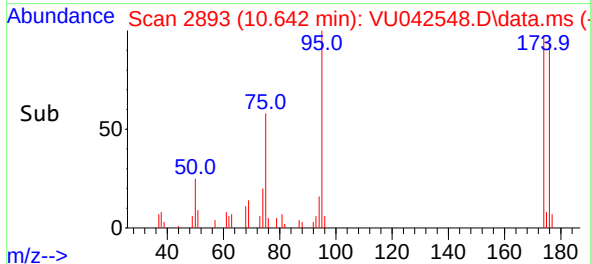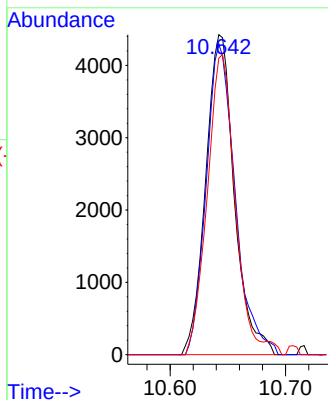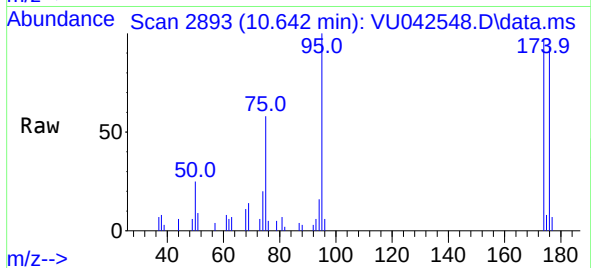

#68
1,2-Dichlorobenzene-d4
Concen: 0.95 ug/l
RT: 12.205 min Scan# 3379
Delta R.T. 0.003 min
Lab File: VU042548.D
Acq: 10 Mar 2021 10:31

Tgt Ion: 152 Resp: 7999
Ion Ratio Lower Upper
152 100
115 57.1 0.0 266.0
150 147.3 0.0 657.2

