

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031021\
 Data File : VU042549.D
 Acq On : 10 Mar 2021 11:17
 Operator : SY/MD
 Sample : VU0310WBL04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK26

Quant Time: Mar 11 13:47:58 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U030921DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Mar 11 12:50:28 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Fluorobenzene	6.124	96	18998	1.00	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.642	95	7955	0.95	ug/l	0.00
Spiked Amount 1.000			Recovery	=	95.00%	
68) 1,2-Dichlorobenzene-d4	12.205	152	7186	0.83	ug/l	0.00
Spiked Amount 1.000			Recovery	=	83.00%	
Target Compounds						
15) Methylene Chloride	3.060	84	1031	0.18	ug/l	# 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031021\
Data File : VU042549.D
Acq On : 10 Mar 2021 11:17
Operator : SY/MD
Sample : VU0310WBL04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK26

Quant Time: Mar 11 13:47:58 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U030921DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu Mar 11 12:50:28 2021
Response via : Initial Calibration




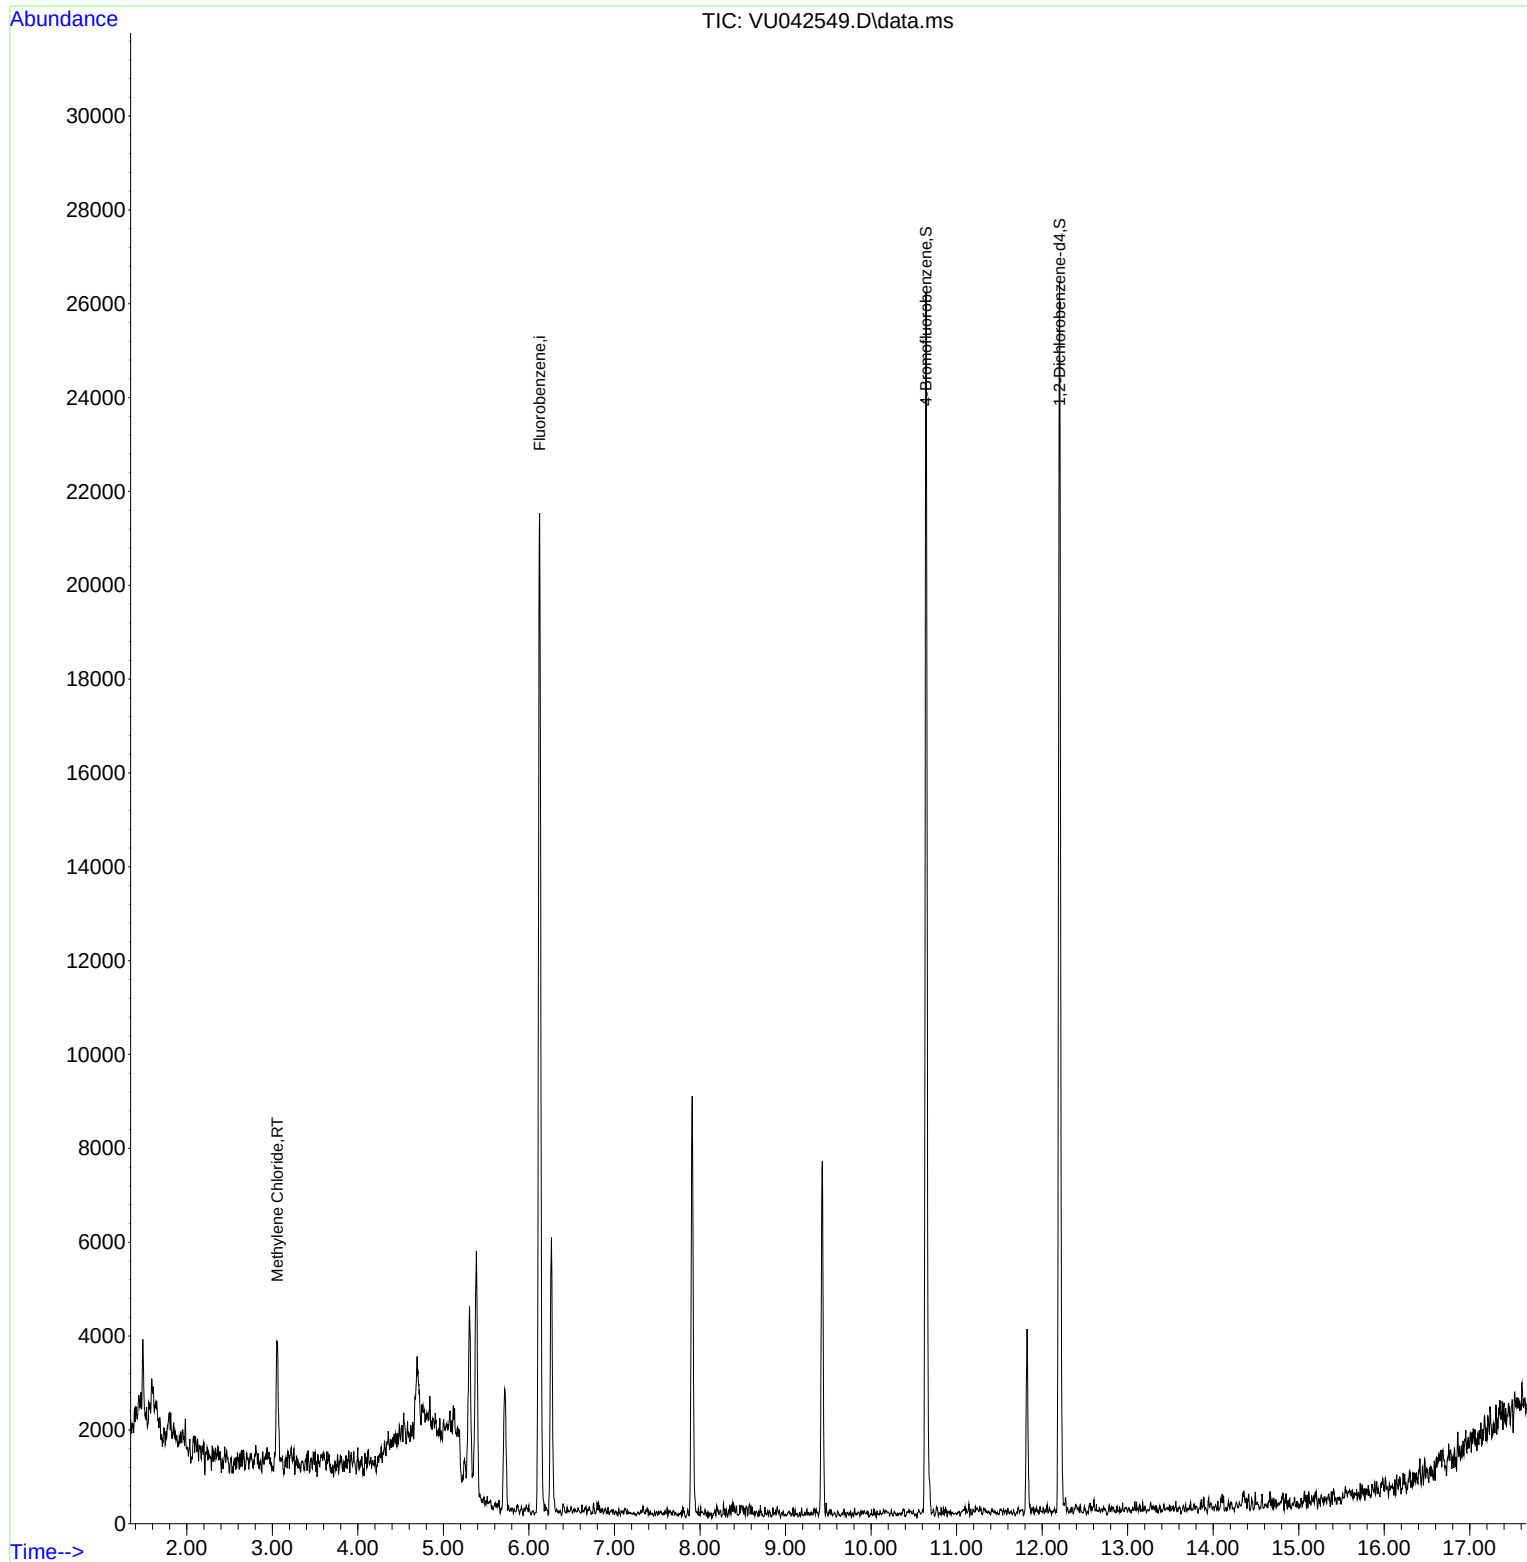


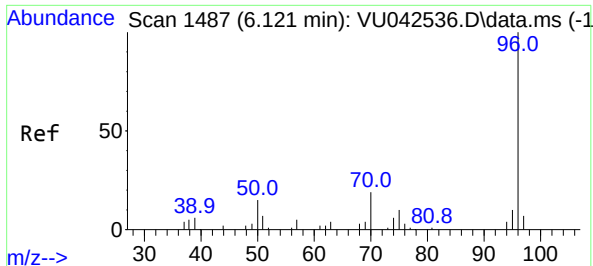

#1
Fluorobenzene
Concen: 1.00 ug/l
RT: 6.124 min Scan# 1488
Delta R.T. 0.003 min
Lab File: VU042549.D
Acq: 10 Mar 2021 11:17




Instrument :
MSVOA_U
ClientSampleId :
VBLK26


Tgt Ion:	96	Resp:	18998
Ion	Ratio	Lower	Upper
96	100		
70	21.0	16.3	24.5
95	9.9	7.0	10.4
97	6.0	0.0	0.0

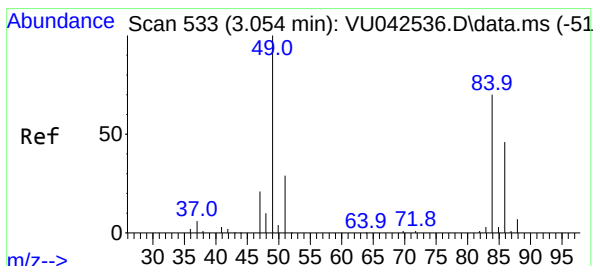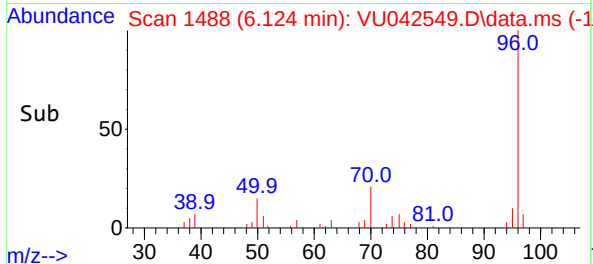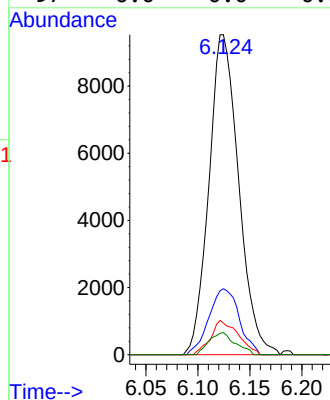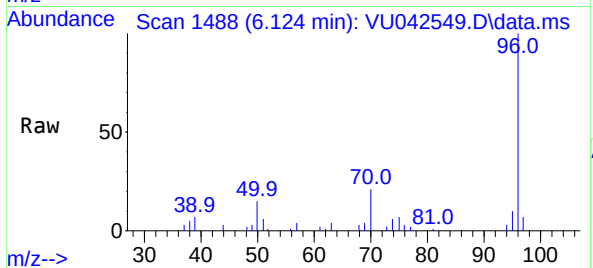

#15
Methylene Chloride
Concen: 0.18 ug/l
RT: 3.060 min Scan# 535
Delta R.T. 0.006 min
Lab File: VU042549.D
Acq: 10 Mar 2021 11:17

Tgt Ion:	84	Resp:	1031
Ion	Ratio	Lower	Upper
84	100		
49	132.6	114.6	172.0
51	39.9	0.0	83.0
86	80.9	52.3	78.5

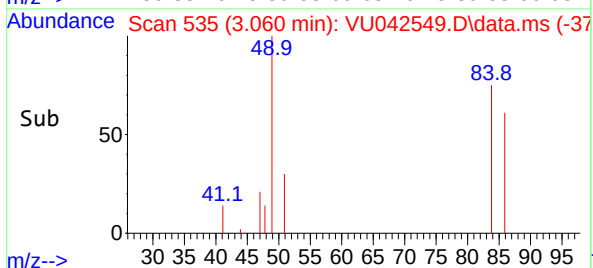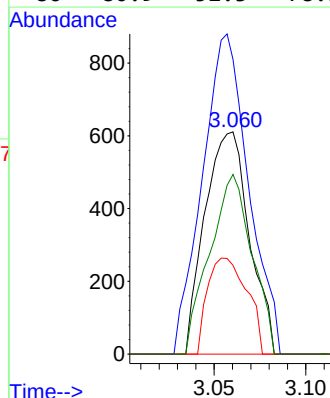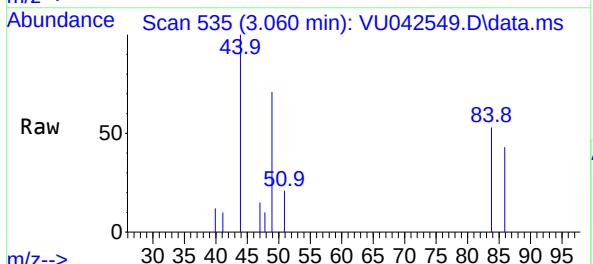




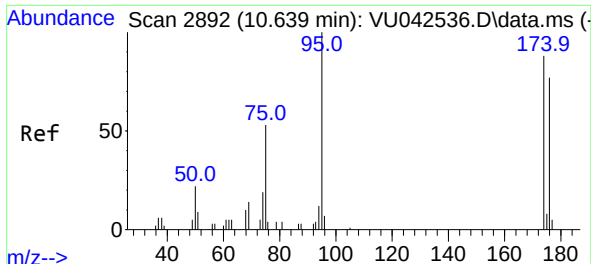


#57
4-Bromofluorobenzene
Concen: 0.95 ug/l
RT: 10.642 min Scan# 2893
Delta R.T. 0.003 min
Lab File: VU042549.D
Acq: 10 Mar 2021 11:17

Instrument :
MSVOA_U
ClientSampleId :
VBLK26

Tgt Ion: 95 Resp: 7955

Ion	Ratio	Lower	Upper
95	100		
174	94.8	73.1	109.7
176	90.9	63.4	95.2

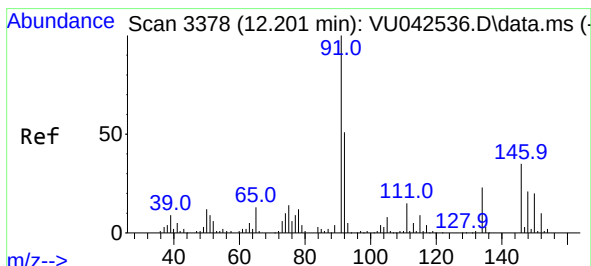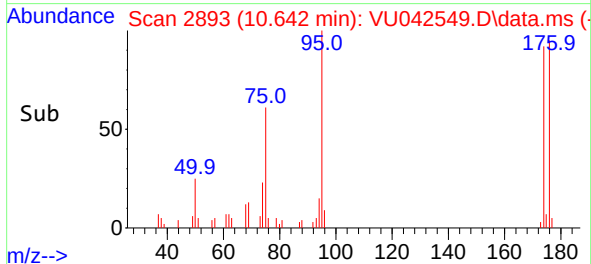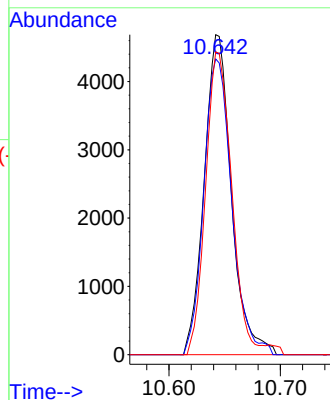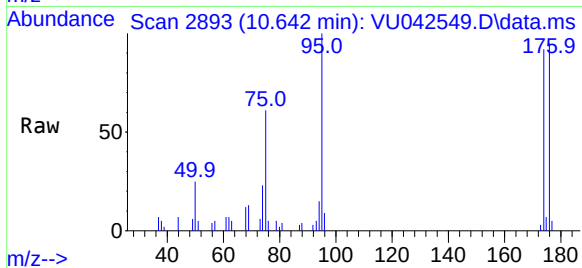

#68
1,2-Dichlorobenzene-d4
Concen: 0.83 ug/l
RT: 12.205 min Scan# 3379
Delta R.T. 0.003 min
Lab File: VU042549.D
Acq: 10 Mar 2021 11:17

Tgt Ion: 152 Resp: 7186

Ion	Ratio	Lower	Upper
152	100		
115	67.4	0.0	266.0
150	167.9	0.0	657.2

