


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031021\
Data File : VU042546.D
Acq On : 10 Mar 2021 08:37
Operator : SY/MD
Sample : BFB
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U030921DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Thu Mar 11 12:50:28 2021

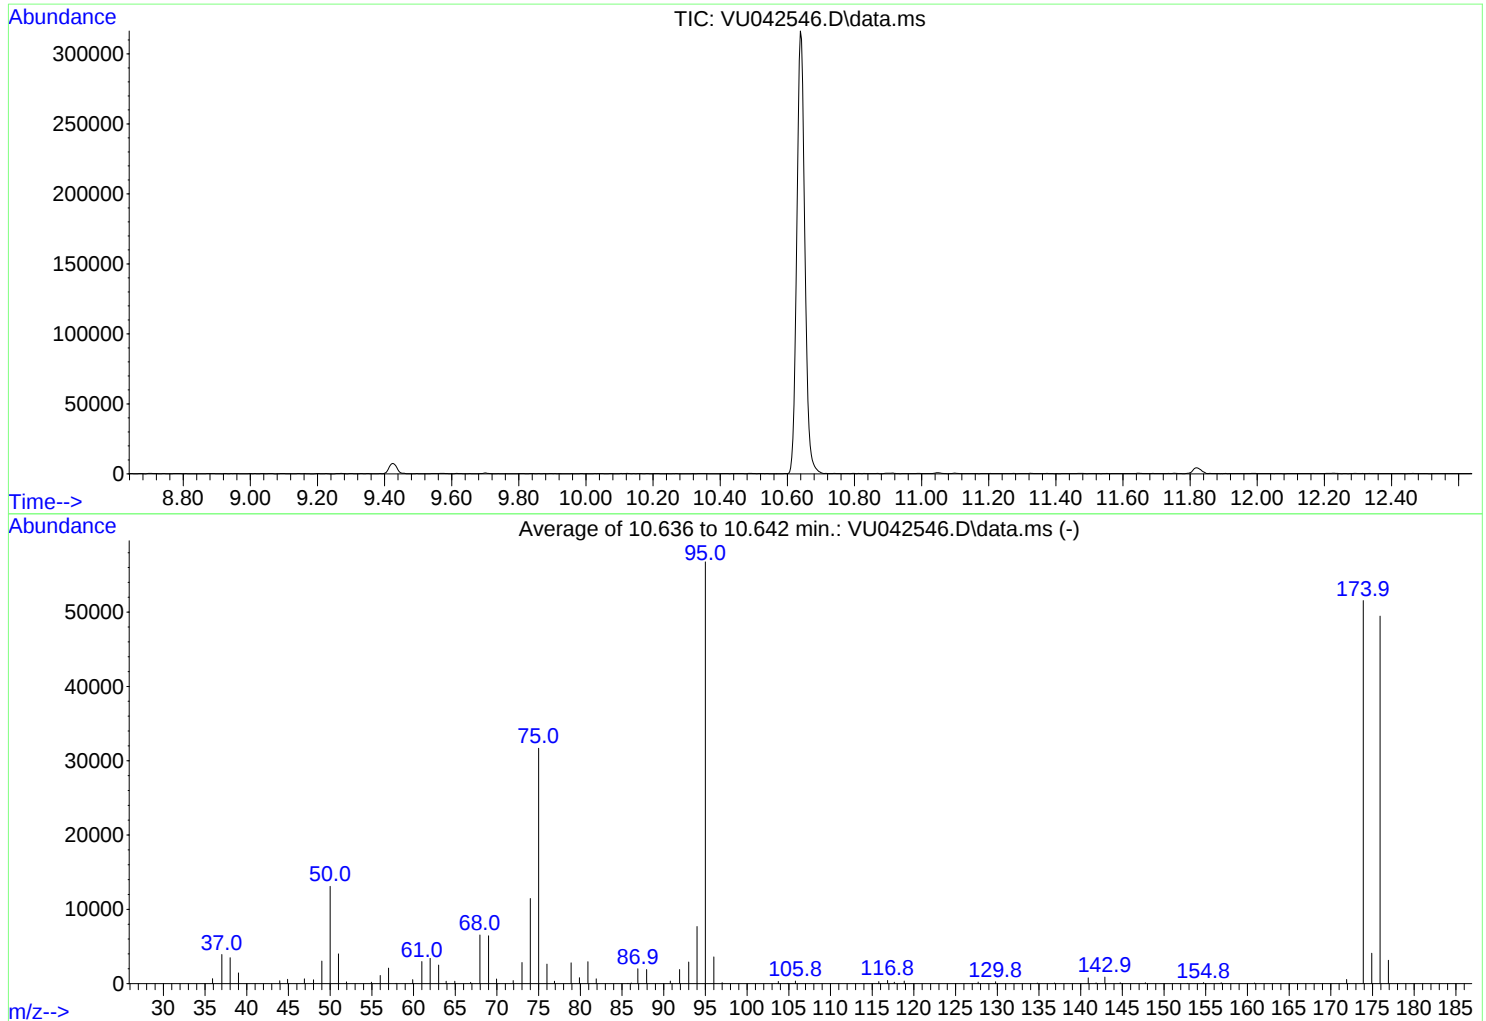

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.1	13105	PASS
75	95	30	60	55.8	31669	PASS
95	95	100	100	100.0	56768	PASS
96	95	5	9	6.3	3597	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	90.8	51557	PASS
175	174	5	9	8.0	4103	PASS
176	174	95	101	95.9	49456	PASS
177	176	5	9	6.3	3139	PASS