




Data File : VU029926.D
Acq On : 09 Mar 2019 17:38
Operator : JC/SP
Sample : K1789-20
Misc : 5.67g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF0Q3

Manual Integrations
APPROVED

MMDadoda
3/11/2019 10:54:25 AM

Quant Time: Mar 11 02:25:52 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031119WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 11 02:20:19 2019
Response via : Initial Calibration

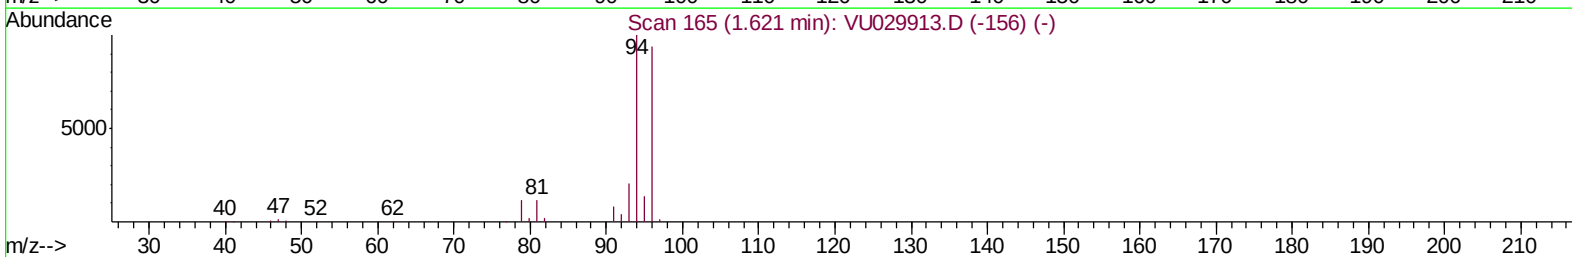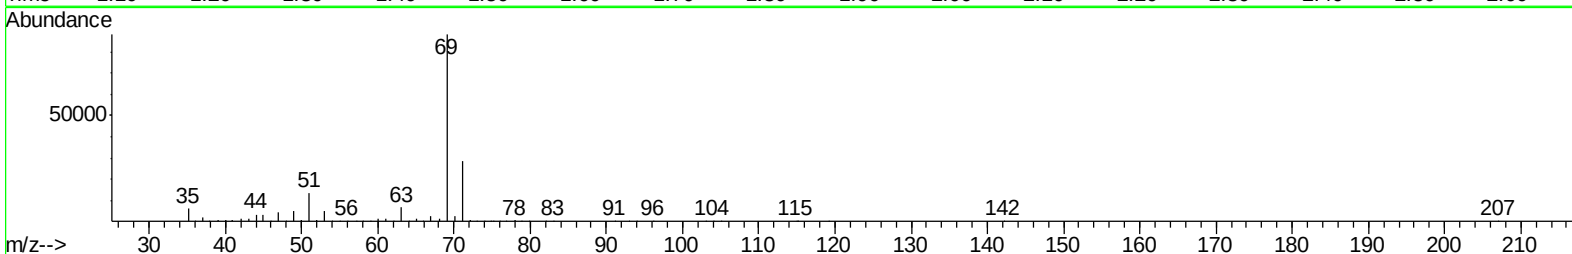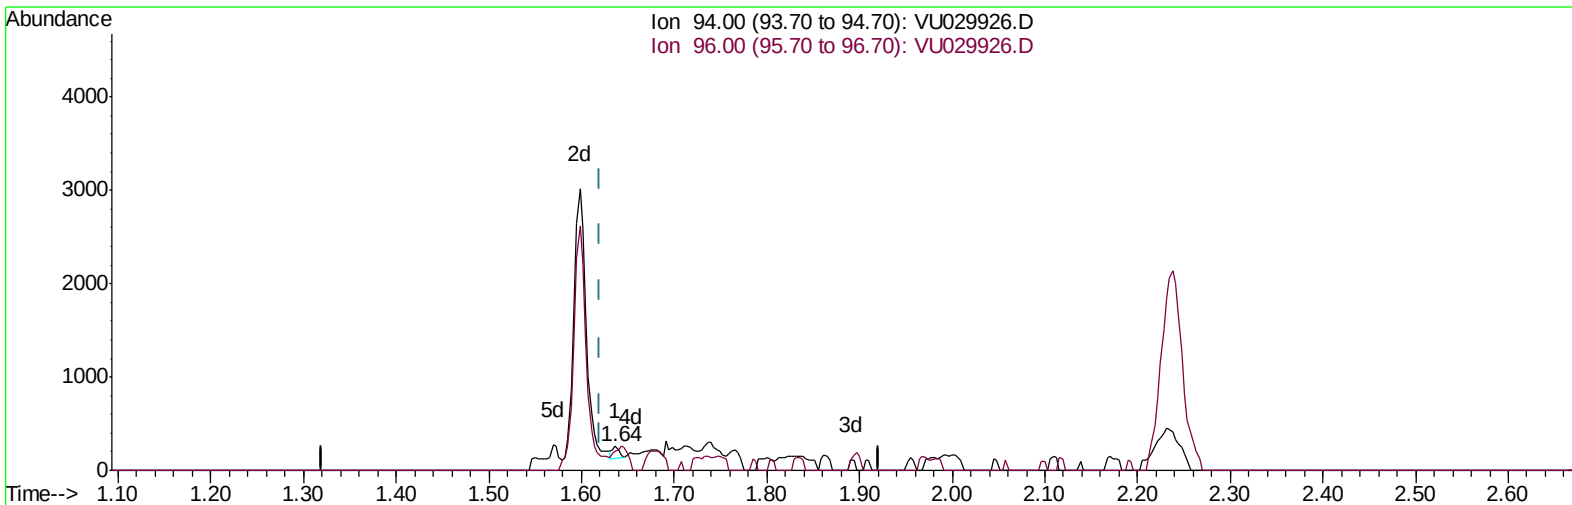

TIC: VU029926.D

(6) Bromomethane (T)

1.637min (+0.016) 0.03ug/L

response 63

Ion	Exp%	Act%
94.00	100	100
96.00	93.80	79.38
0.00	0.00	0.00
0.00	0.00	0.00




Data File : VU029926.D
Acq On : 09 Mar 2019 17:38
Operator : JC/SP
Sample : K1789-20
Misc : 5.67g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF0Q3

Manual Integrations
APPROVED

MMDadoda
3/11/2019 10:54:25 AM

Quant Time: Mar 11 02:25:52 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031119WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 11 02:20:19 2019
Response via : Initial Calibration

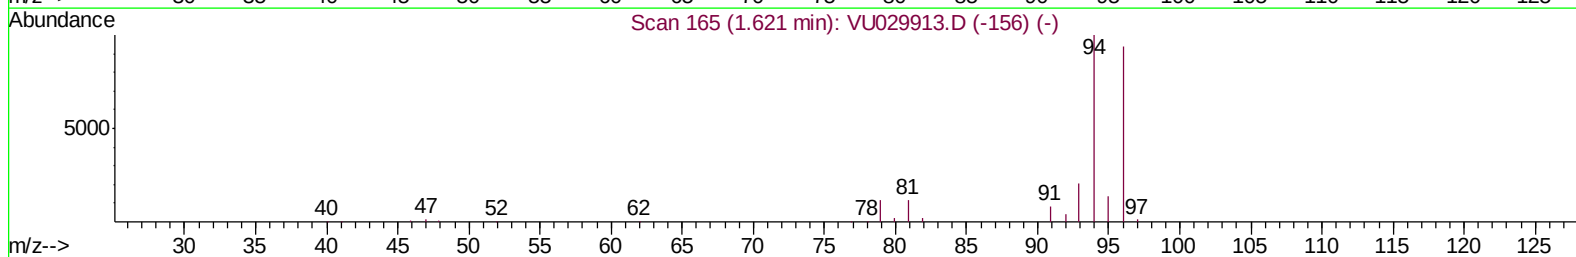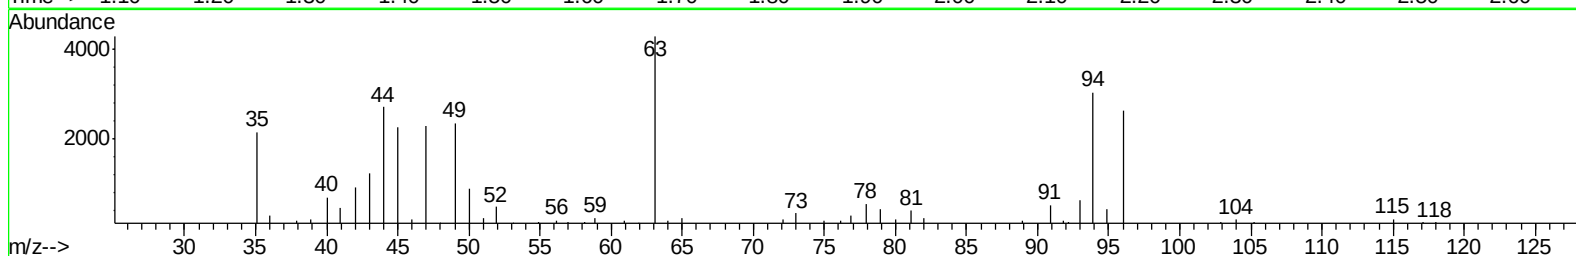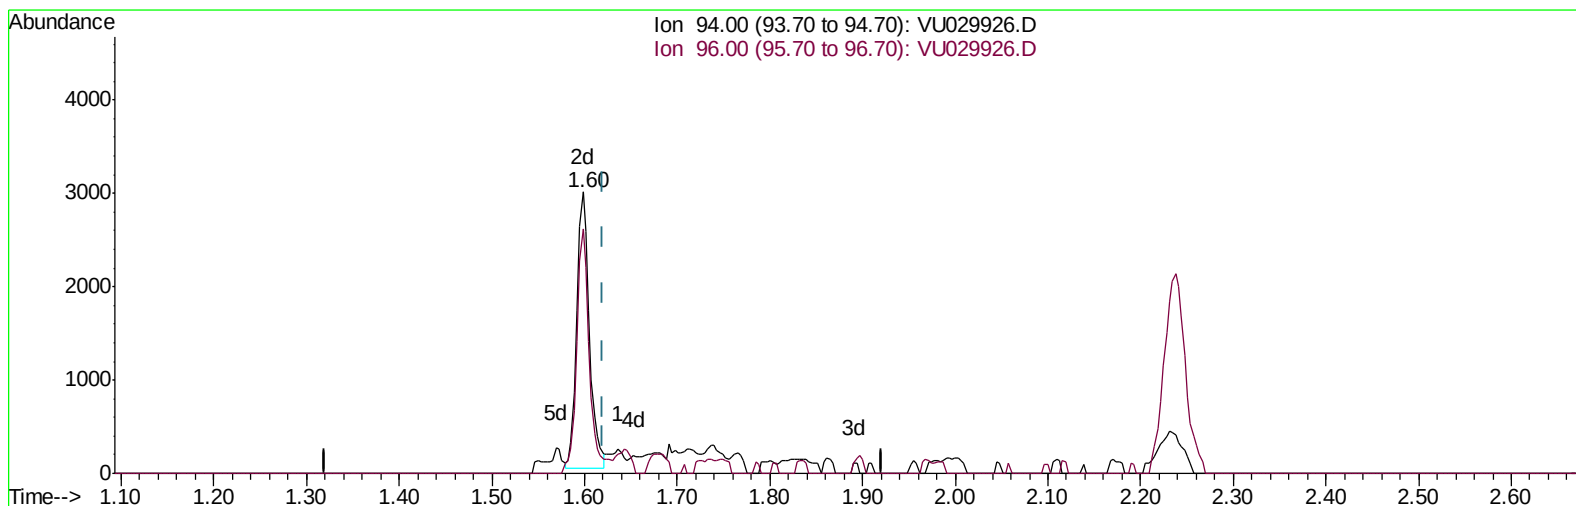

TIC: VU029926.D

(6) Bromomethane (T)

1.598min (-0.023) 1.21ug/L m

response 2870

Ion	Exp%	Act%
94.00	100	100
96.00	93.80	86.87
0.00	0.00	0.00
0.00	0.00	0.00

Data File : VU029926.D
Acq On : 09 Mar 2019 17:38
Operator : JC/SP
Sample : K1789-20
Misc : 5.67g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF0Q3

Manual Integrations
APPROVED

MMDadoda
3/11/2019 10:54:25 AM

Quant Time: Mar 11 03:54:40 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031119WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 11 02:20:19 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	1142574	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	1160574	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	625627	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	236801	33.97	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	67.94%
7) Chloroethane-d5	1.64	69	102297	17.46	ug/L	-0.04
Spiked Amount	50.000	Range	70 - 130	Recovery	=	34.92%#
11) 1,1-Dichloroethene-d2	2.23	63	328884	25.03	ug/L	-0.04
Spiked Amount	50.000	Range	60 - 125	Recovery	=	50.06%#
21) 2-Butanone-d5	4.19	46	366212	67.80	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	67.80%
24) Chloroform-d	4.64	84	427241	31.49	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	62.98%#
26) 1,2-Dichloroethane-d4	5.30	65	266150	33.48	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	66.96%#
32) Benzene-d6	5.33	84	937208	32.41	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	64.82%#
36) 1,2-Dichloropropane-d6	6.32	67	284702	32.59	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	65.18%#
41) Toluene-d8	7.56	98	897863	32.35	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	64.70%#
43) trans-1,3-Dichloropropene-	7.85	79	133839	31.66	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	63.32%
47) 2-Hexanone-d5	8.32	63	357196	76.00	ug/L	0.01
Spiked Amount	100.000	Range	45 - 130	Recovery	=	76.00%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	497535	36.07	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	72.14%
64) 1,2-Dichlorobenzene-d4	11.86	152	411705	33.55	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	67.10%#

Target Compounds					Qvalue
3) Chloromethane	1.32	50	58156	5.042 ug/L	99
6) Bromomethane	1.60	94	2870m	1.212 ug/L	
46) Tetrachloroethene	8.22	164	381950	53.078 ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VU029926.D
Acq On : 09 Mar 2019 17:38
Operator : JC/SP
Sample : K1789-20
Misc : 5.67g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF0Q3

Manual Integrations
APPROVED

MMDadoda
3/11/2019 10:54:25 AM

Quant Time: Mar 11 03:54:40 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031119WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 11 02:20:19 2019
Response via : Initial Calibration

