




Data File : VU029927.D
Acq On : 09 Mar 2019 18:02
Operator : JC/SP
Sample : K1789-21
Misc : 5.70g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF0Q4

Manual Integrations
APPROVED

MMDadoda
3/11/2019 10:54:30 AM

Quant Time: Mar 11 02:25:58 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031119WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 11 02:20:19 2019
Response via : Initial Calibration

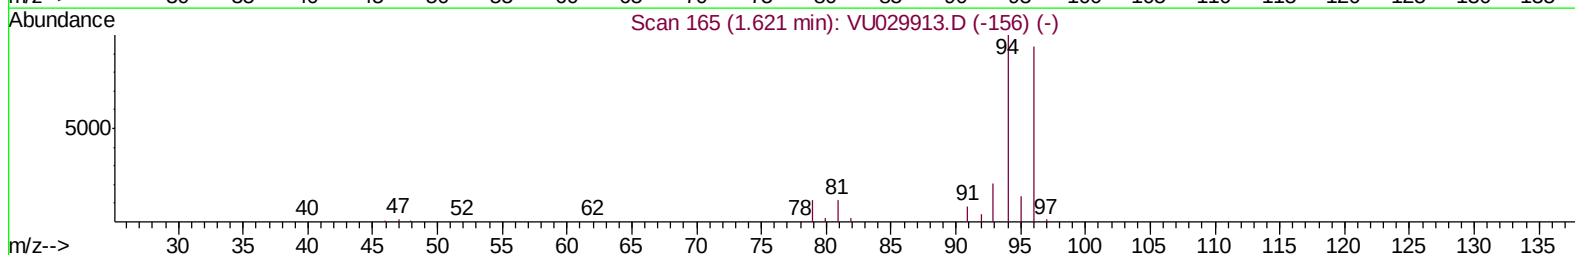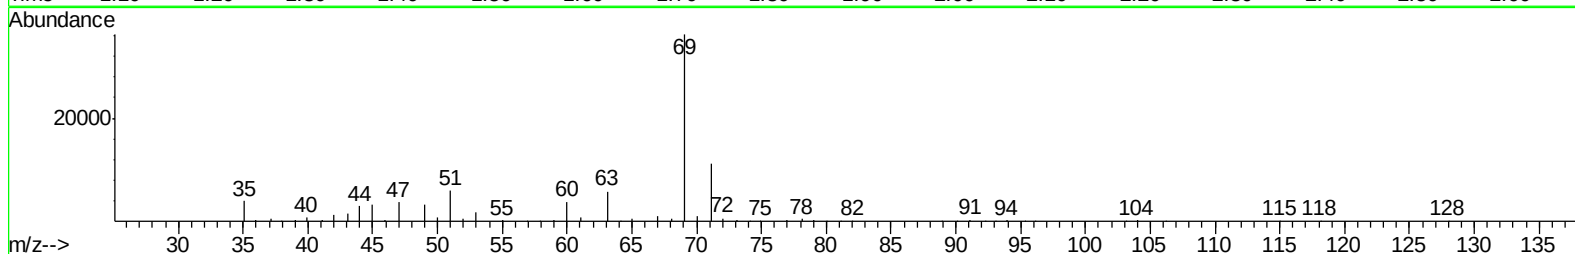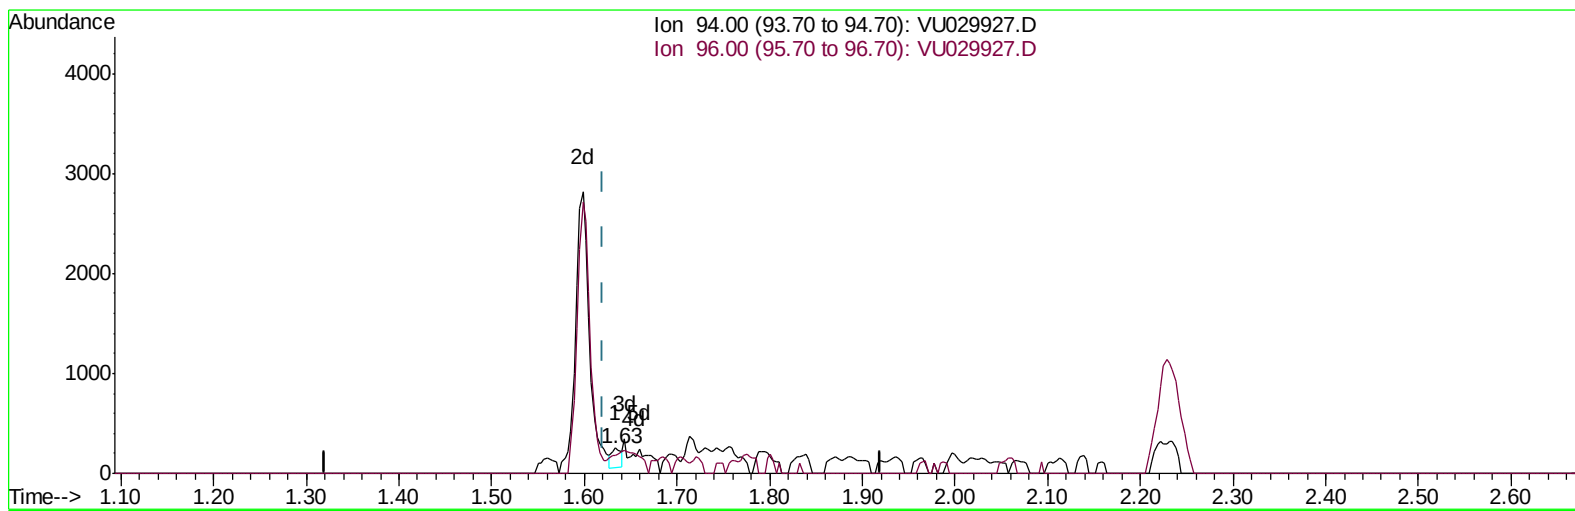

TIC: VU029927.D

(6) Bromomethane (T)

1.634min (+0.013) 0.11ug/L

response 134

Ion	Exp%	Act%
94.00	100	100
96.00	93.80	72.27
0.00	0.00	0.00
0.00	0.00	0.00




Data File : VU029927.D
Acq On : 09 Mar 2019 18:02
Operator : JC/SP
Sample : K1789-21
Misc : 5.70g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF0Q4

Manual Integrations
APPROVED

MMDadoda
3/11/2019 10:54:30 AM

Quant Time: Mar 11 02:25:58 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031119WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 11 02:20:19 2019
Response via : Initial Calibration

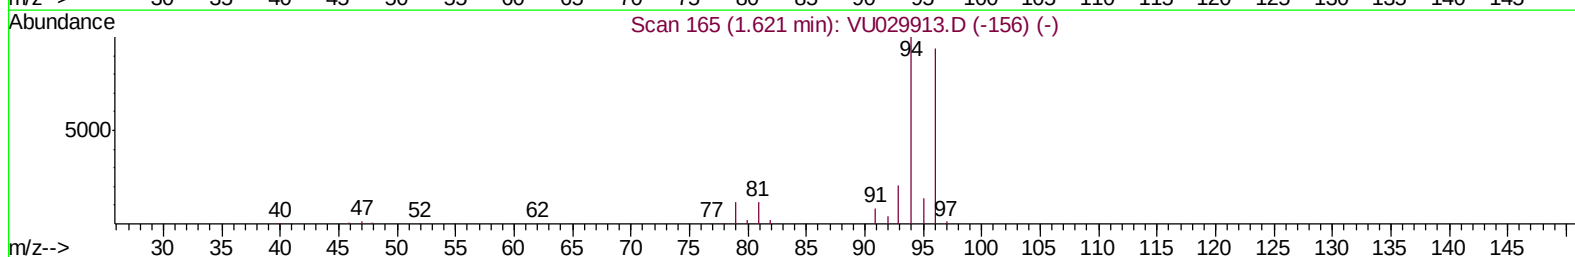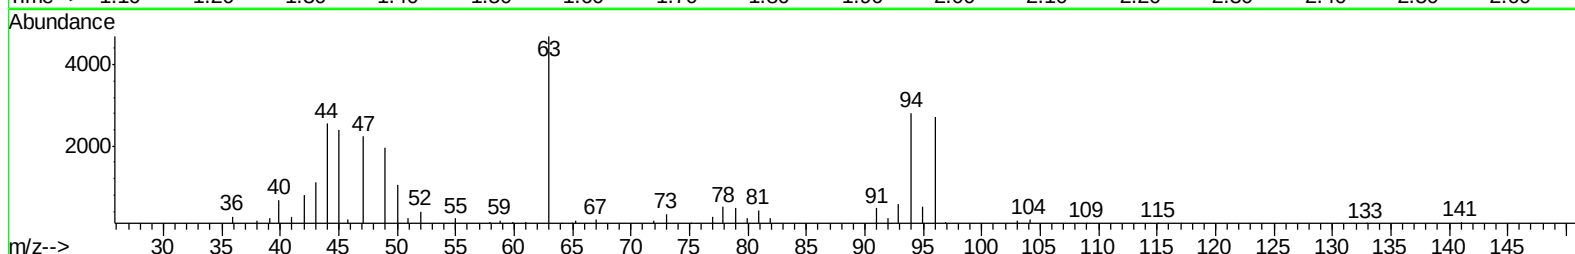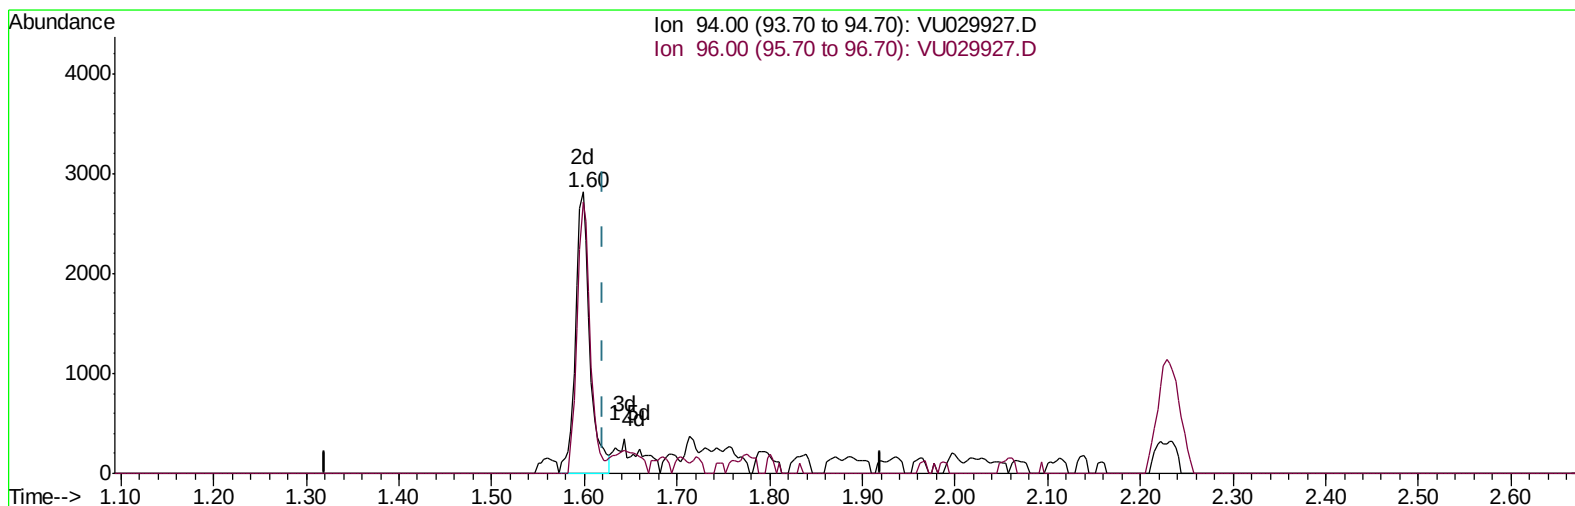

TIC: VU029927.D

(6) Bromomethane (T)

1.598min (-0.022) 2.60ug/L m

response 3060

Ion	Exp%	Act%
94.00	100	100
96.00	93.80	96.16
0.00	0.00	0.00
0.00	0.00	0.00




Data File : VU029927.D
Acq On : 09 Mar 2019 18:02
Operator : JC/SP
Sample : K1789-21
Misc : 5.70g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF0Q4

Manual Integrations
APPROVED

MMDadoda
3/11/2019 10:54:30 AM

Quant Time: Mar 11 02:25:58 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031119WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 11 02:20:19 2019
Response via : Initial Calibration

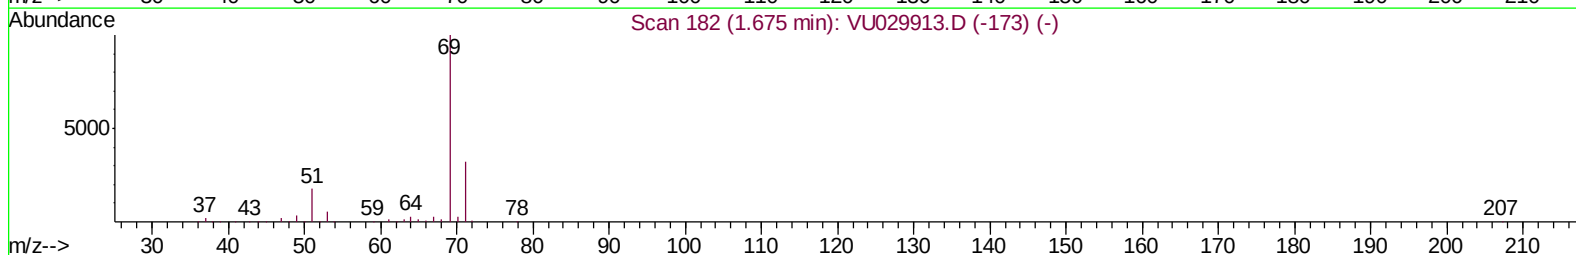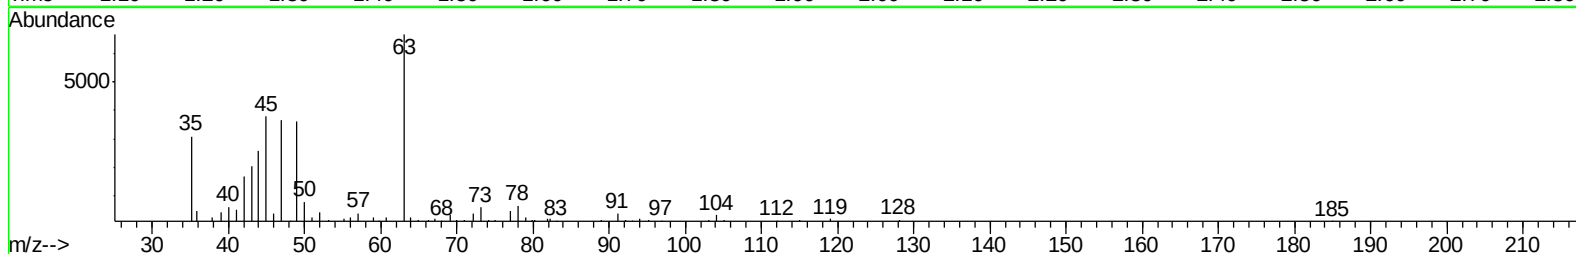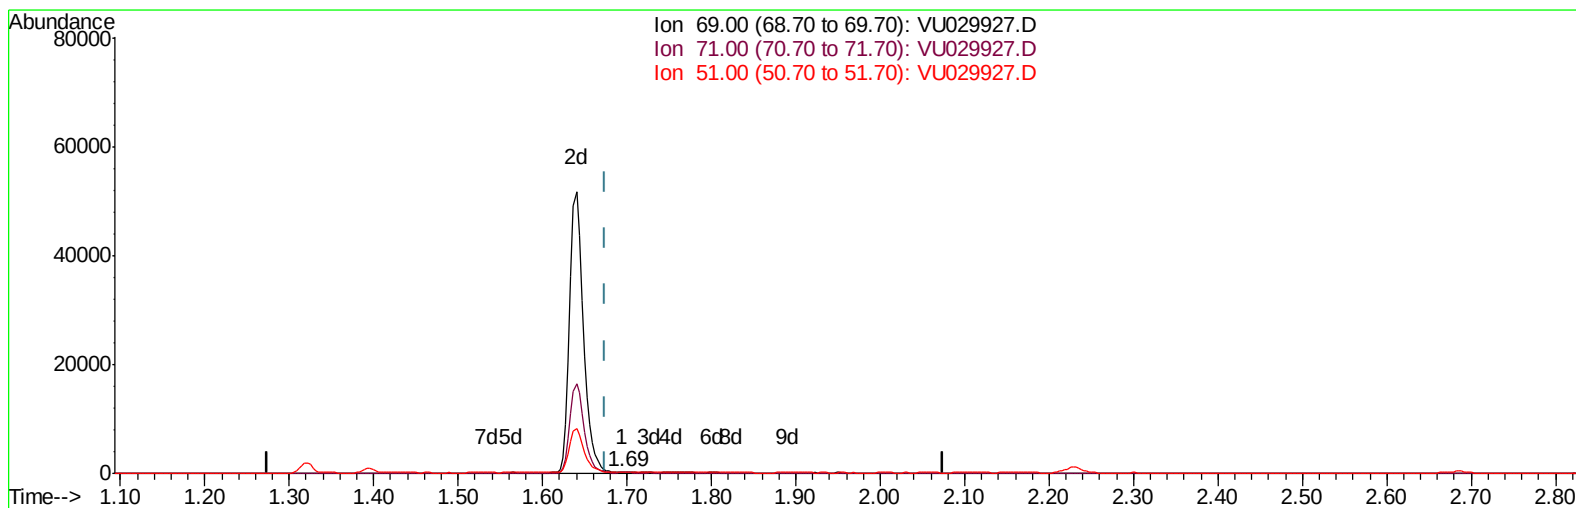

TIC: VU029927.D

(7) Chloroethane-d5 (S)

1.695min (+0.019) 0.03ug/L

response 86

Ion	Exp%	Act%
69.00	100	100
71.00	31.90	218.60#
51.00	24.10	210.47#
0.00	0.00	0.00




Data File : VU029927.D
Acq On : 09 Mar 2019 18:02
Operator : JC/SP
Sample : K1789-21
Misc : 5.70g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF0Q4

Manual Integrations
APPROVED

MMDadoda
3/11/2019 10:54:30 AM

Quant Time: Mar 11 02:25:58 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031119WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 11 02:20:19 2019
Response via : Initial Calibration

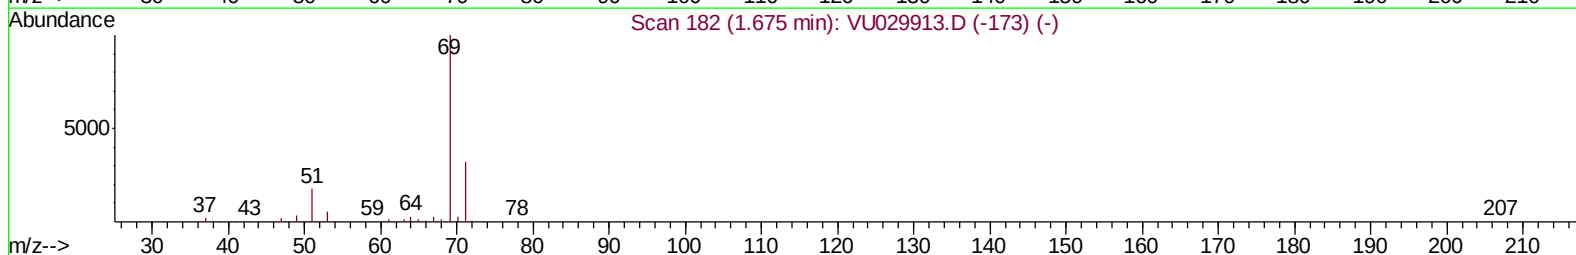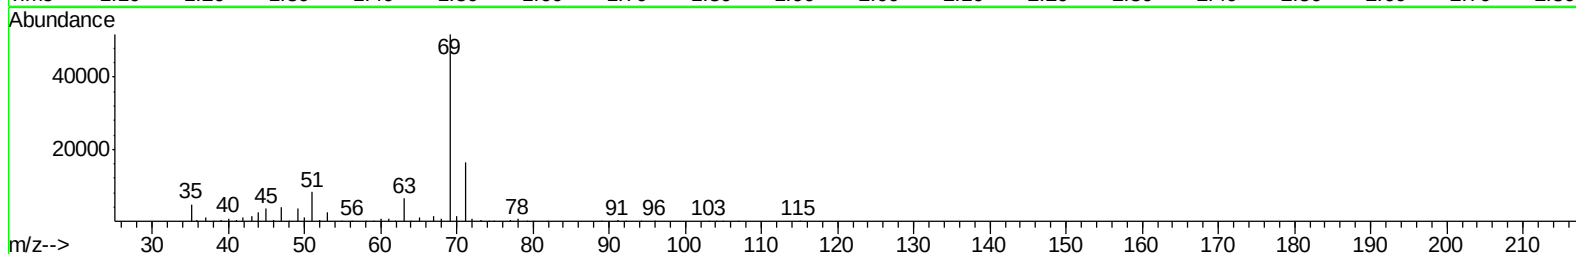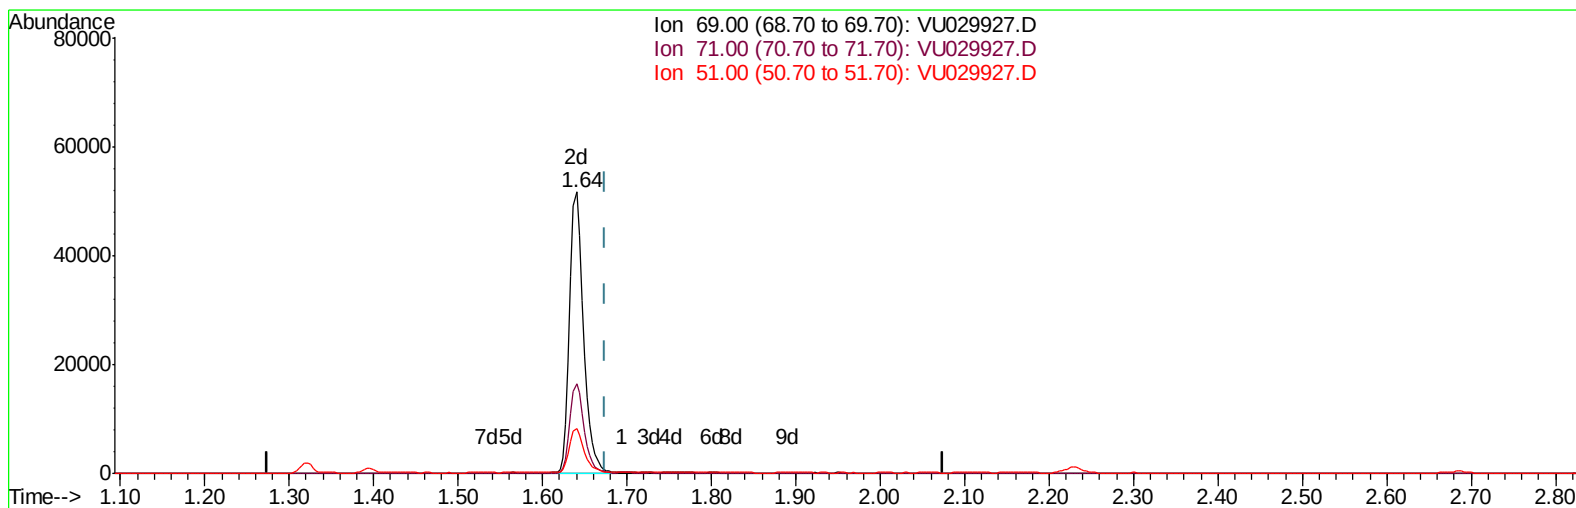

TIC: VU029927.D

(7) Chloroethane-d5 (S)

1.640min (-0.035) 20.26ug/L m

response 58929

Ion	Exp%	Act%
69.00	100	100
71.00	31.90	0.32#
51.00	24.10	0.31#
0.00	0.00	0.00




Data File : VU029927.D
Acq On : 09 Mar 2019 18:02
Operator : JC/SP
Sample : K1789-21
Misc : 5.70g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF0Q4

Manual Integrations
APPROVED

MMDadoda
3/11/2019 10:54:30 AM

Quant Time: Mar 11 02:25:58 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031119WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 11 02:20:19 2019
Response via : Initial Calibration

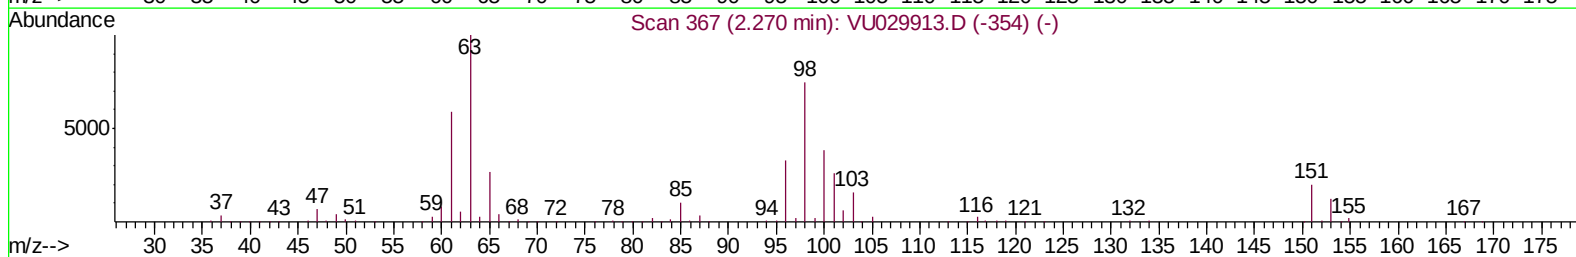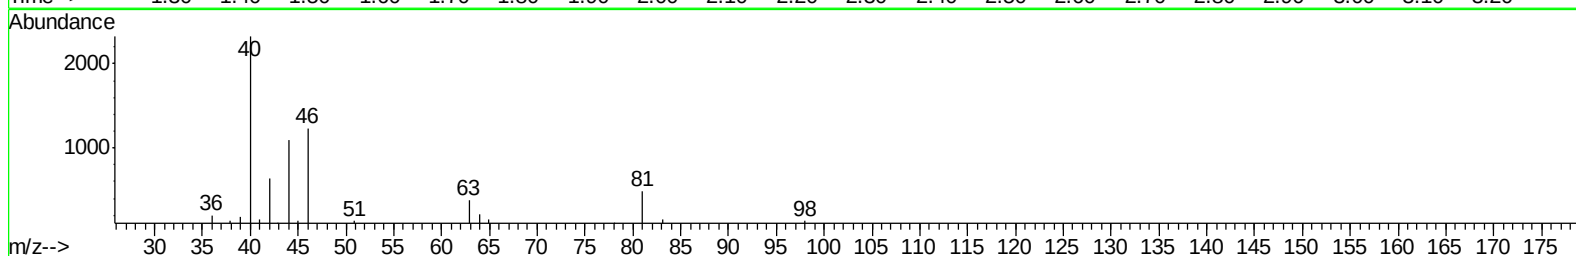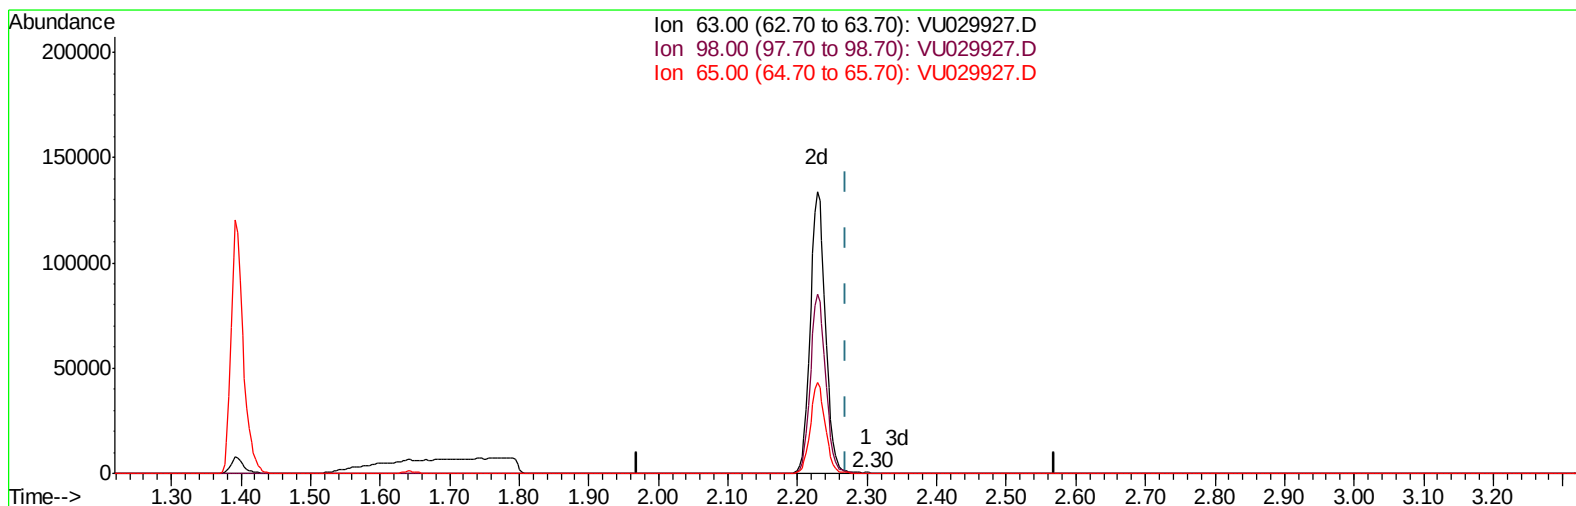

TIC: VU029927.D

(11) 1,1-Dichloroethene-d2 (S)

2.299min (+0.029) 0.05ug/L

response 337

Ion	Exp%	Act%
63.00	100	100
98.00	82.90	0.00#
65.00	23.60	31.75#
0.00	0.00	0.00




Data File : VU029927.D
Acq On : 09 Mar 2019 18:02
Operator : JC/SP
Sample : K1789-21
Misc : 5.70g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF0Q4

Manual Integrations
APPROVED

MMDadoda
3/11/2019 10:54:30 AM

Quant Time: Mar 11 02:25:58 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031119WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 11 02:20:19 2019
Response via : Initial Calibration

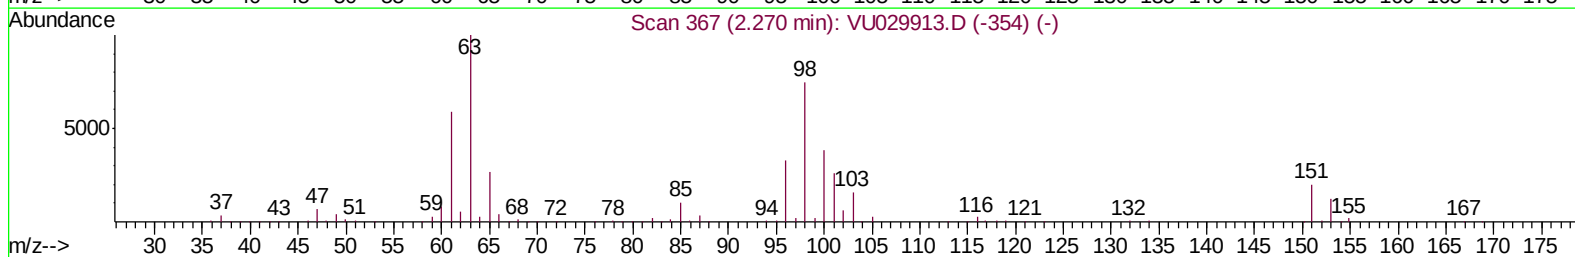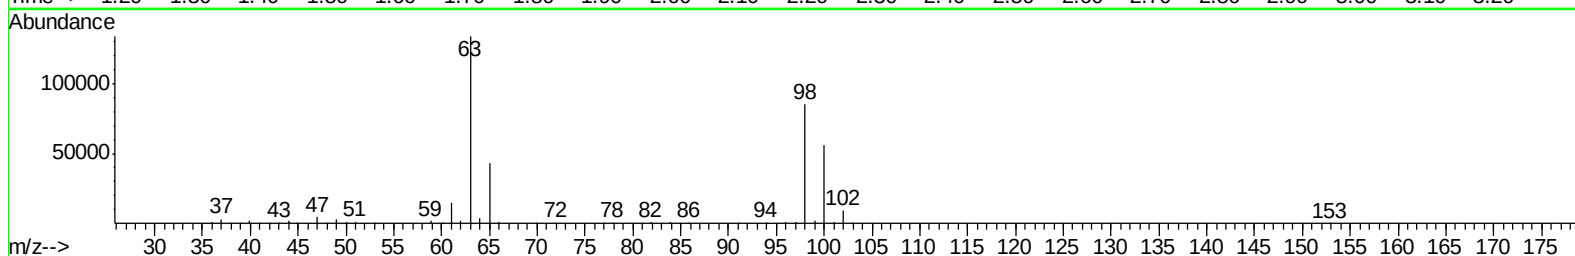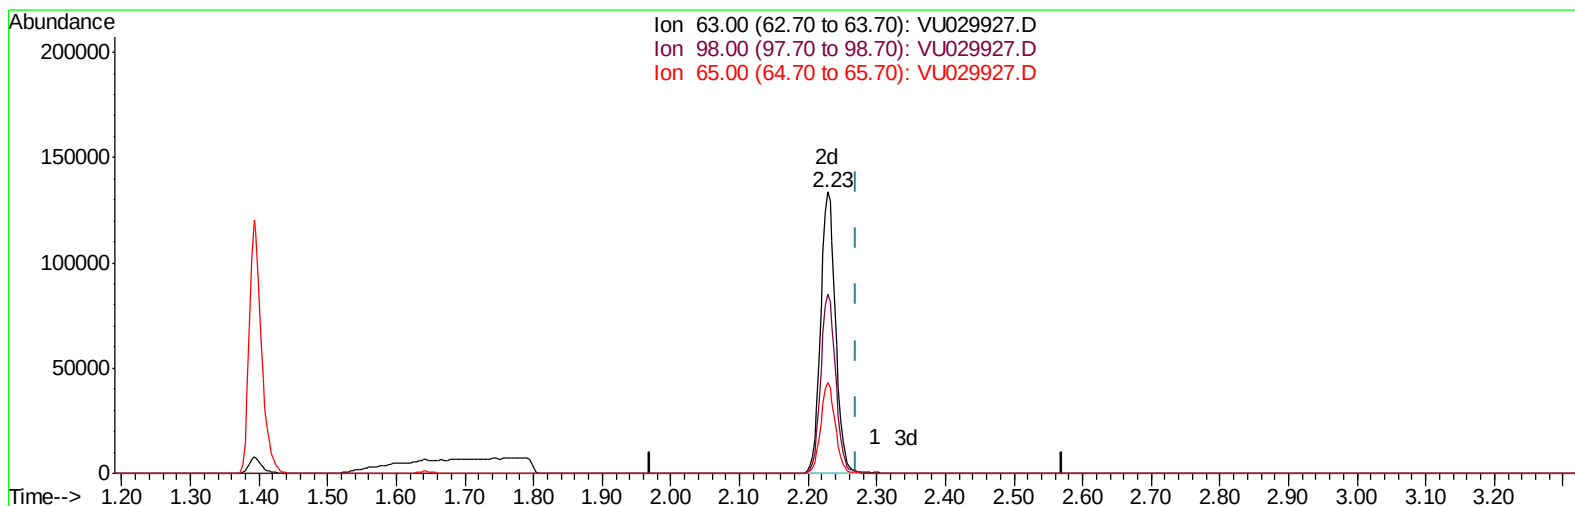

TIC: VU029927.D

(11) 1,1-Dichloroethene-d2 (S)

2.228min (-0.042) 30.90ug/L m

response 201542

Ion	Exp%	Act%
63.00	100	100
98.00	82.90	0.00#
65.00	23.60	0.05#
0.00	0.00	0.00

Data File : VU029927.D
Acq On : 09 Mar 2019 18:02
Operator : JC/SP
Sample : K1789-21
Misc : 5.70g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF0Q4

Manual Integrations
APPROVED

MMDadoda
3/11/2019 10:54:30 AM

Quant Time: Mar 11 03:57:51 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031119WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 11 02:20:19 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	567119	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	568560	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	303435	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	146233	42.26	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	84.52%
7) Chloroethane-d5	1.64	69	58929m	20.26	ug/L	-0.04
Spiked Amount	50.000	Range	70 - 130	Recovery	=	40.52%#
11) 1,1-Dichloroethene-d2	2.23	63	201542m	30.90	ug/L	-0.04
Spiked Amount	50.000	Range	60 - 125	Recovery	=	61.80%
21) 2-Butanone-d5	4.19	46	223013	83.19	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	83.19%
24) Chloroform-d	4.64	84	263175	39.08	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	78.16%
26) 1,2-Dichloroethane-d4	5.30	65	161585	40.95	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	81.90%
32) Benzene-d6	5.33	84	576364	40.68	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	81.36%
36) 1,2-Dichloropropane-d6	6.32	67	172599	40.33	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	80.66%
41) Toluene-d8	7.56	98	542060	39.87	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	79.74%#
43) trans-1,3-Dichloropropene-	7.85	79	81158	39.19	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	78.38%
47) 2-Hexanone-d5	8.32	63	211640	91.91	ug/L	0.02
Spiked Amount	100.000	Range	45 - 130	Recovery	=	91.91%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	299741	44.36	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	88.72%
64) 1,2-Dichlorobenzene-d4	11.86	152	243591	40.93	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	81.86%

Target Compounds					Qvalue
3) Chloromethane	1.32	50	56559	9.880 ug/L	100
6) Bromomethane	1.60	94	3060m	2.603 ug/L	
46) Tetrachloroethene	8.22	164	61923	17.565 ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VU029927.D
Acq On : 09 Mar 2019 18:02
Operator : JC/SP
Sample : K1789-21
Misc : 5.70g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF0Q4

Manual Integrations
APPROVED

MMDadoda
3/11/2019 10:54:30 AM

Quant Time: Mar 11 03:57:51 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031119WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 11 02:20:19 2019
Response via : Initial Calibration

