

Data File : VU029929.D

Acq On : 09 Mar 2019 18:48

Operator : JC/SP

Sample : K1838-02

Misc : 5.70g/5mL/100uL/5.0mL/MSVOA_U/MEOH

ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF0S3

Manual Integrations
APPROVED

MMDadoda
3/11/2019 10:54:38 AM




Quant Time: Mar 11 02:26:12 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031119WMA.M

Quant Title : VOC Analysis

QLast Update : Mon Mar 11 02:20:19 2019

Response via : Initial Calibration

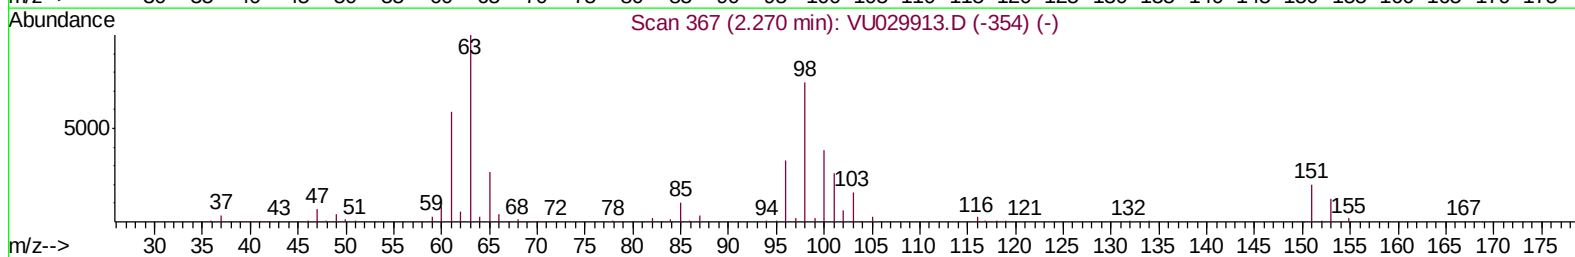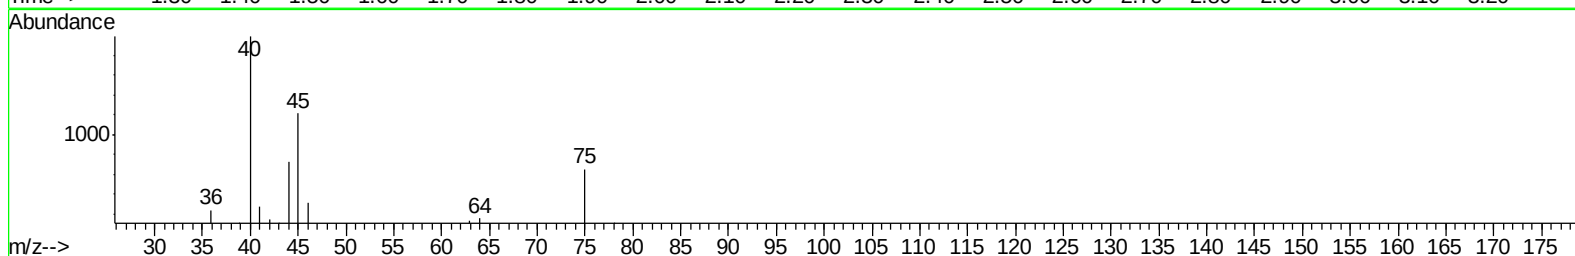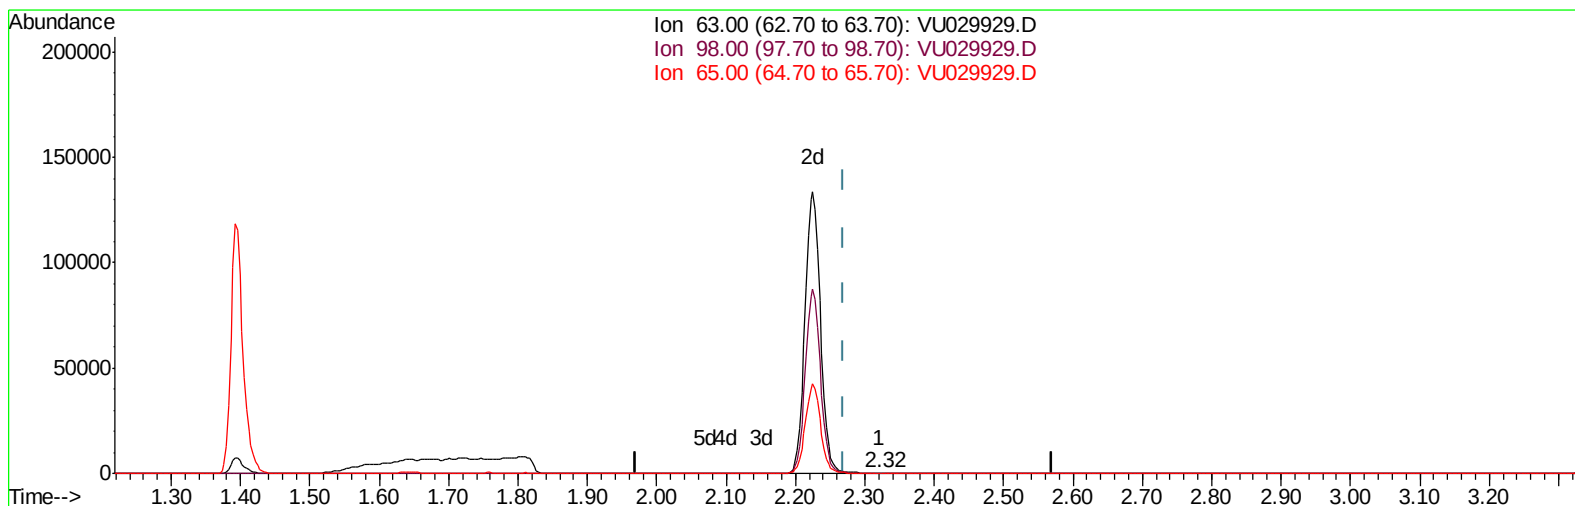

TIC: VU029929.D

(11) 1,1-Dichloroethene-d2 (S)

2.322min (+0.051) 0.01ug/L

response 72

Ion	Exp%	Act%
63.00	100	100
98.00	82.90	0.00#
65.00	23.60	162.50#
0.00	0.00	0.00




Data File : VU029929.D
Acq On : 09 Mar 2019 18:48
Operator : JC/SP
Sample : K1838-02
Misc : 5.70g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF0S3

Manual Integrations
APPROVED

MMDadoda
3/11/2019 10:54:38 AM

Quant Time: Mar 11 02:26:12 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031119WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 11 02:20:19 2019
Response via : Initial Calibration

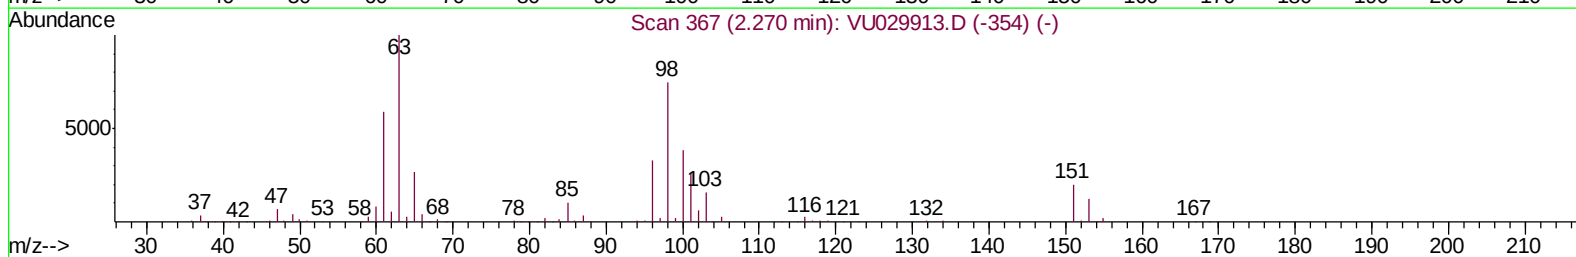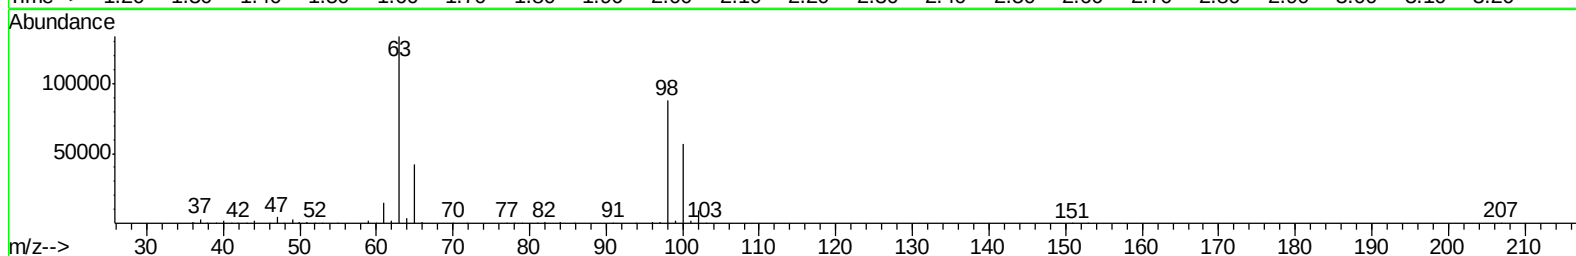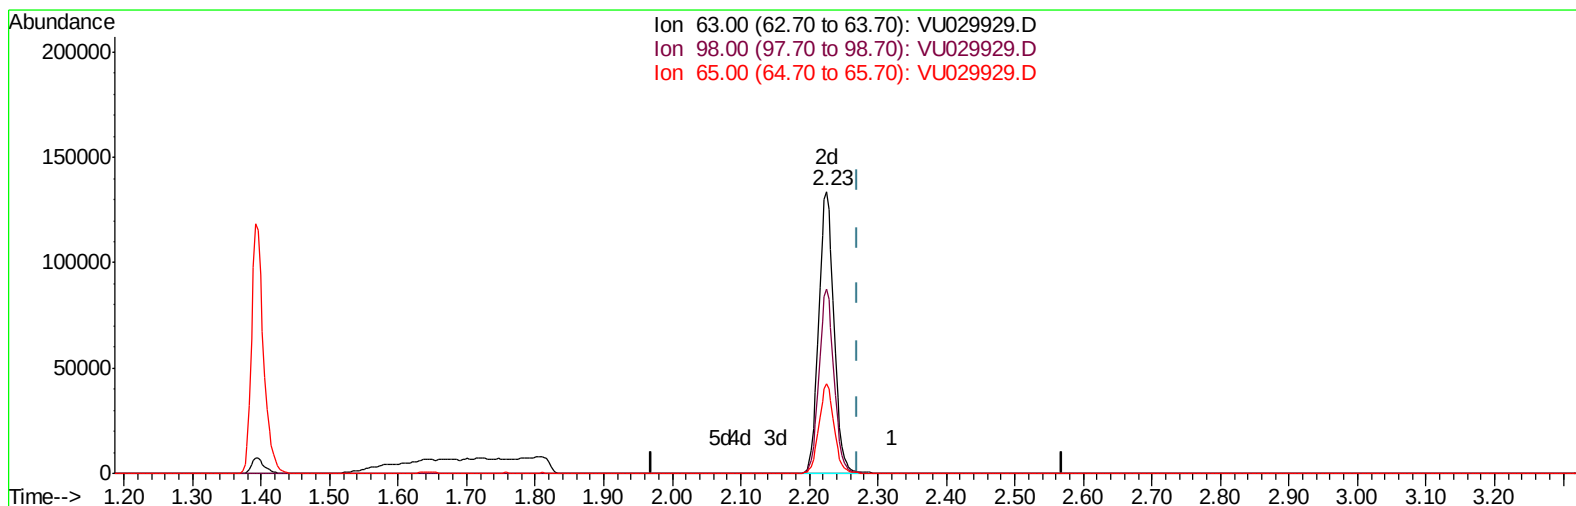

TIC: VU029929.D

(11) 1,1-Dichloroethene-d2 (S)

2.225min (-0.045) 31.72ug/L m

response 205891

Ion	Exp%	Act%
63.00	100	100
98.00	82.90	0.00#
65.00	23.60	0.06#
0.00	0.00	0.00

Data File : VU029929.D
Acq On : 09 Mar 2019 18:48
Operator : JC/SP
Sample : K1838-02
Misc : 5.70g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF0S3

Manual Integrations
APPROVED

MMDadoda
3/11/2019 10:54:38 AM

Quant Time: Mar 11 04:04:55 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031119WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 11 02:20:19 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	564450	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	560907	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	288874	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	142639	41.42	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	82.84%
7) Chloroethane-d5	1.64	69	56183	19.41	ug/L	-0.04
Spiked Amount	50.000	Range	70 - 130	Recovery	=	38.82%#
11) 1,1-Dichloroethene-d2	2.23	63	205891m	31.72	ug/L	-0.05
Spiked Amount	50.000	Range	60 - 125	Recovery	=	63.44%
21) 2-Butanone-d5	4.20	46	219962	82.44	ug/L	0.03
Spiked Amount	100.000	Range	40 - 130	Recovery	=	82.44%
24) Chloroform-d	4.64	84	262078	39.10	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	78.20%
26) 1,2-Dichloroethane-d4	5.30	65	161432	41.11	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	82.22%
32) Benzene-d6	5.33	84	582967	41.71	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	83.42%
36) 1,2-Dichloropropane-d6	6.32	67	175335	41.53	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	83.06%
41) Toluene-d8	7.56	98	536306	39.99	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	79.98%#
43) trans-1,3-Dichloropropene-	7.85	79	80096	39.20	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	78.40%
47) 2-Hexanone-d5	8.32	63	204763	90.14	ug/L	0.02
Spiked Amount	100.000	Range	45 - 130	Recovery	=	90.14%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	285951	42.90	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	85.80%
64) 1,2-Dichlorobenzene-d4	11.86	152	237099	41.85	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	83.70%

Target Compounds					Qvalue
3) Chloromethane	1.32	50	75762	13.297 ug/L	100
6) Bromomethane	1.60	94	3677	3.142 ug/L	91
46) Tetrachloroethene	8.22	164	293418	84.368 ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VU029929.D
Acq On : 09 Mar 2019 18:48
Operator : JC/SP
Sample : K1838-02
Misc : 5.70g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF0S3

Manual Integrations
APPROVED

MMDadoda
3/11/2019 10:54:38 AM

Quant Time: Mar 11 04:04:55 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031119WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 11 02:20:19 2019
Response via : Initial Calibration

