




Data File : VU029931.D
Acq On : 09 Mar 2019 19:34
Operator : JC/SP
Sample : K1838-04
Misc : 5.71g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1J2

Manual Integrations
APPROVED

MMDadoda
3/11/2019 10:54:43 AM

Quant Time: Mar 11 02:26:27 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031119WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 11 02:20:19 2019
Response via : Initial Calibration

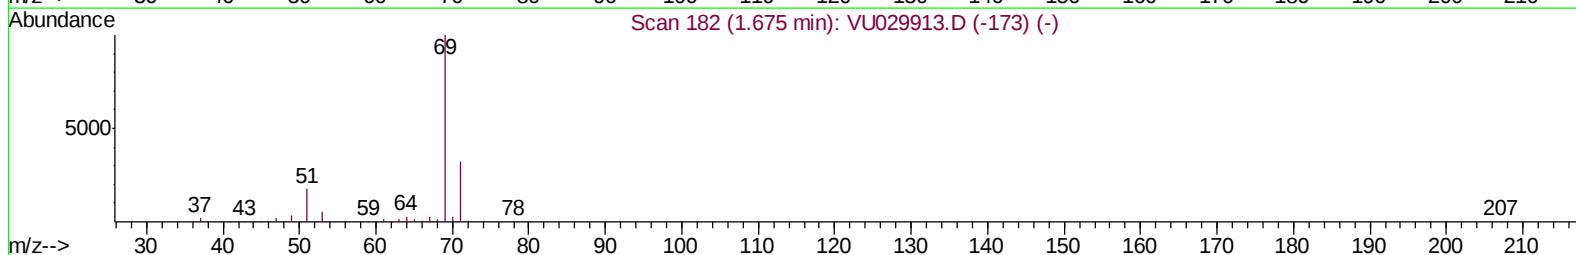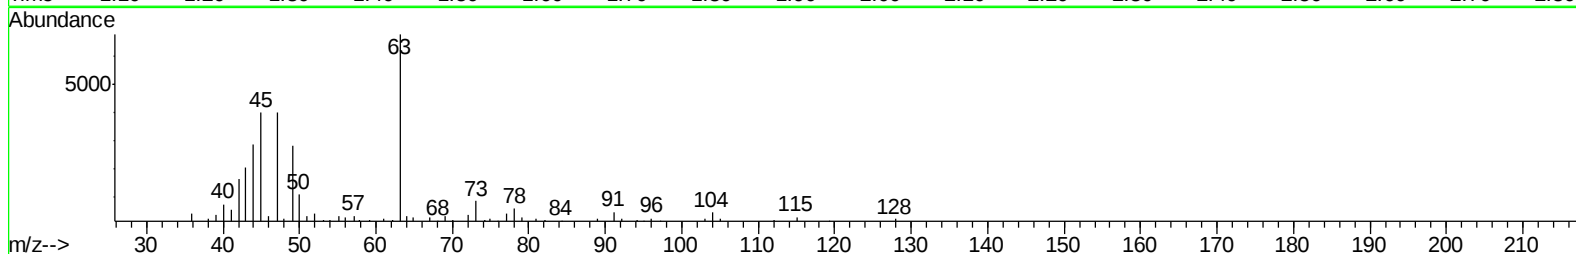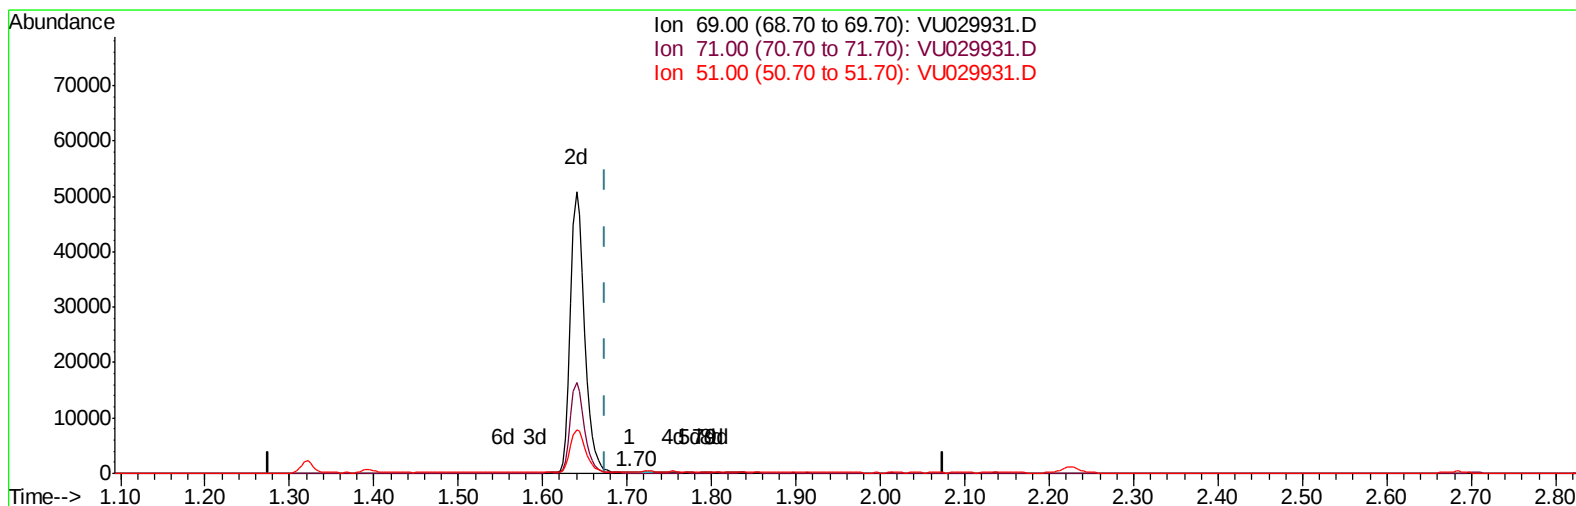

TIC: VU029931.D

(7) Chloroethane-d5 (S)

1.704min (+0.029) 0.06ug/L

response 163

Ion	Exp%	Act%
69.00	100	100
71.00	31.90	26.38
51.00	24.10	53.99#
0.00	0.00	0.00




Data File : VU029931.D
Acq On : 09 Mar 2019 19:34
Operator : JC/SP
Sample : K1838-04
Misc : 5.71g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1J2

Manual Integrations
APPROVED

MMDadoda
3/11/2019 10:54:43 AM

Quant Time: Mar 11 02:26:27 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031119WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 11 02:20:19 2019
Response via : Initial Calibration

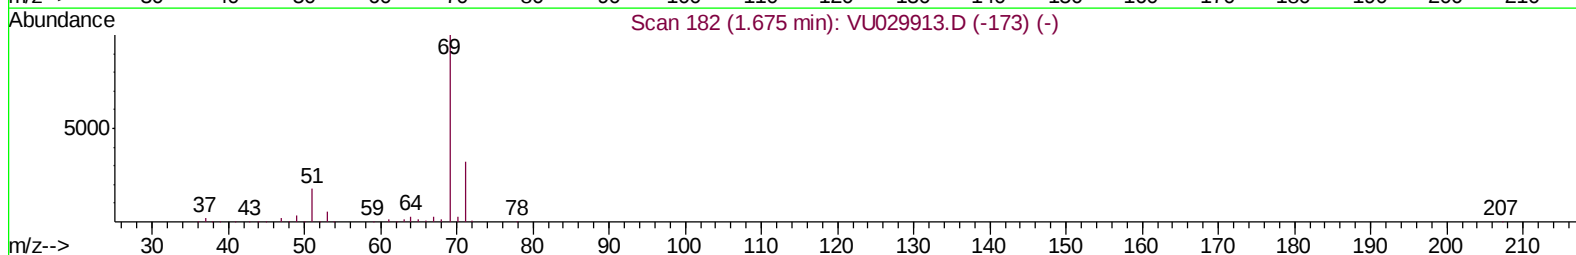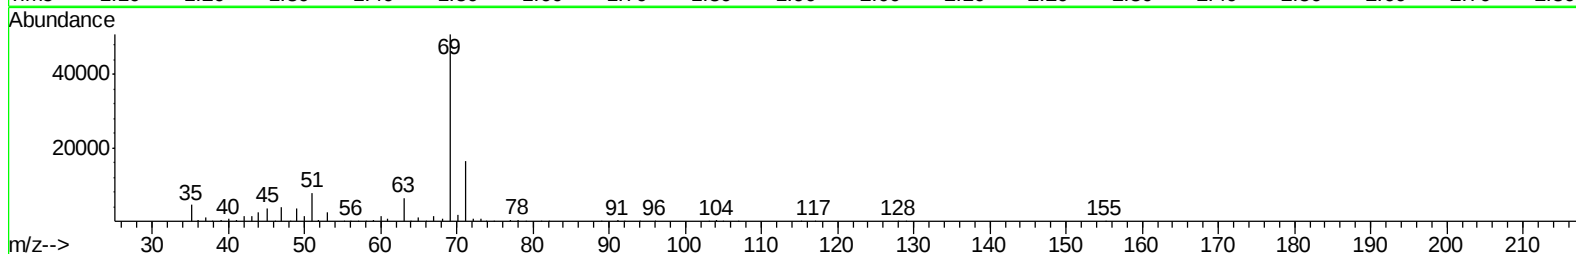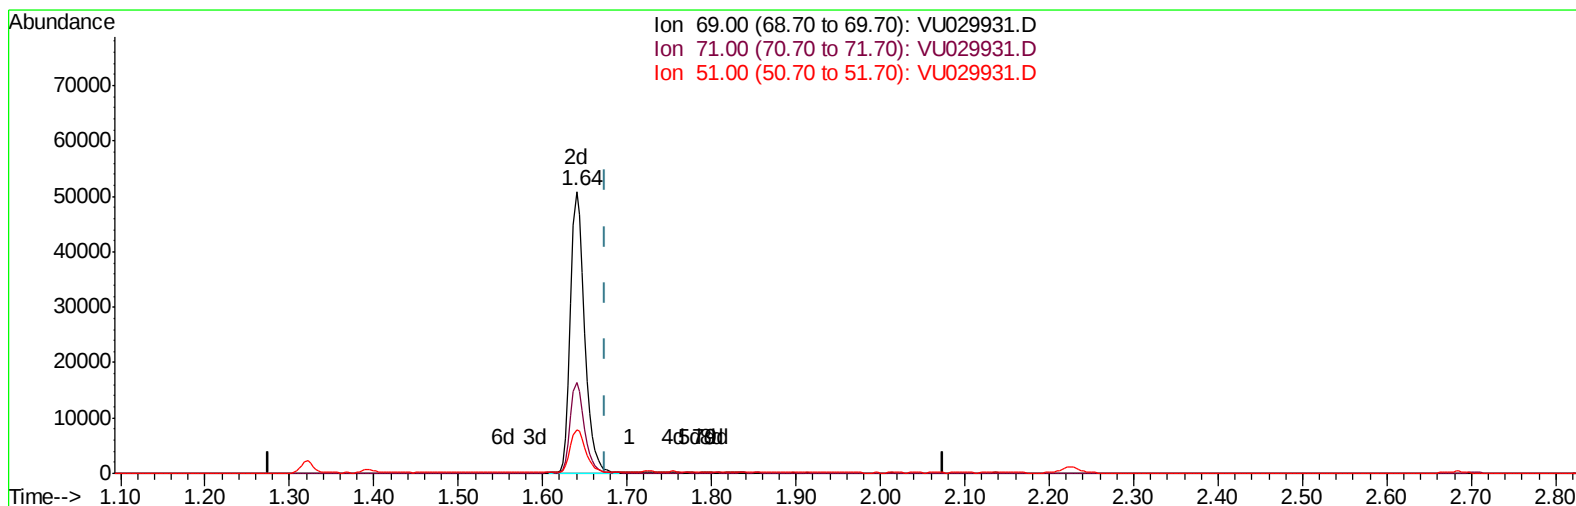

TIC: VU029931.D

(7) Chloroethane-d5 (S)

1.640min (-0.035) 19.88ug/L m

response 58722

Ion	Exp%	Act%
69.00	100	100
71.00	31.90	0.07#
51.00	24.10	0.15#
0.00	0.00	0.00




Data File : VU029931.D
Acq On : 09 Mar 2019 19:34
Operator : JC/SP
Sample : K1838-04
Misc : 5.71g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1J2

Manual Integrations
APPROVED

MMDadoda
3/11/2019 10:54:43 AM

Quant Time: Mar 11 02:26:27 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031119WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 11 02:20:19 2019
Response via : Initial Calibration

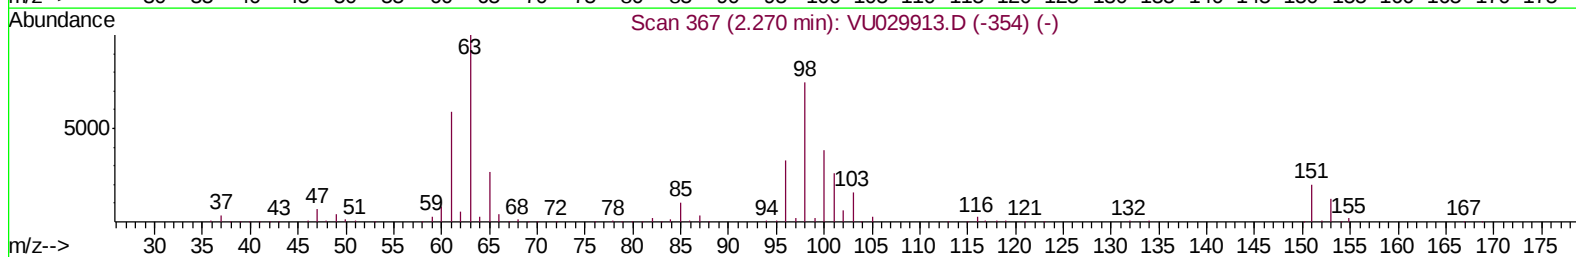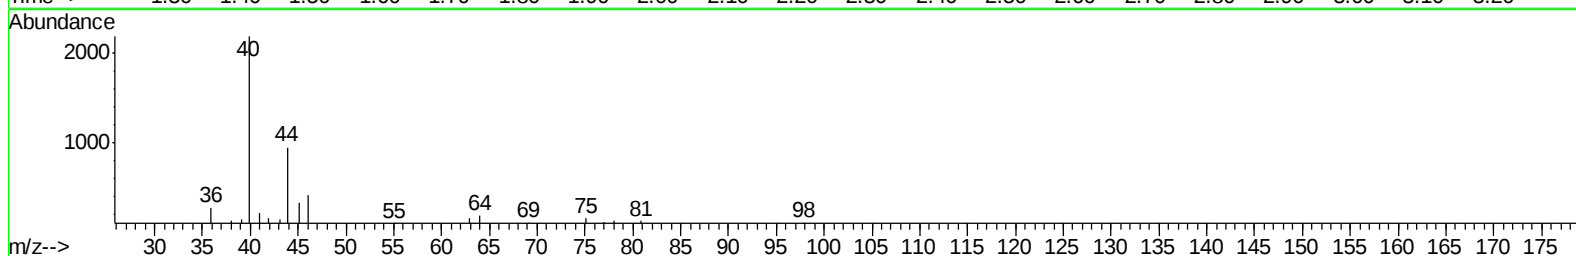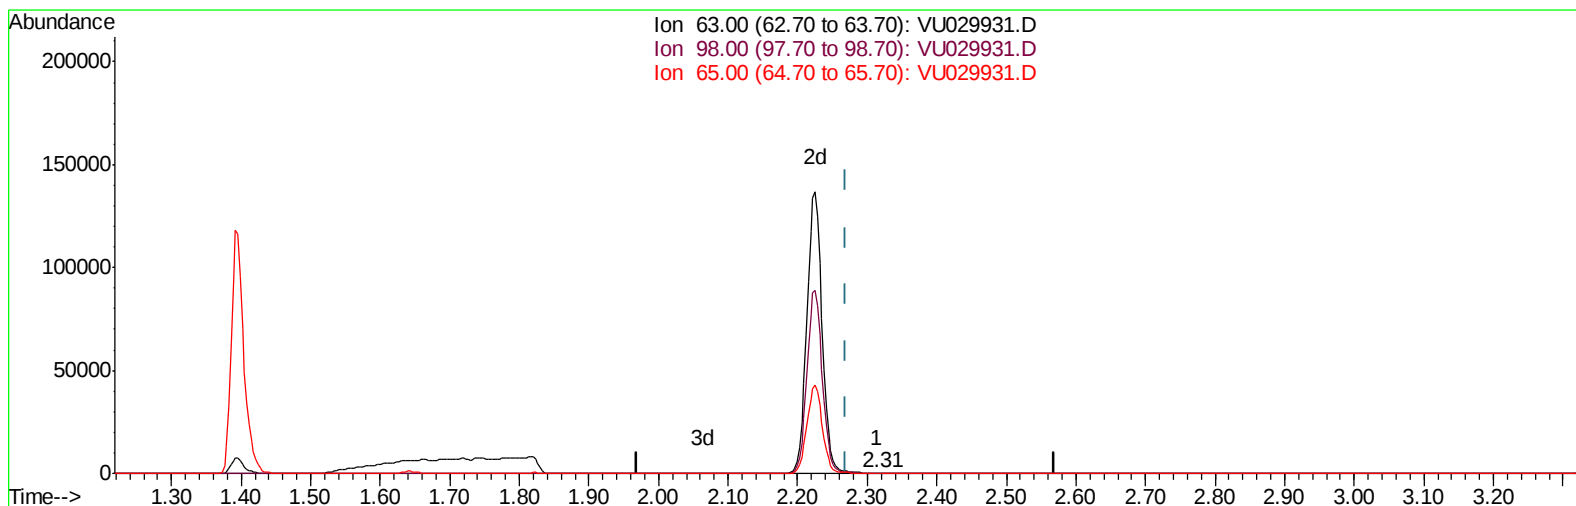

TIC: VU029931.D

(11) 1,1-Dichloroethene-d2 (S)

2.315min (+0.045) 0.01ug/L

response 83

Ion	Exp%	Act%
63.00	100	100
98.00	82.90	87.95
65.00	23.60	127.71#
0.00	0.00	0.00




Data File : VU029931.D
Acq On : 09 Mar 2019 19:34
Operator : JC/SP
Sample : K1838-04
Misc : 5.71g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1J2

Manual Integrations
APPROVED

MMDadoda
3/11/2019 10:54:43 AM

Quant Time: Mar 11 02:26:27 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031119WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 11 02:20:19 2019
Response via : Initial Calibration

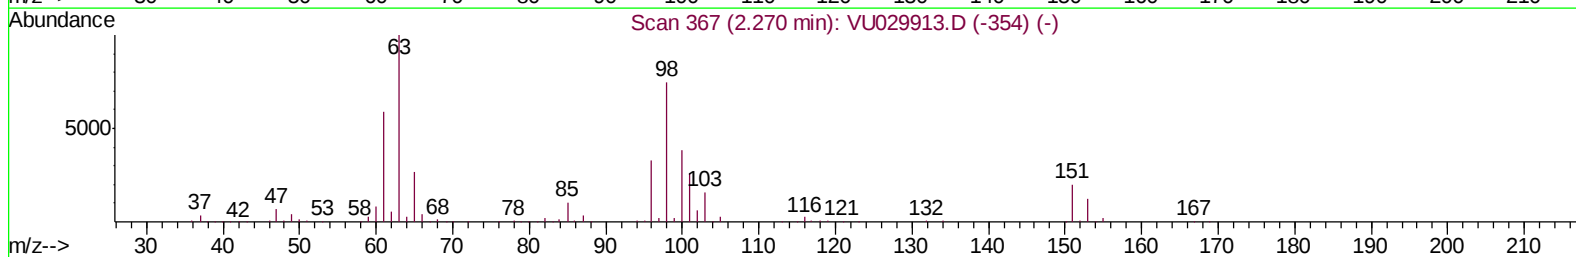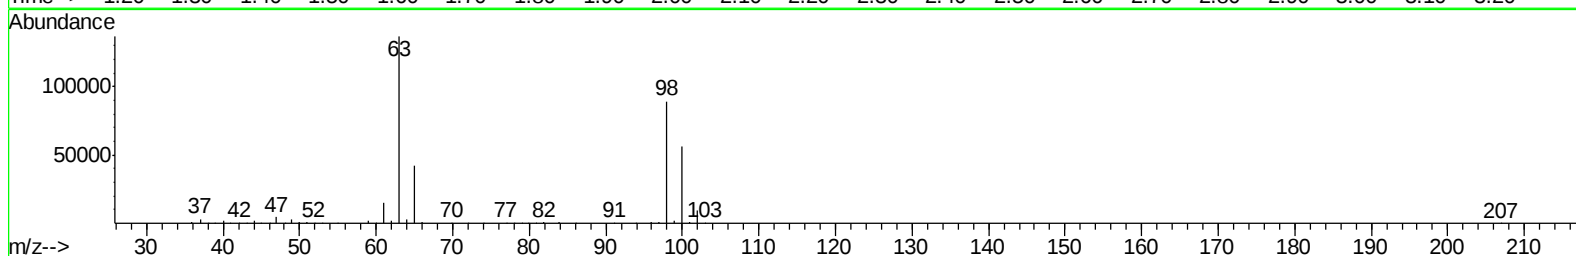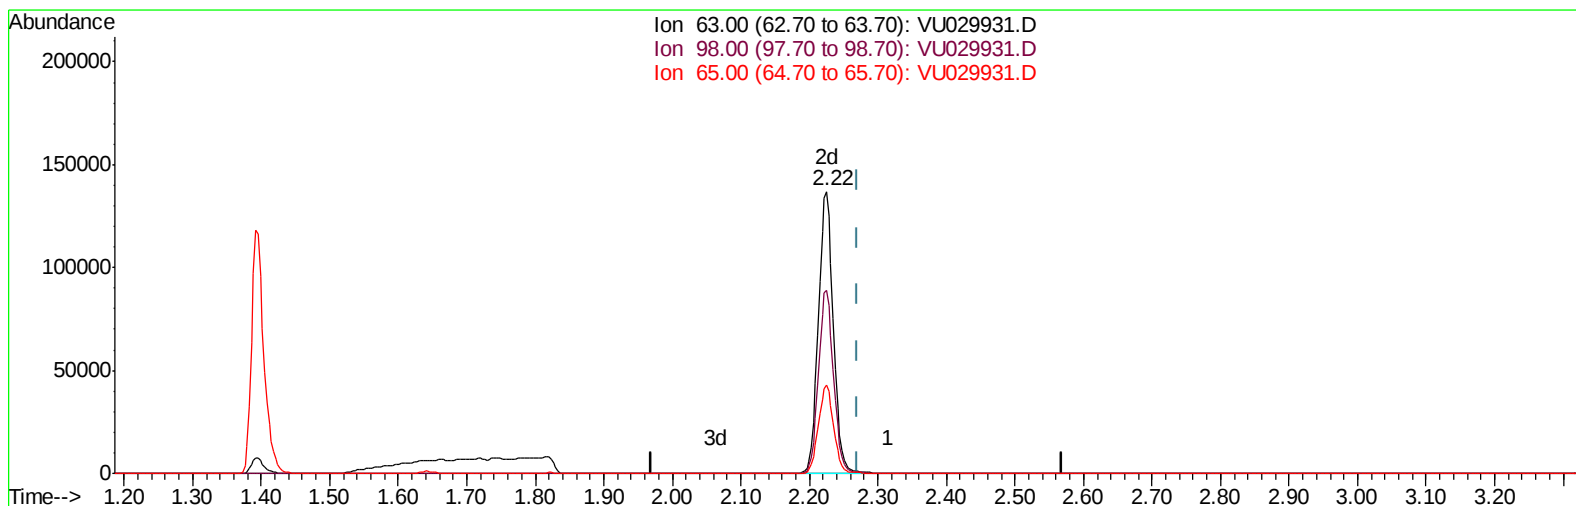

TIC: VU029931.D

(11) 1,1-Dichloroethene-d2 (S)

2.225min (-0.045) 31.30ug/L m

response 207324

Ion	Exp%	Act%
63.00	100	100
98.00	82.90	0.04#
65.00	23.60	0.05#
0.00	0.00	0.00

Data File : VU029931.D
Acq On : 09 Mar 2019 19:34
Operator : JC/SP
Sample : K1838-04
Misc : 5.71g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1J2

Manual Integrations
APPROVED

MMDadoda
3/11/2019 10:54:43 AM

Quant Time: Mar 11 04:11:20 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031119WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 11 02:20:19 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	575946	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	569531	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	291325	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	146943	41.82	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	83.64%
7) Chloroethane-d5	1.64	69	58722m	19.88	ug/L	-0.04
Spiked Amount	50.000	Range	70 - 130	Recovery	=	39.76%#
11) 1,1-Dichloroethene-d2	2.22	63	207324m	31.30	ug/L	-0.05
Spiked Amount	50.000	Range	60 - 125	Recovery	=	62.60%
21) 2-Butanone-d5	4.20	46	228172	83.81	ug/L	0.03
Spiked Amount	100.000	Range	40 - 130	Recovery	=	83.81%
24) Chloroform-d	4.64	84	268361	39.24	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	78.48%
26) 1,2-Dichloroethane-d4	5.30	65	166175	41.47	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	82.94%
32) Benzene-d6	5.33	84	597777	42.12	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	84.24%
36) 1,2-Dichloropropane-d6	6.32	67	179729	41.93	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	83.86%
41) Toluene-d8	7.56	98	551886	40.52	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	81.04%
43) trans-1,3-Dichloropropene-	7.85	79	82160	39.60	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	79.20%
47) 2-Hexanone-d5	8.33	63	204438	88.63	ug/L	0.02
Spiked Amount	100.000	Range	45 - 130	Recovery	=	88.63%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	292154	43.16	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	86.32%
64) 1,2-Dichlorobenzene-d4	11.86	152	238913	41.81	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	83.62%

Target Compounds					Qvalue
3) Chloromethane	1.32	50	66811	11.492 ug/L	99
6) Bromomethane	1.60	94	3482	2.916 ug/L	89
46) Tetrachloroethene	8.22	164	3874	1.097 ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VU029931.D
Acq On : 09 Mar 2019 19:34
Operator : JC/SP
Sample : K1838-04
Misc : 5.71g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1J2

Manual Integrations
APPROVED

MMDadoda
3/11/2019 10:54:43 AM

Quant Time: Mar 11 04:11:20 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031119WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 11 02:20:19 2019
Response via : Initial Calibration

