




Data File : VU029936.D
Acq On : 09 Mar 2019 21:31
Operator : JC/SP
Sample : K1818-09
Misc : 5.54g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 56 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF0Q9

Manual Integrations
APPROVED

MMDadoda
3/11/2019 11:13:05 AM

Quant Time: Mar 11 02:27:04 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031119WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 11 02:20:19 2019
Response via : Initial Calibration

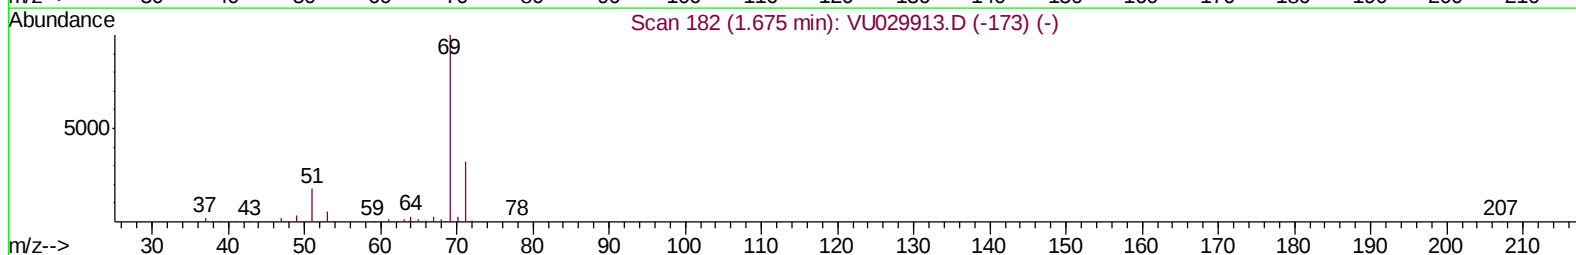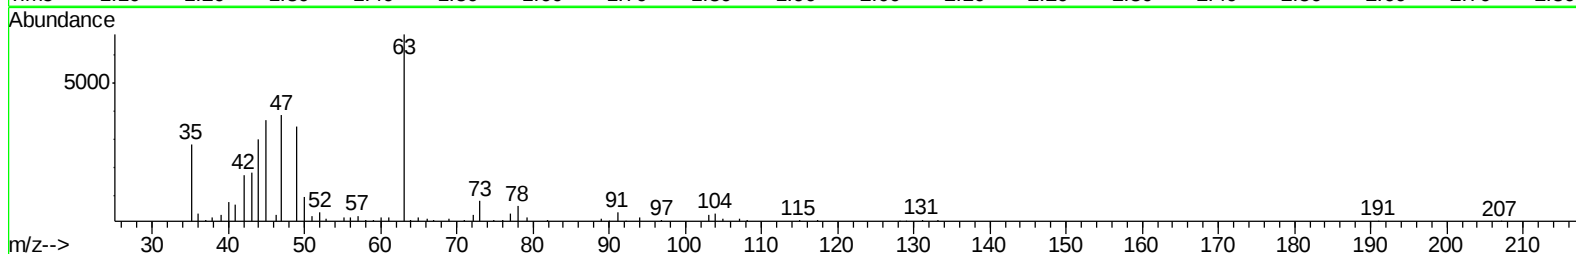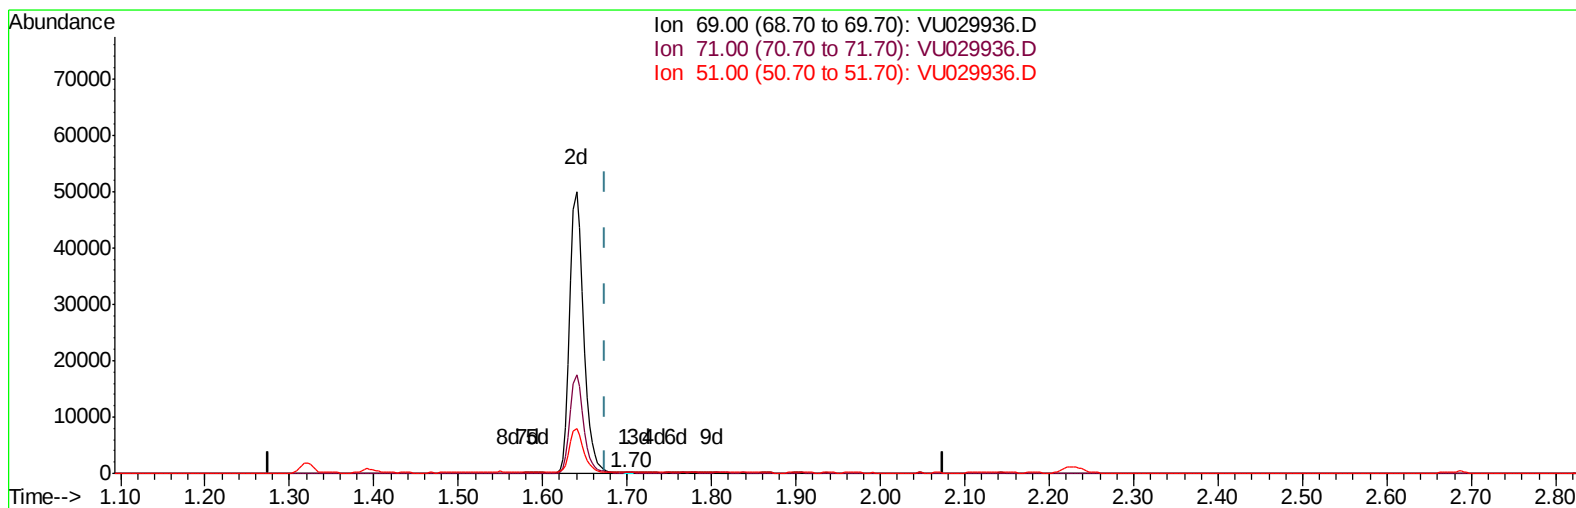

TIC: VU029936.D

(7) Chloroethane-d5 (S)

1.698min (+0.022) 0.03ug/L

response 90

Ion	Exp%	Act%
69.00	100	100
71.00	31.90	194.44#
51.00	24.10	40.00#
0.00	0.00	0.00




Data File : VU029936.D
Acq On : 09 Mar 2019 21:31
Operator : JC/SP
Sample : K1818-09
Misc : 5.54g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 56 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF0Q9

Manual Integrations
APPROVED

MMDadoda
3/11/2019 11:13:05 AM

Quant Time: Mar 11 02:27:04 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031119WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 11 02:20:19 2019
Response via : Initial Calibration

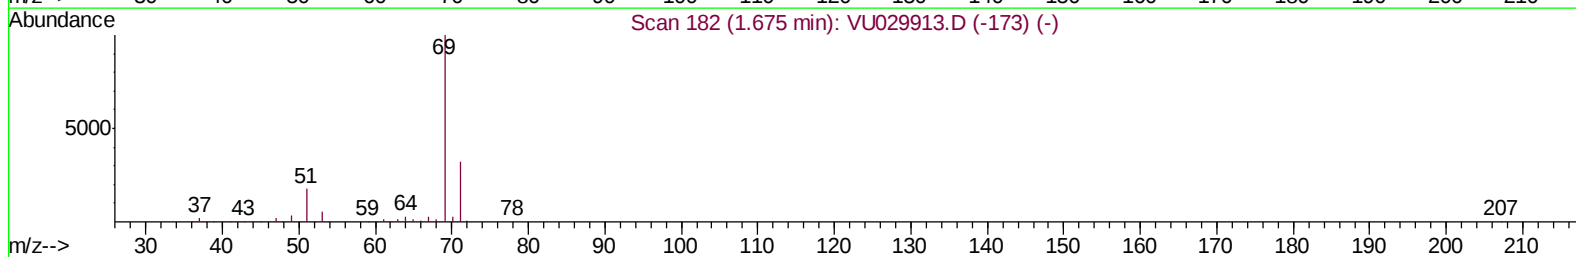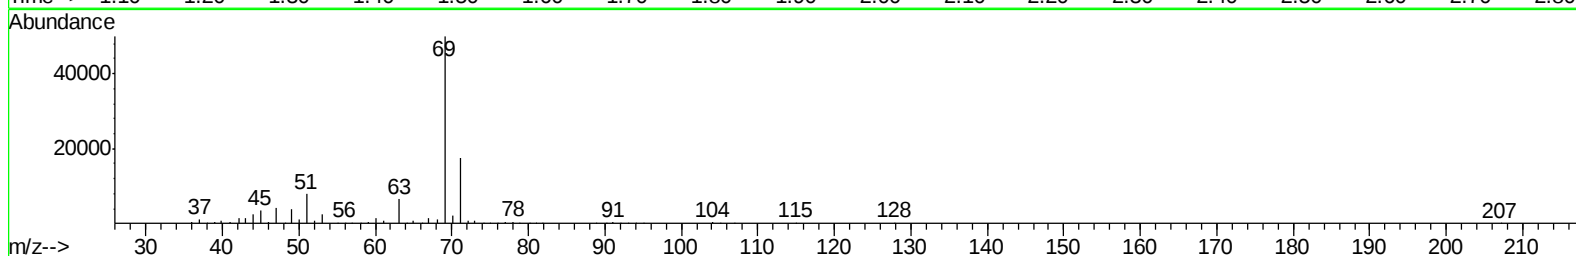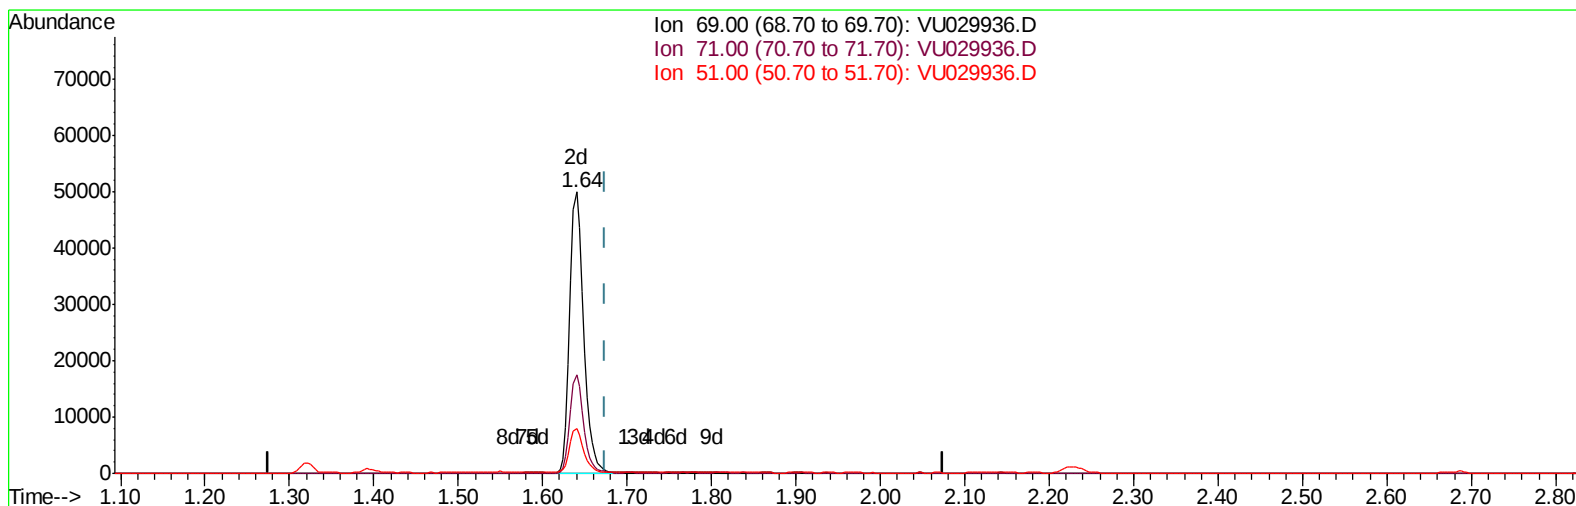

TIC: VU029936.D

(7) Chloroethane-d5 (S)

1.640min (-0.035) 19.65ug/L m

response 56868

Ion	Exp%	Act%
69.00	100	100
71.00	31.90	0.31#
51.00	24.10	0.06#
0.00	0.00	0.00

Data File : VU029936.D
Acq On : 09 Mar 2019 21:31
Operator : JC/SP
Sample : K1818-09
Misc : 5.54g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 56 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF0Q9

Manual Integrations
APPROVED

MMDadoda
3/11/2019 11:13:05 AM

Quant Time: Mar 11 04:24:31 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031119WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 11 02:20:19 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	564155	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	557903	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	277215	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	142454	41.39	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	82.78%
7) Chloroethane-d5	1.64	69	56868m	19.65	ug/L	-0.04
Spiked Amount	50.000	Range	70 - 130	Recovery	=	39.30%#
11) 1,1-Dichloroethene-d2	2.23	63	198851	30.65	ug/L	-0.04
Spiked Amount	50.000	Range	60 - 125	Recovery	=	61.30%
21) 2-Butanone-d5	4.20	46	230040	86.26	ug/L	0.03
Spiked Amount	100.000	Range	40 - 130	Recovery	=	86.26%
24) Chloroform-d	4.64	84	266279	39.75	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	79.50%
26) 1,2-Dichloroethane-d4	5.30	65	166779	42.49	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	84.98%
32) Benzene-d6	5.33	84	584369	42.03	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	84.06%
36) 1,2-Dichloropropane-d6	6.32	67	178259	42.45	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	84.90%
41) Toluene-d8	7.56	98	540566	40.52	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	81.04%
43) trans-1,3-Dichloropropene-	7.85	79	79893	39.31	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	78.62%
47) 2-Hexanone-d5	8.32	63	211720	93.71	ug/L	0.02
Spiked Amount	100.000	Range	45 - 130	Recovery	=	93.71%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	295528	44.57	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	89.14%
64) 1,2-Dichlorobenzene-d4	11.86	152	231317	42.54	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	85.08%

Target Compounds					Qvalue
3) Chloromethane	1.32	50	62765	11.022 ug/L	99
6) Bromomethane	1.60	94	3175	2.715 ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VU029936.D
Acq On : 09 Mar 2019 21:31
Operator : JC/SP
Sample : K1818-09
Misc : 5.54g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 56 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF0Q9

Manual Integrations
APPROVED

MMDadoda
3/11/2019 11:13:05 AM

Quant Time: Mar 11 04:24:31 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031119WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 11 02:20:19 2019
Response via : Initial Calibration

