


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU031119\
 Data File : VU029882.D
 Acq On : 08 Mar 2019 12:54
 Operator : JC/SP
 Sample : BFB58
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB58

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM021519WMA.M
 Title : VOC Analysis
 Last Update : Fri Mar 08 22:13:16 2019

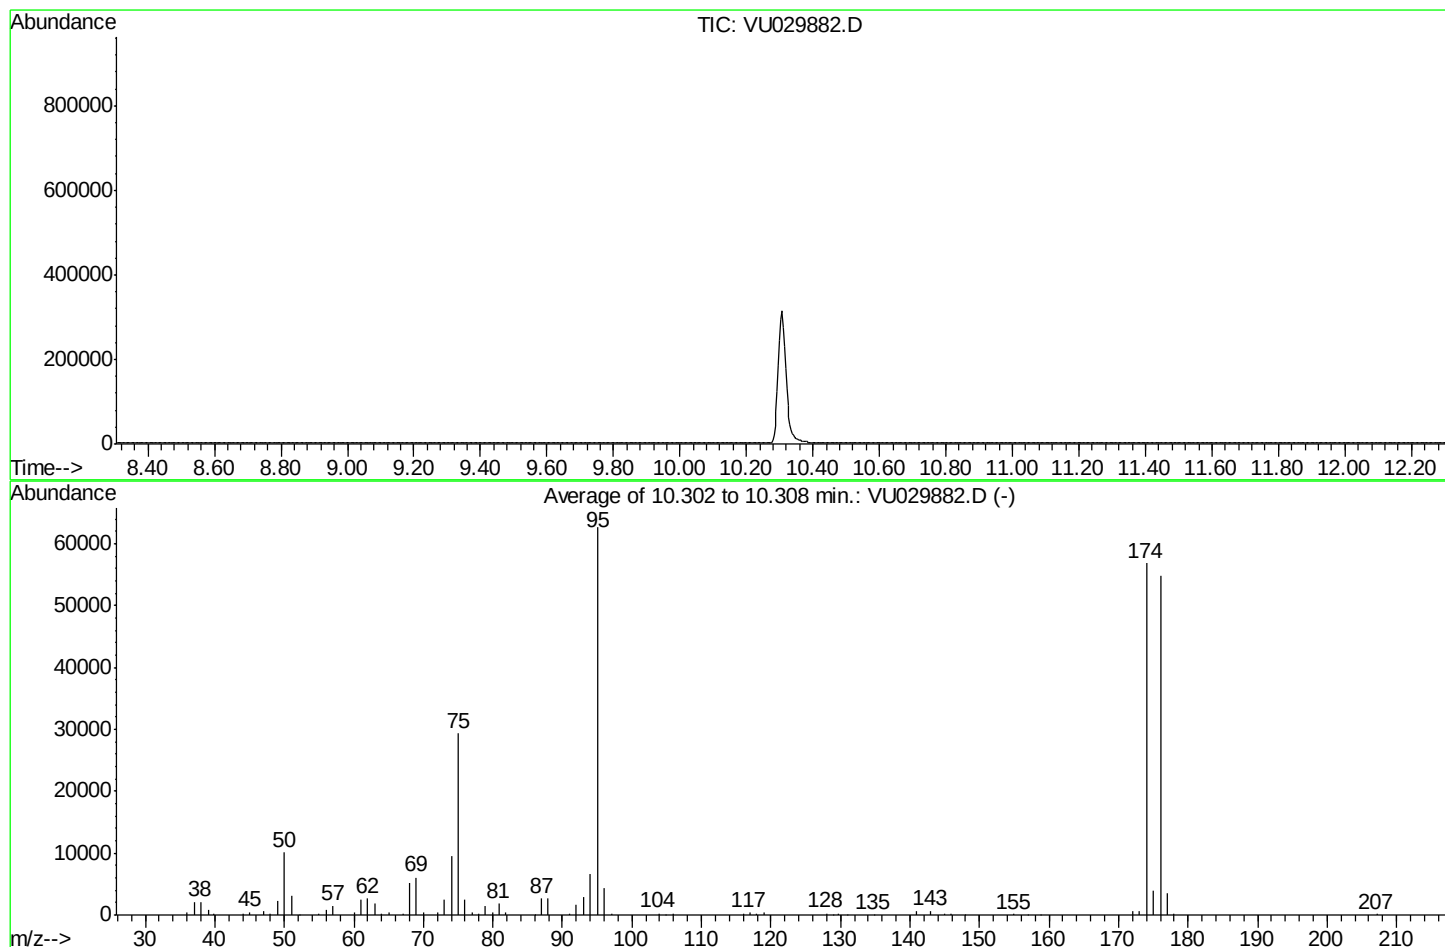

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2854

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	10134	PASS
75	95	30	80	46.8	29352	PASS
95	95	100	100	100.0	62653	PASS
96	95	5	9	6.8	4265	PASS
173	174	0.00	2	1.0	596	PASS
174	95	50	120	90.8	56858	PASS
175	174	5	9	7.1	4041	PASS
176	174	95	101	96.5	54861	PASS
177	176	5	9	6.3	3459	PASS

m/z	Abundance
39.90	1657.0
44.00	493.0

Instrument :
MSVOA_U
ClientSampleId :
BFB58

m/z	Abundance
35.90	464.0
37.00	2020.0
38.00	2031.0
39.10	823.0
39.90	2051.0
44.00	573.0
45.00	413.0
47.00	645.0
47.90	291.0
49.00	2095.0
50.00	10127.0
51.00	3066.0
55.00	177.0
56.00	943.0
57.00	1415.0
60.00	415.0
61.00	2348.0
62.00	2708.0
63.00	1779.0
63.90	234.0
65.10	361.0
67.00	137.0
68.00	4949.0
69.00	5863.0
70.00	452.0
72.10	243.0
73.00	2374.0
74.00	9296.0
75.00	28488.0
76.00	2415.0
77.00	347.0
78.00	289.0
78.90	1487.0
80.00	407.0
80.90	1738.0
81.80	368.0
87.00	2628.0
88.00	2624.0
91.10	170.0
92.00	1429.0
93.00	2812.0
94.00	6438.0
95.10	60560.0
96.00	4178.0
97.00	132.0
103.90	291.0
104.90	133.0
106.00	252.0
116.00	243.0
116.90	390.0
117.90	292.0
118.90	268.0
127.90	267.0
129.80	203.0
140.90	595.0
143.00	568.0
145.00	143.0
145.80	130.0
155.00	130.0
172.00	649.0
173.00	571.0
174.00	53784.0
175.00	3903.0
176.00	51600.0
177.00	3287.0
177.90	121.0
207.10	122.0

Instrument :
MSVOA_U
ClientSampleId :
BFB58

m/z	Abundance
35.90	457.0
37.00	2125.0
38.00	2206.0
39.10	941.0
39.90	1917.0
44.00	635.0
45.00	449.0
47.00	672.0
47.90	270.0
49.10	2280.0
50.00	10400.0
51.00	3148.0
54.90	161.0
56.10	926.0
57.00	1567.0
60.00	415.0
61.00	2474.0
62.00	2841.0
63.00	1837.0
63.90	331.0
65.10	416.0
67.00	163.0
68.00	5301.0
69.00	6234.0
70.00	501.0
72.00	358.0
73.10	2561.0
74.00	9855.0
75.00	30328.0
76.00	2468.0
77.00	474.0
78.00	342.0
78.90	1590.0
79.90	404.0
80.90	1887.0
81.70	392.0
86.00	110.0
87.00	2779.0
87.90	2725.0
91.00	250.0
92.00	1604.0
93.00	2940.0
94.10	6770.0
95.10	64736.0
96.10	4429.0
97.00	150.0
103.80	304.0
104.90	100.0
106.00	283.0
116.00	243.0
116.90	409.0
117.90	244.0
119.00	332.0
128.00	299.0
128.90	123.0
129.80	213.0
131.00	111.0
134.80	123.0
141.00	643.0
143.00	663.0
144.90	151.0
145.80	132.0
155.00	145.0
157.00	119.0
172.00	619.0
173.00	612.0
174.00	58760.0
175.00	4159.0
176.00	56472.0
177.00	3510.0
177.90	149.0
207.20	138.0

Instrument :
MSVOA_U
ClientSampleId :
BFB58

m/z	Abundance
35.90	448.0
37.00	2120.0
38.00	2097.0
39.00	964.0
39.90	1809.0
44.00	657.0
45.00	404.0
47.00	555.0
47.90	296.0
49.10	2354.0
50.10	9875.0
51.00	3047.0
52.10	104.0
54.90	120.0
56.10	751.0
57.00	1491.0
60.00	416.0
61.00	2390.0
62.00	2461.0
63.00	1850.0
63.90	355.0
65.00	427.0
67.00	163.0
68.00	5237.0
69.00	6142.0
70.00	493.0
72.00	414.0
73.10	2590.0
74.00	9490.0
75.10	29240.0
76.00	2328.0
77.10	494.0
78.00	311.0
78.90	1565.0
79.90	395.0
80.90	1722.0
81.70	380.0
86.00	102.0
87.00	2592.0
87.90	2610.0
91.00	307.0
92.00	1667.0
93.00	2691.0
94.10	6525.0
95.10	62664.0
96.10	4189.0
97.10	131.0
103.80	265.0
105.90	251.0
116.00	222.0
116.90	402.0
117.90	171.0
119.00	361.0
127.90	270.0
129.00	102.0
129.70	216.0
131.10	181.0
134.80	140.0
140.90	595.0
143.00	764.0
144.90	137.0
145.90	107.0
147.90	106.0
155.00	144.0
157.00	126.0
158.80	116.0
172.00	564.0
173.00	607.0
174.00	58032.0
175.00	4061.0
176.00	56512.0
177.00	3580.0
178.00	167.0
207.20	112.0

Instrument :
MSVOA_U
ClientSampleId :
BFB58