


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU031119\
 Data File : VU029909.D
 Acq On : 09 Mar 2019 10:18
 Operator : JC/SP
 Sample : BFB59
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB59

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031119WMA.M
 Title : VOC Analysis
 Last Update : Mon Mar 11 12:44:43 2019

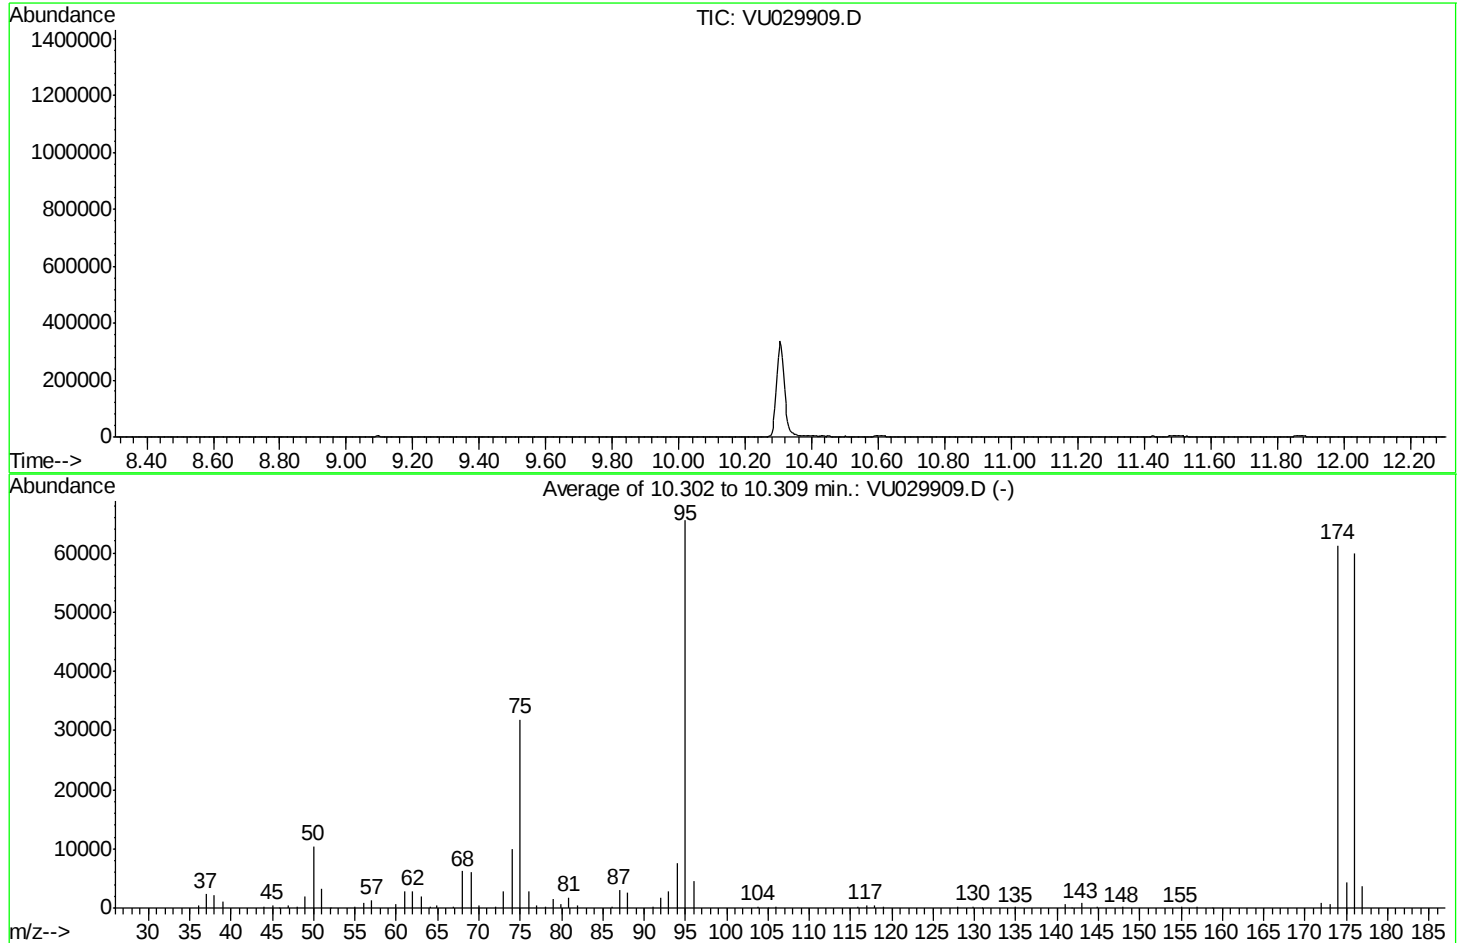

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2854

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	10445	PASS
75	95	30	80	48.6	31808	PASS
95	95	100	100	100.0	65490	PASS
96	95	5	9	7.0	4613	PASS
173	174	0.00	2	1.1	665	PASS
174	95	50	120	93.6	61266	PASS
175	174	5	9	7.0	4277	PASS
176	174	95	101	98.0	60013	PASS
177	176	5	9	6.3	3779	PASS

Scan 2854 (10.267 min): VU029909.D
BFB59

m/z	Abundance
36.00	496.0
37.90	137.0
39.90	1042.0
43.90	381.0

Instrument :
MSVOA_U
ClientSampleId :
BFB59

m/z	Abundance
36.00	911.0
37.00	2364.0
38.00	2347.0
39.00	1168.0
40.00	912.0
43.90	666.0
45.10	478.0
47.00	562.0
47.90	273.0
49.00	2065.0
50.00	10383.0
51.00	3348.0
52.10	145.0
54.90	284.0
56.00	963.0
57.00	1385.0
60.00	553.0
61.00	2673.0
62.00	3219.0
63.00	1960.0
64.00	294.0
65.00	302.0
66.90	140.0
68.00	6183.0
69.00	5990.0
70.00	520.0
72.00	313.0
73.00	2876.0
74.00	10010.0
75.00	31016.0
76.00	2603.0
77.10	508.0
78.10	205.0
78.90	1553.0
79.90	526.0
80.90	1781.0
81.90	371.0
86.10	163.0
87.00	3145.0
88.00	2777.0
91.00	271.0
92.00	1647.0
93.00	2660.0
94.00	7515.0
95.00	64816.0
96.10	4623.0
103.80	296.0
105.00	127.0
105.90	275.0
115.80	249.0
116.90	479.0
117.90	387.0
118.90	298.0
127.90	237.0
129.80	250.0
131.00	101.0
135.00	126.0
141.00	546.0
141.70	144.0
142.90	733.0
144.80	172.0
147.90	134.0
155.10	154.0
157.00	129.0
158.90	106.0
172.00	681.0
173.00	709.0
174.00	59336.0
175.00	4244.0
176.00	57592.0
177.00	3817.0

Instrument :
MSVOA_U
ClientSampleId :
BFB59

m/z	Abundance
36.00	913.0
37.00	2540.0
38.00	2306.0
39.00	1161.0
40.00	962.0
43.90	670.0
45.00	473.0
45.80	122.0
47.00	506.0
47.90	253.0
49.00	2082.0
50.00	10718.0
51.00	3270.0
52.00	101.0
54.90	297.0
56.00	952.0
57.00	1372.0
60.00	604.0
61.00	2871.0
62.00	3023.0
63.00	2022.0
64.00	253.0
64.90	373.0
67.00	166.0
68.00	6426.0
69.00	6226.0
70.00	492.0
72.00	284.0
73.00	2868.0
74.00	10261.0
75.00	32792.0
76.00	2825.0
77.10	414.0
78.00	162.0
79.00	1579.0
79.90	604.0
80.90	1769.0
81.90	432.0
86.10	155.0
87.00	3214.0
88.00	2751.0
91.00	293.0
92.10	1703.0
93.00	2897.0
94.00	7738.0
95.00	67560.0
96.10	4790.0
103.80	328.0
105.00	103.0
106.00	284.0
115.80	215.0
116.90	504.0
117.90	396.0
118.90	260.0
127.90	204.0
129.90	311.0
130.90	110.0
135.00	170.0
141.00	639.0
141.70	125.0
142.90	847.0
144.80	183.0
147.90	150.0
155.00	170.0
156.90	147.0
158.80	113.0
172.00	777.0
173.00	674.0
174.00	63040.0
175.00	4371.0
176.00	62024.0
177.00	3903.0

Instrument :
MSVOA_U
ClientSampleId :
BFB59

m/z	Abundance
36.00	810.0
37.00	2411.0
38.00	2110.0
39.00	1007.0
39.90	1079.0
43.90	678.0
45.00	433.0
45.80	104.0
46.80	542.0
48.00	243.0
49.00	1901.0
50.00	10235.0
51.00	2913.0
54.90	245.0
56.00	834.0
57.00	1241.0
60.00	552.0
61.00	2602.0
62.00	2504.0
63.00	1936.0
64.10	242.0
65.00	450.0
67.00	164.0
68.00	5915.0
69.00	5997.0
70.00	446.0
72.00	269.0
73.00	2599.0
74.00	9454.0
75.00	31616.0
76.00	2816.0
77.00	314.0
77.90	167.0
79.00	1520.0
79.90	657.0
80.90	1680.0
81.90	416.0
86.10	121.0
87.00	3029.0
88.00	2408.0
91.00	279.0
92.00	1740.0
93.00	2806.0
94.00	7160.0
95.00	64096.0
96.10	4428.0
103.80	276.0
105.90	214.0
115.80	206.0
116.90	464.0
117.90	316.0
118.90	229.0
128.00	160.0
129.90	312.0
135.00	162.0
141.00	716.0
143.00	861.0
144.90	172.0
147.90	152.0
155.00	149.0
156.80	143.0
172.00	852.0
173.00	613.0
174.00	61424.0
175.00	4217.0
176.00	60424.0
177.00	3617.0

Instrument :
MSVOA_U
ClientSampleId :
BFB59