

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031120\
 Data File : VU037176.D
 Acq On : 11 Mar 2020 19:10
 Operator : JC/MD
 Sample : L1883-14
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0NA4

Quant Time: Mar 12 04:03:56 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR031120WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Mar 12 01:55:55 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	111590	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	112686	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	43381	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	36853	5.03	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	100.60%
7) Chloroethane-d5	1.93	69	29281	5.66	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	113.20%
11) 1,1-Dichloroethene-d2	2.59	63	55052	3.65	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.00%
20) 2-Butanone-d5	4.68	46	99149	52.90	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	105.80%
24) Chloroform-d	5.10	84	76019	5.07	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.40%
26) 1,2-Dichloroethane-d4	5.74	65	44834	5.15	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.00%
32) Benzene-d6	5.76	84	138228	4.99	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.80%
36) 1,2-Dichloropropane-d6	6.73	67	44282	4.94	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.80%
41) Toluene-d8	7.93	98	122149	4.70	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.00%
43) trans-1,3-Dichloropropene-	8.20	79	17039	4.71	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.20%
46) 2-Hexanone-d5	8.66	63	73792	49.01	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	98.02%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	36453	4.95	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.00%
64) 1,2-Dichlorobenzene-d4	12.21	152	40766	5.44	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	108.80%


Target Compounds					Ovalue
13) Acetone	2.67	43	3736	2.432 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU031120\
Data File : VU037176.D
Acq On : 11 Mar 2020 19:10
Operator : JC/MD
Sample : L1883-14
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0NA4

Quant Time: Mar 12 04:03:56 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR031120WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Mar 12 01:55:55 2020
Response via : Initial Calibration

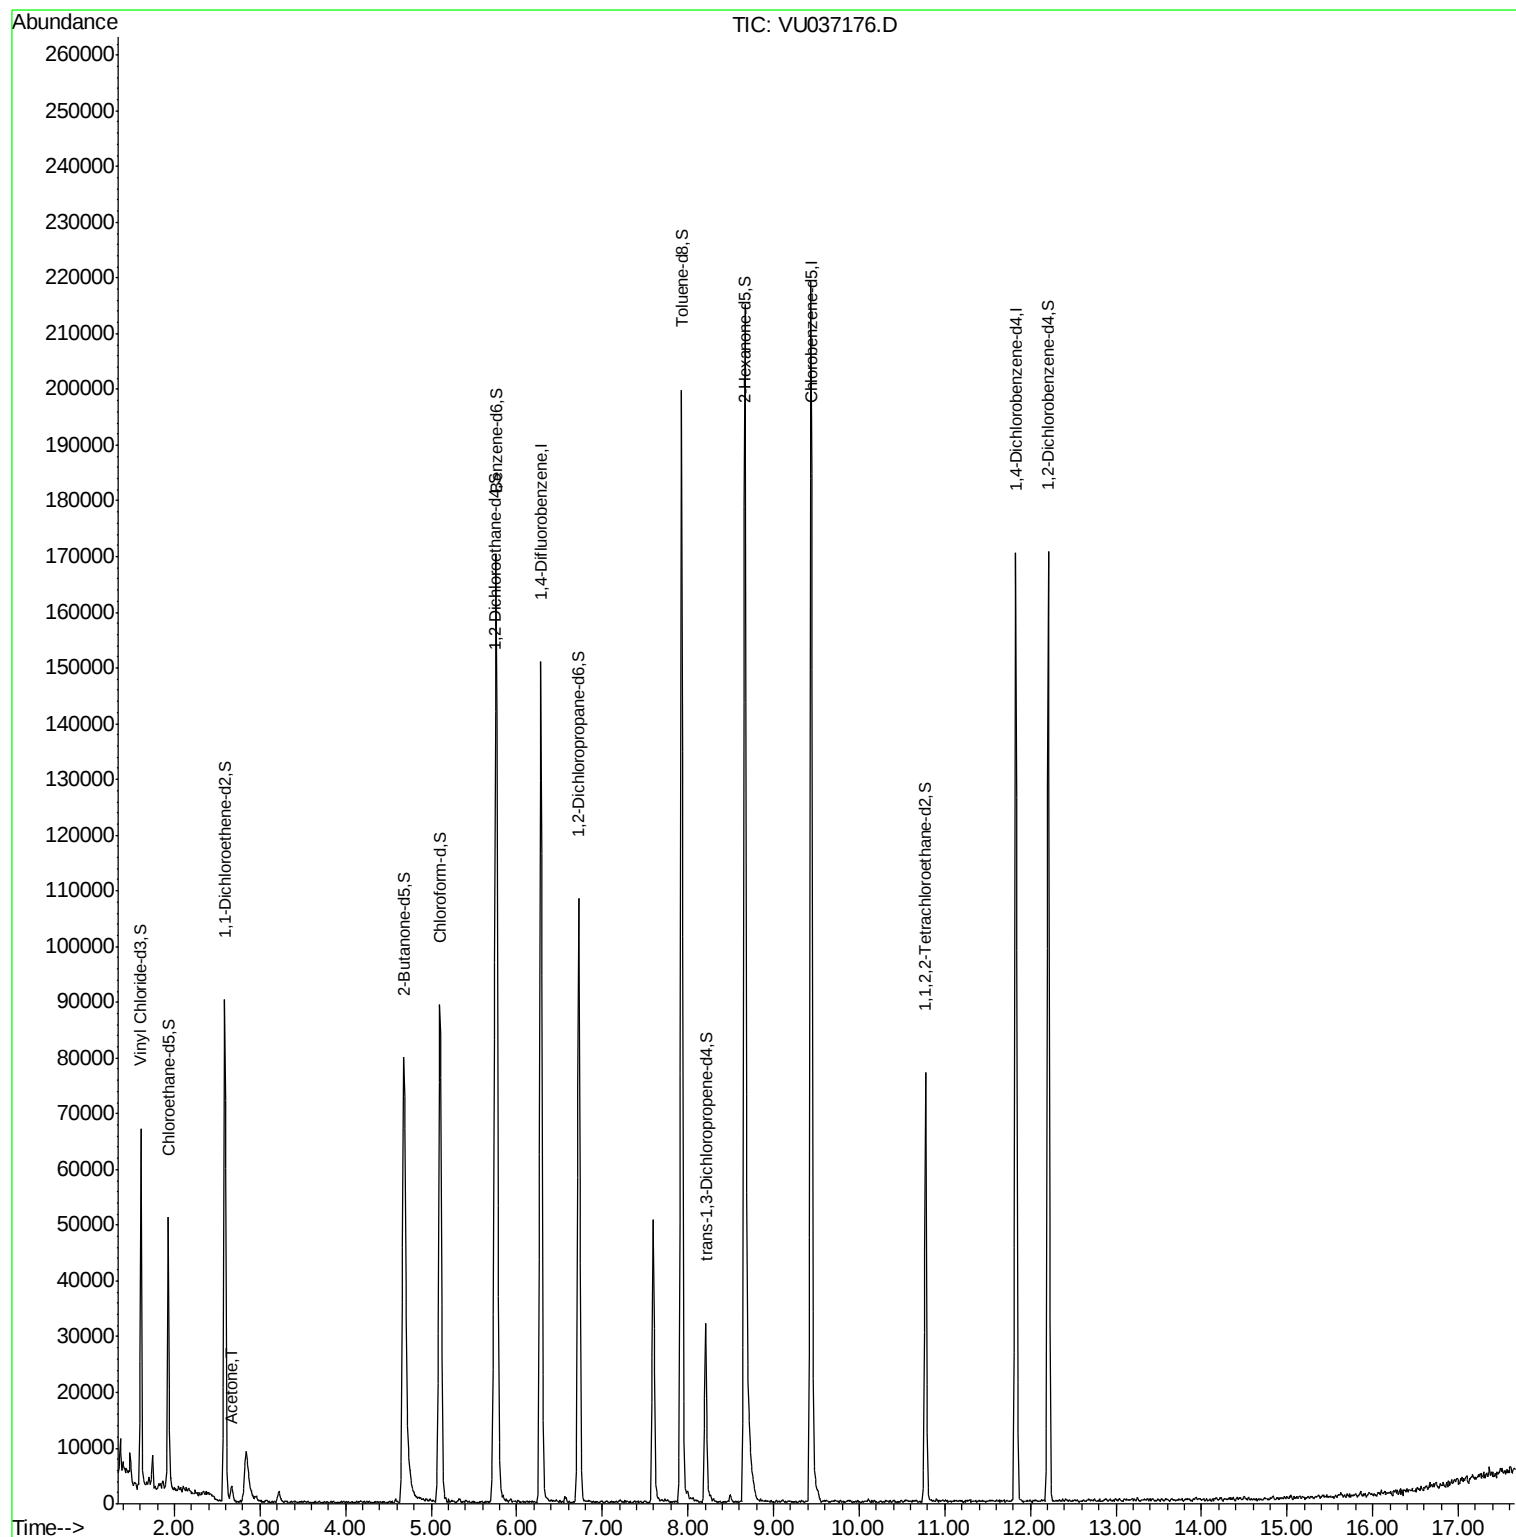

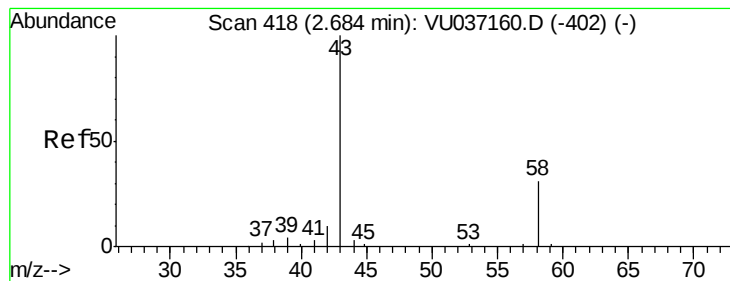

#13
 Acetone
 Concen: 2.432 ug/L
 RT: 2.67 min Scan# 413
 Delta R.T. -0.02 min
 Lab File: VU037176.D
 Acq: 11 Mar 2020 19:10

Instrument :
 MSVOA_U
 ClientSampleId :
 C0NA4

Tot Ion: 43 Resp: 3736
 Ion Ratio Lower Upper
 43 100
 58 25.8 0.0 52.2

