

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031120\
 Data File : VU037177.D
 Acq On : 11 Mar 2020 19:35
 Operator : JC/MD
 Sample : L1891-01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBEQ9

Quant Time: Mar 12 04:08:14 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR031120WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Mar 12 01:55:55 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.29	114	114754	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	116082	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	40621	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	39460	5.24	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	104.80%
7) Chloroethane-d5	1.93	69	31840	5.98	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	119.60%
11) 1,1-Dichloroethene-d2	2.59	63	56807	3.66	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.20%
20) 2-Butanone-d5	4.67	46	98703	51.21	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.42%
24) Chloroform-d	5.10	84	77706	5.04	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.80%
26) 1,2-Dichloroethane-d4	5.74	65	46175	5.16	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.20%
32) Benzene-d6	5.76	84	142456	4.99	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.80%
36) 1,2-Dichloropropane-d6	6.72	67	45924	4.98	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.60%
41) Toluene-d8	7.93	98	126153	4.72	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.40%
43) trans-1,3-Dichloropropene-	8.21	79	17727	4.76	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	95.20%
46) 2-Hexanone-d5	8.66	63	76650	49.42	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	98.84%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	36328	4.79	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.80%
64) 1,2-Dichlorobenzene-d4	12.21	152	40355	5.75	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	115.00%

Target Compounds


					Ovalue
13) Acetone	2.66	43	6636	4.201 ug/L	96
16) Methylene chloride	3.08	84	1912	0.213 ug/L	85
25) Chloroform	5.13	83	9104	0.521 ug/L	92
38) Bromodichloromethane	7.13	83	2269	0.189 ug/L #	76
47) Tetrachloroethene	8.57	164	1091	0.151 ug/L	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031120\
Data File : VU037177.D
Acq On : 11 Mar 2020 19:35
Operator : JC/MD
Sample : L1891-01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBEQ9

Quant Time: Mar 12 04:08:14 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR031120WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Mar 12 01:55:55 2020
Response via : Initial Calibration

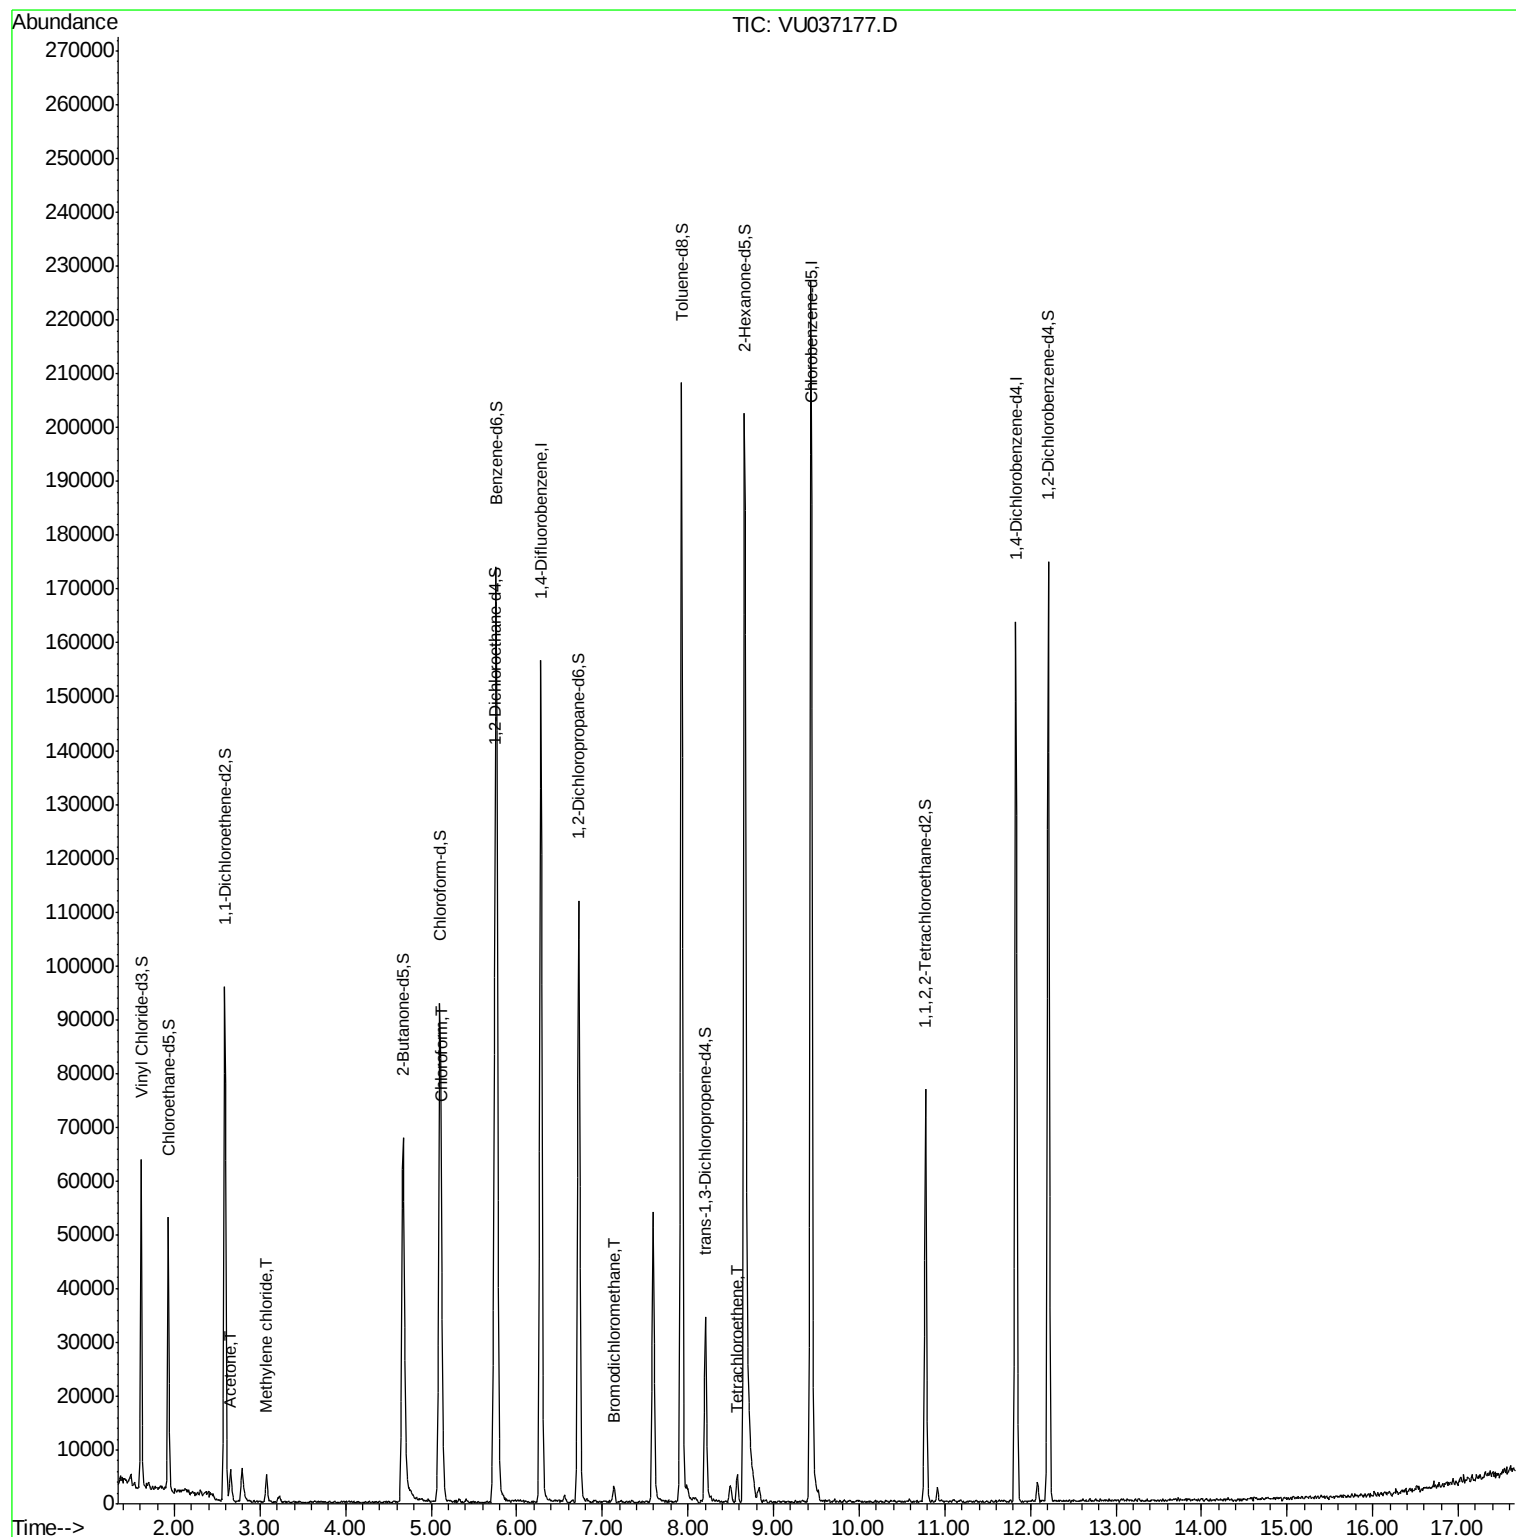

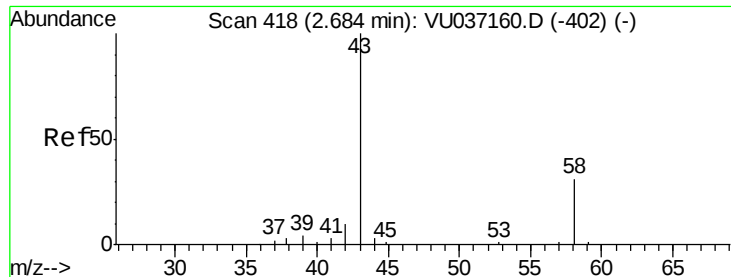

#13

Acetone

Concen: 4.201 ug/L

RT: 2.66 min Scan# 410

Delta R.T. -0.03 min

Lab File: VU037177.D

Acq: 11 Mar 2020 19:35

Instrument :

MSVOA_U

ClientSampleId :


DBEQ9

Tot Ion: 43 Resp: 6636

Ion Ratio Lower Upper




43 100

58 24.1 0.0 52.2

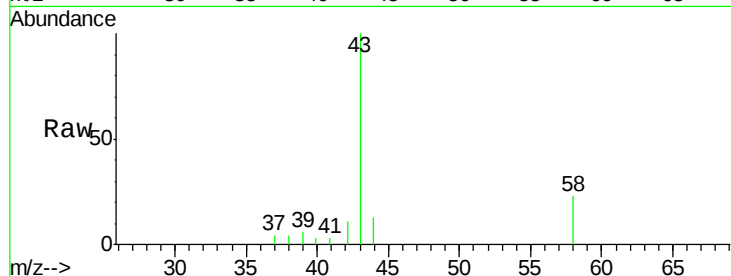

Abundance Ion 43.05 (42.75 to 43.75): VU037160.D (-402) (-)

Ion 58.05 (57.75 to 58.75): VU037160.D (-402) (-)

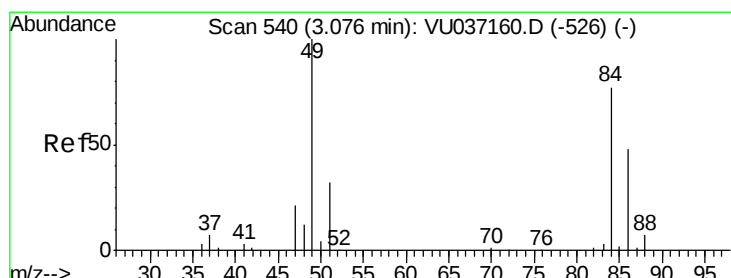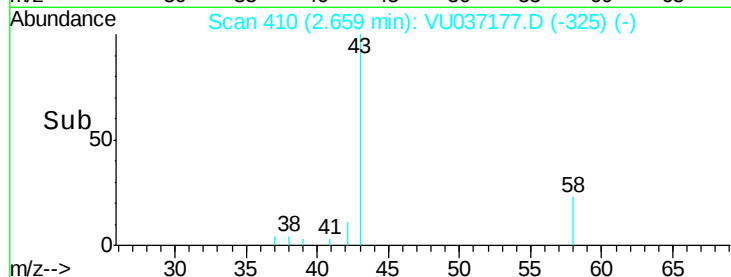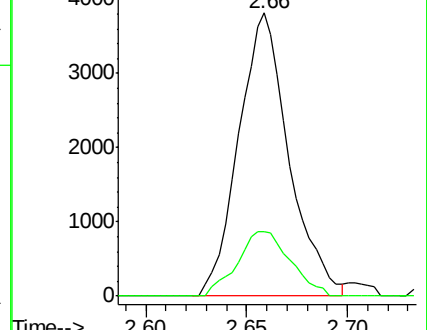

#16

Methylene chloride

Concen: 0.213 ug/L

RT: 3.08 min Scan# 540

Delta R.T. 0.00 min

Lab File: VU037177.D

Acq: 11 Mar 2020 19:35


Tgt Ion: 84 Resp: 1912

Ion Ratio Lower Upper

84 100

86 54.8 44.3 82.3



49 115.9 95.3 177.1

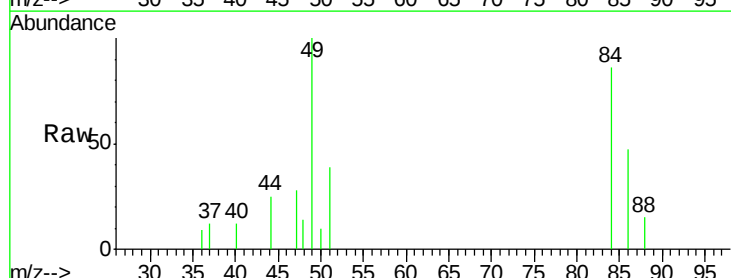


Abundance Ion 84.05 (83.75 to 84.75): VU037160.D (-526) (-)

Ion 86.00 (85.70 to 86.70): VU037160.D (-526) (-)

Ion 49.10 (48.80 to 49.80): VU037160.D (-526) (-)



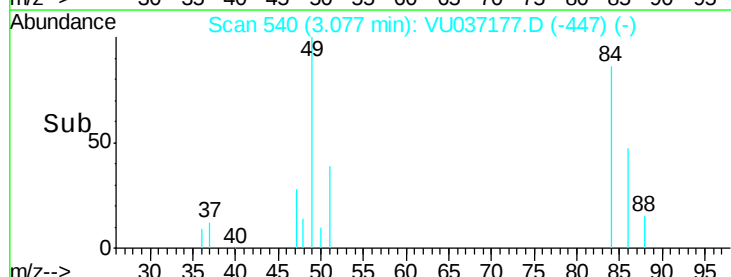
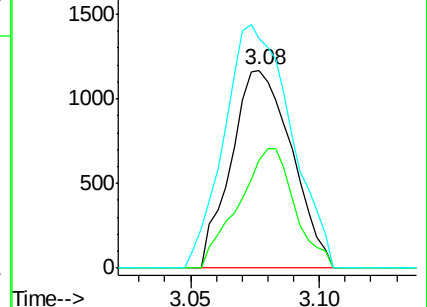


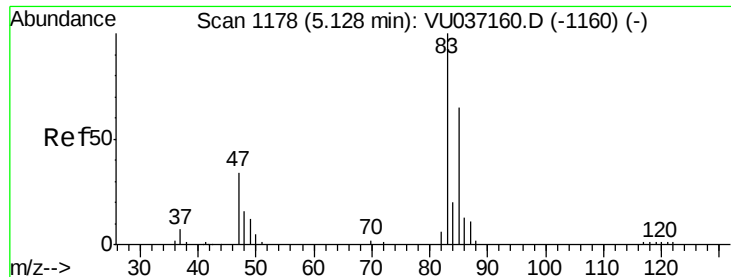

#25
Chloroform
Concen: 0.521 ug/L
RT: 5.13 min Scan# 1178
Delta R.T. 0.00 min
Lab File: VU037177.D
Acq: 11 Mar 2020 19:35




Instrument :
MSVOA_U
ClientSampleId :
DBEQ9


Tot Ion: 83 Resp: 9104
Ion Ratio Lower Upper
83 100
85 58.7 45.3 84.1

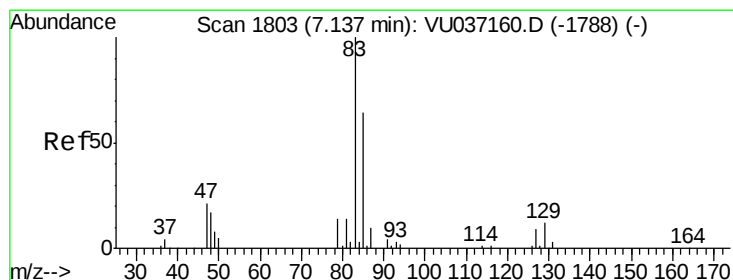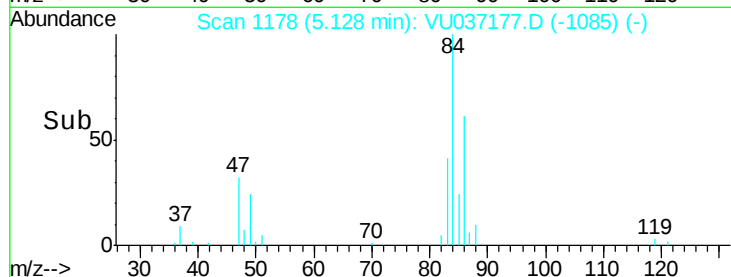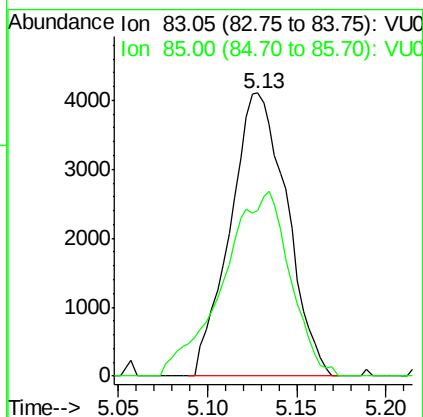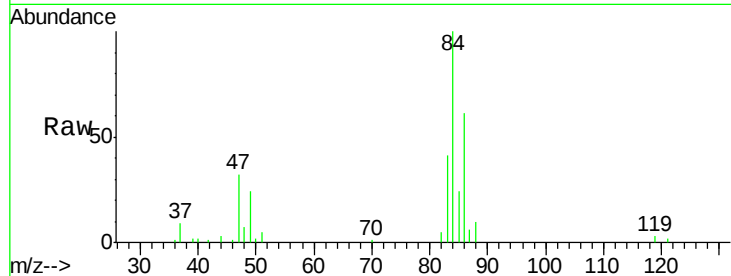

#38
Bromodichloromethane
Concen: 0.189 ug/L
RT: 7.13 min Scan# 1802
Delta R.T. -0.00 min
Lab File: VU037177.D
Acq: 11 Mar 2020 19:35

Tgt Ion: 83 Resp: 2269
Ion Ratio Lower Upper
83 100
85 45.2 45.1 83.7
127 0.0 6.7 10.1#

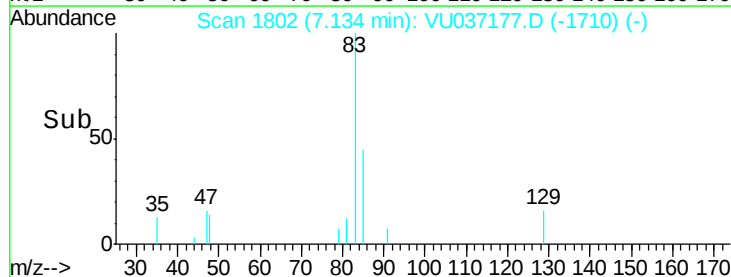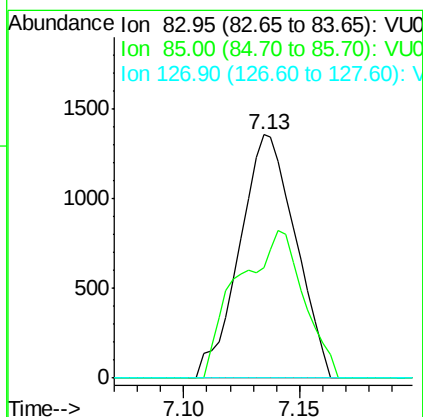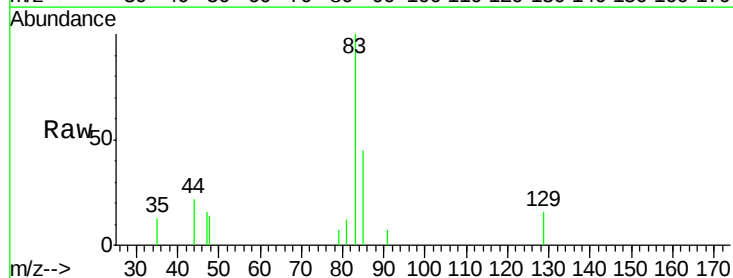

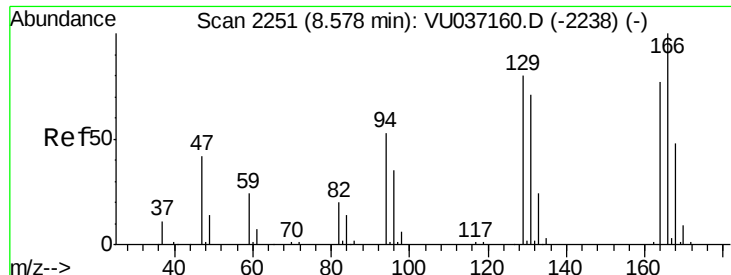

#47

Tetrachloroethene

Concen: 0.151 ug/L

RT: 8.57 min Scan# 2250

Delta R.T. -0.00 min

Lab File: VU037177.D


Acq: 11 Mar 2020 19:35

Instrument :

MSVOA_U

ClientSampleId :

DBEQ9

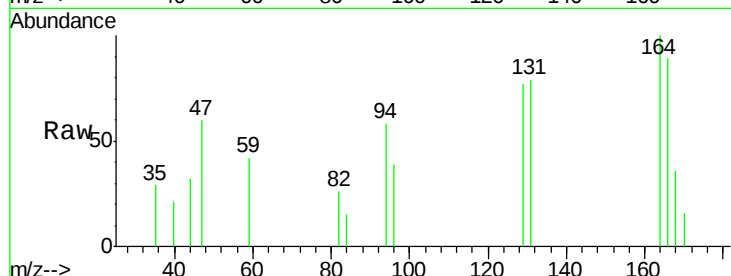

Tot Ion:164 Resp: 1091

Ion Ratio Lower Upper

164 100

129 76.7 69.8 129.6

131 79.1 66.1 122.8

166 89.1 88.1 163.5

Abundance Ion 163.90 (163.60 to 164.60): V

Ion 128.95 (128.65 to 129.65): V

Ion 130.95 (130.65 to 131.65): V

Ion 165.90 (165.60 to 166.60): V

